

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102021\
 Data File : VU045341.D
 Acq On : 20 Oct 2021 12:17
 Operator : SY/MD
 Sample : VU1020MBL04
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK028

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101921WMA.M

Title : VOC Analysis

Signal : TIC: VU045341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.462	32	38	51	rBV2	12445	23648	2.54%	0.287%
2	1.601	73	81	96	rBV	77896	85250	9.16%	1.034%
3	1.874	160	166	182	rVB	39096	51553	5.54%	0.626%
4	2.549	364	376	386	rBV	109976	180717	19.43%	2.193%
5	2.697	418	422	424	rBV2	173	163	0.02%	0.002%
6	2.774	439	446	454	rVB3	828	1302	0.14%	0.016%
7	2.957	494	503	515	rBV2	1822	3335	0.36%	0.040%
8	3.041	520	529	545	rVB2	3235	6107	0.66%	0.074%
9	3.109	545	550	552	rBV	218	221	0.02%	0.003%
10	3.189	561	575	587	rBV2	4943	10827	1.16%	0.131%
11	3.308	609	612	614	rBV	195	160	0.02%	0.002%
12	3.340	620	622	624	rBV	243	172	0.02%	0.002%
13	3.517	674	677	681	rBV	143	162	0.02%	0.002%
14	3.575	692	695	697	rBV	221	166	0.02%	0.002%
15	3.726	739	742	746	rVB2	195	184	0.02%	0.002%
16	3.781	752	759	762	rBV	227	305	0.03%	0.004%
17	3.951	807	812	818	rVV2	183	235	0.03%	0.003%
18	3.990	821	824	828	rVB2	198	161	0.02%	0.002%
19	4.047	837	842	845	rBV2	181	210	0.02%	0.003%
20	4.112	858	862	868	rVB2	241	264	0.03%	0.003%
21	4.398	944	951	955	rBV	237	361	0.04%	0.004%
22	4.472	972	974	979	rVB	197	156	0.02%	0.002%
23	4.501	979	983	987	rBV	151	190	0.02%	0.002%
24	4.633	1007	1024	1049	rBV	131995	336048	36.12%	4.077%
25	4.874	1095	1099	1105	rVB2	241	251	0.03%	0.003%
26	4.919	1110	1113	1116	rVB2	227	139	0.01%	0.002%
27	5.064	1142	1158	1186	rVB	169566	374844	40.29%	4.548%
28	5.166	1186	1190	1194	rVB2	166	181	0.02%	0.002%
29	5.208	1200	1203	1206	rVV2	306	212	0.02%	0.003%
30	5.337	1239	1243	1248	rBV2	332	427	0.05%	0.005%
31	5.372	1252	1254	1261	rVB2	235	171	0.02%	0.002%
32	5.443	1272	1276	1280	rBV2	175	222	0.02%	0.003%
33	5.723	1341	1363	1386	rBV2	304599	841106	90.41%	10.206%
34	5.877	1408	1411	1416	rVB2	324	302	0.03%	0.004%
35	5.977	1432	1442	1454	rVV5	1864	3729	0.40%	0.045%
36	6.038	1458	1461	1470	rVB3	287	393	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102021\
 Data File : VU045341.D
 Acq On : 20 Oct 2021 12:17
 Operator : SY/MD
 Sample : VU1020MBL04
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK028

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101921WMA.M
 Title : VOC Analysis

37	6.182	1502	1506	1511	rBV2	236	335	0.04%	0.004%
38	6.250	1511	1527	1550	rBV	370985	699429	75.18%	8.487%
39	6.372	1559	1565	1566	rBV2	162	169	0.02%	0.002%
40	6.533	1605	1615	1624	rVB4	4023	7159	0.77%	0.087%
41	6.594	1624	1634	1645	rBV3	1816	3632	0.39%	0.044%
42	6.694	1651	1665	1685	rBV	224763	434559	46.71%	5.273%
43	6.809	1696	1701	1703	rBV	336	312	0.03%	0.004%
44	7.051	1769	1776	1778	rBV2	366	374	0.04%	0.005%
45	7.179	1805	1816	1827	rBV5	2356	4480	0.48%	0.054%
46	7.224	1827	1830	1834	rVB3	703	549	0.06%	0.007%
47	7.369	1868	1875	1877	rBV2	187	217	0.02%	0.003%
48	7.446	1892	1899	1901	rBV2	178	229	0.02%	0.003%
49	7.481	1907	1910	1913	rBV	210	189	0.02%	0.002%
50	7.568	1923	1937	1953	rBV	125560	219067	23.55%	2.658%
51	7.681	1969	1972	1973	rBV2	432	236	0.03%	0.003%
52	7.803	2000	2010	2017	rVB4	1412	2110	0.23%	0.026%
53	7.899	2026	2040	2054	rBV	331788	562805	60.50%	6.829%
54	7.973	2057	2063	2079	rVB6	5090	10836	1.16%	0.131%
55	8.134	2107	2113	2116	rBV2	223	293	0.03%	0.004%
56	8.182	2116	2128	2147	rVV	97260	162596	17.48%	1.973%
57	8.481	2219	2221	2225	rVB2	308	179	0.02%	0.002%
58	8.530	2232	2236	2239	rBV2	227	207	0.02%	0.003%
59	8.642	2258	2271	2303	rBV	457996	840813	90.38%	10.202%
60	9.118	2416	2419	2425	rVB2	178	184	0.02%	0.002%
61	9.153	2425	2430	2431	rBV	195	174	0.02%	0.002%
62	9.189	2437	2441	2444	rBB	266	221	0.02%	0.003%
63	9.208	2444	2447	2449	rBV2	223	186	0.02%	0.002%
64	9.272	2461	2467	2468	rBV2	206	208	0.02%	0.003%
65	9.353	2489	2492	2498	rVB2	303	315	0.03%	0.004%
66	9.420	2498	2513	2538	rBV	568384	930295	100.00%	11.288%
67	9.571	2555	2560	2567	rVB2	534	655	0.07%	0.008%
68	9.639	2578	2581	2584	rBV2	168	144	0.02%	0.002%
69	9.697	2590	2599	2602	rBV5	949	1326	0.14%	0.016%
70	9.851	2641	2647	2654	rVB2	221	321	0.03%	0.004%
71	9.931	2667	2672	2675	rBV2	172	172	0.02%	0.002%
72	10.488	2840	2845	2848	rBV	507	546	0.06%	0.007%
73	10.542	2858	2862	2865	rBV2	208	182	0.02%	0.002%
74	10.558	2865	2867	2870	rBV	211	180	0.02%	0.002%
75	10.761	2916	2930	2949	rBV	459182	738798	79.42%	8.964%
76	10.919	2972	2979	2984	rBV2	207	354	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102021\
 Data File : VU045341.D
 Acq On : 20 Oct 2021 12:17
 Operator : SY/MD
 Sample : VU1020MBL04
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK028

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101921WMA.M
 Title : VOC Analysis

77	10.983	2995	2999	3004	rBV	218	236	0.03%	0.003%
78	11.089	3028	3032	3034	rBV	506	440	0.05%	0.005%
79	11.182	3057	3061	3062	rBV2	197	157	0.02%	0.002%
80	11.227	3071	3075	3079	rBV2	222	233	0.03%	0.003%
81	11.250	3079	3082	3086	rVV	241	220	0.02%	0.003%
82	11.279	3088	3091	3094	rVB2	233	154	0.02%	0.002%
83	11.391	3123	3126	3131	rBV2	192	226	0.02%	0.003%
84	11.475	3145	3152	3158	rVB2	1371	1852	0.20%	0.022%
85	11.552	3174	3176	3179	rBV2	176	142	0.02%	0.002%
86	11.751	3231	3238	3245	rBV3	1680	2142	0.23%	0.026%
87	11.816	3245	3258	3277	rBV	527818	843688	90.69%	10.237%
88	12.198	3363	3377	3399	rBV	500133	800255	86.02%	9.710%
89	12.375	3428	3432	3438	rBV2	254	246	0.03%	0.003%
90	12.893	3590	3593	3596	rBV	209	155	0.02%	0.002%
91	13.002	3622	3627	3630	rVB2	403	414	0.04%	0.005%
92	13.224	3689	3696	3704	rVB3	2501	3264	0.35%	0.040%
93	13.844	3881	3889	3900	rVB4	4819	7203	0.77%	0.087%
94	14.092	3956	3966	3980	rBV	12380	20093	2.16%	0.244%
95	14.179	3989	3993	3998	rBV2	495	568	0.06%	0.007%
96	14.246	4008	4014	4020	rVB2	384	644	0.07%	0.008%
97	14.279	4020	4024	4027	rBV2	393	352	0.04%	0.004%
98	14.304	4029	4032	4034	rVV	519	405	0.04%	0.005%
99	14.336	4034	4042	4053	rVB5	5860	9329	1.00%	0.113%
100	16.250	4634	4637	4638	rBV	426	249	0.03%	0.003%


Sum of corrected areas: 8241577

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102021\
Data File : VU045341.D
Acq On : 20 Oct 2021 12:17
Operator : SY/MD
Sample : VU1020MBL04
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK028

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

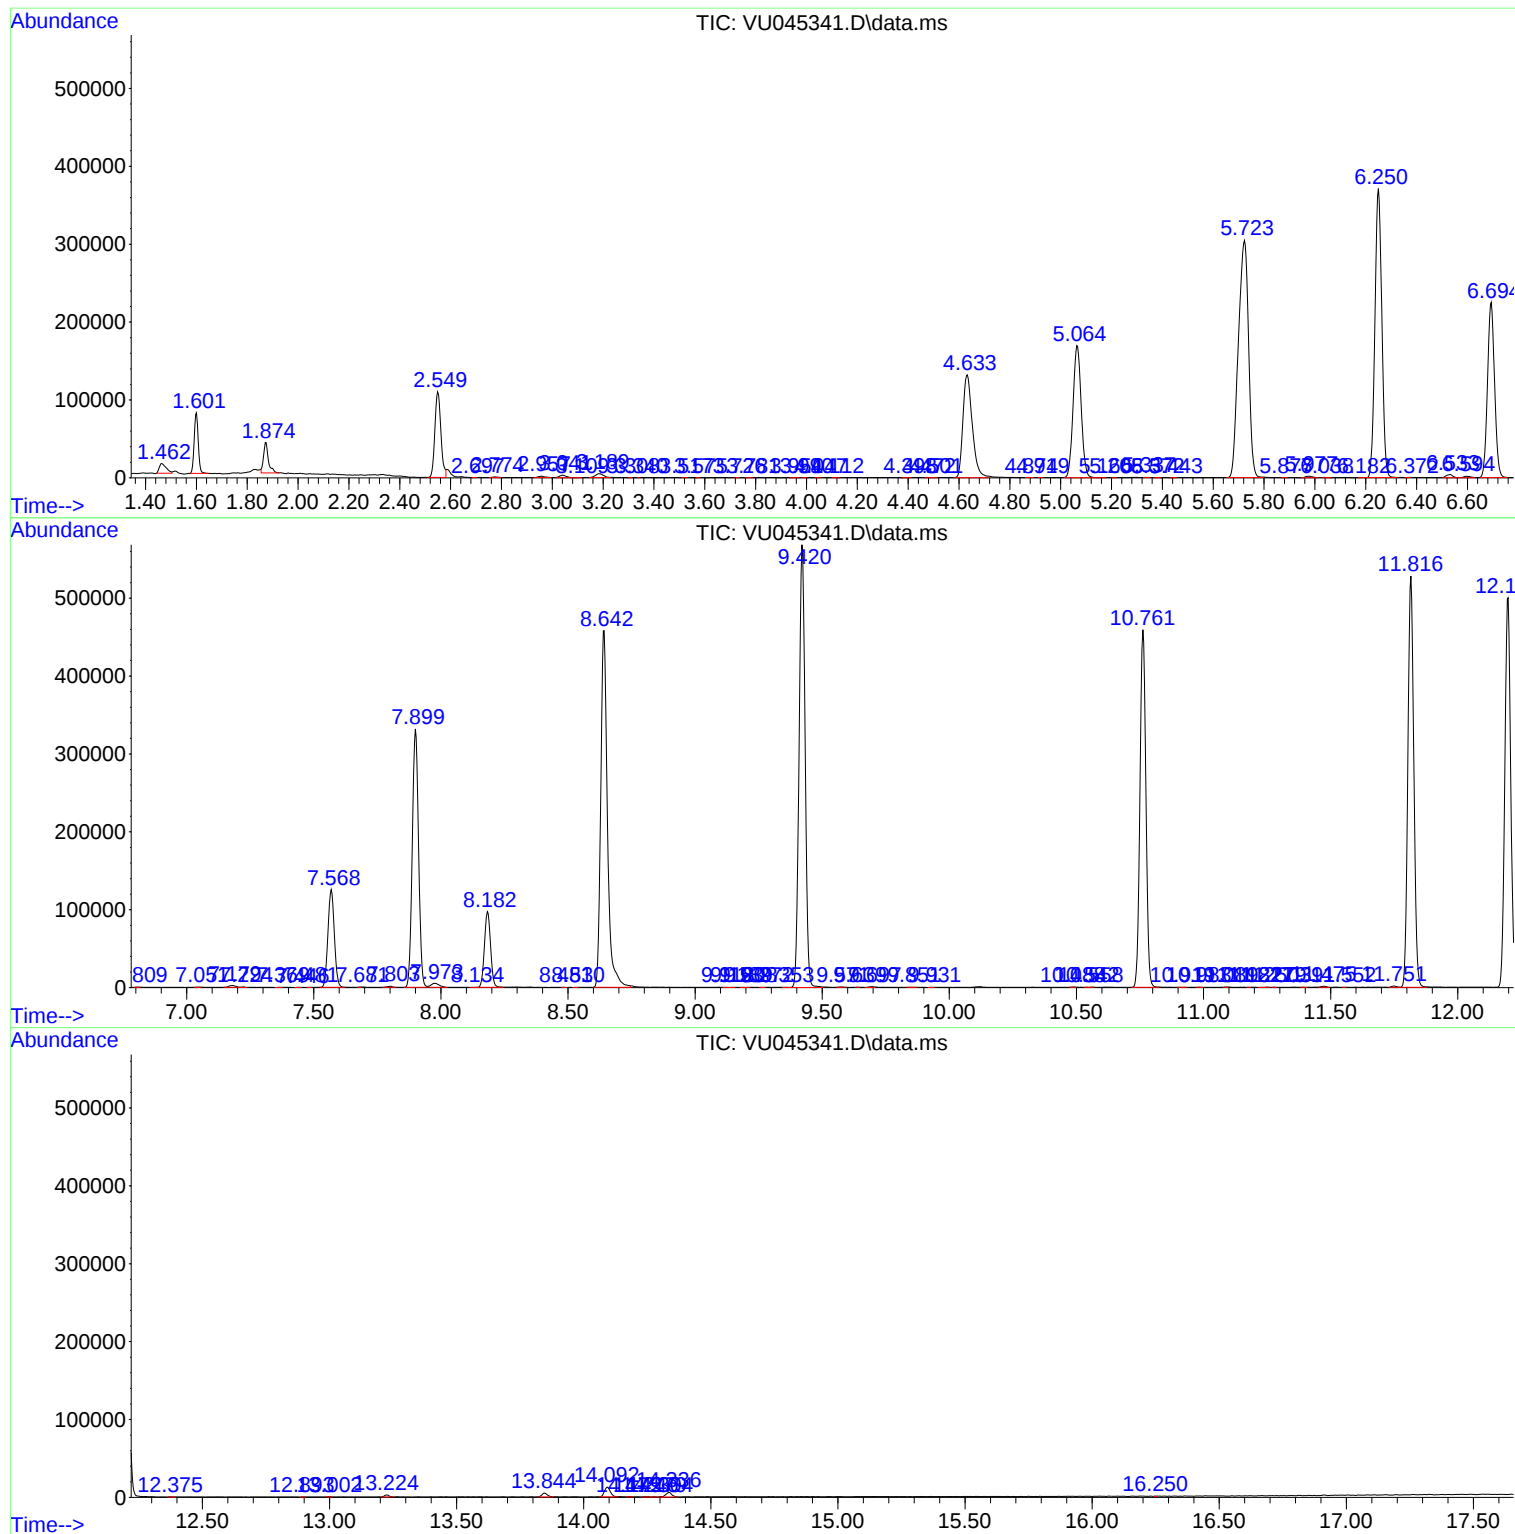

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102021\
Data File : VU045341.D
Acq On : 20 Oct 2021 12:17
Operator : SY/MD
Sample : VU1020MBL04
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK028

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102021\
Data File : VU045341.D
Acq On : 20 Oct 2021 12:17
Operator : SY/MD
Sample : VU1020MBL04
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK028

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101921WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
