
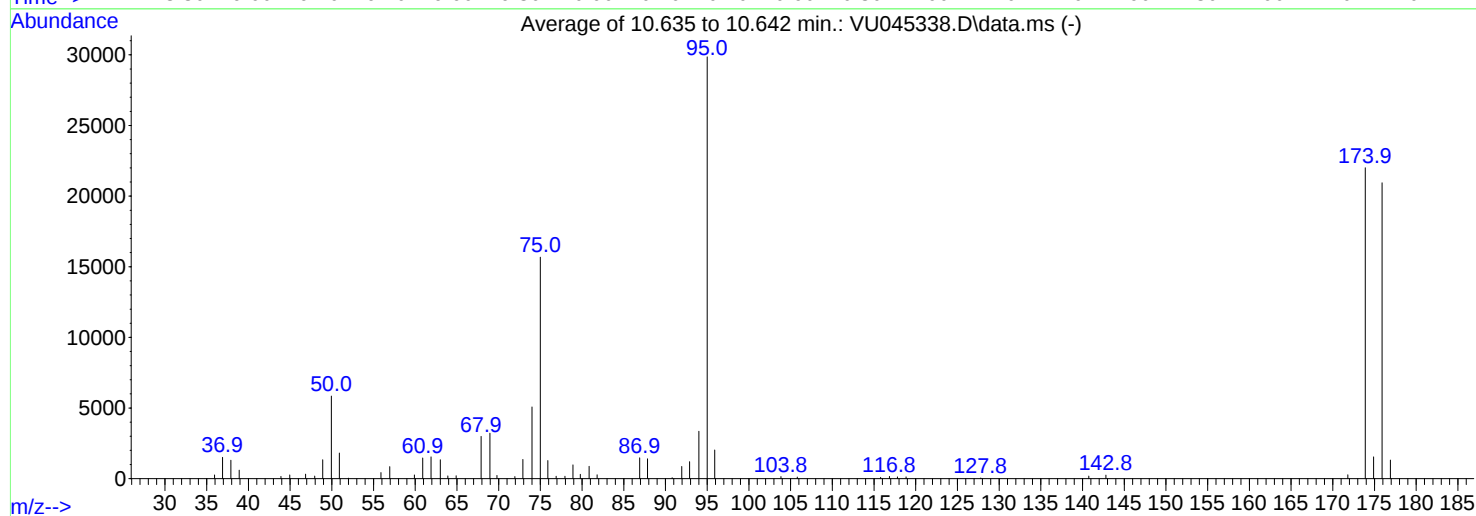


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102021\
 Data File : VU045338.D
 Acq On : 20 Oct 2021 09:22
 Operator : SY/MD
 Sample : BFB014
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB014

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101921WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 22 01:23:11 2021

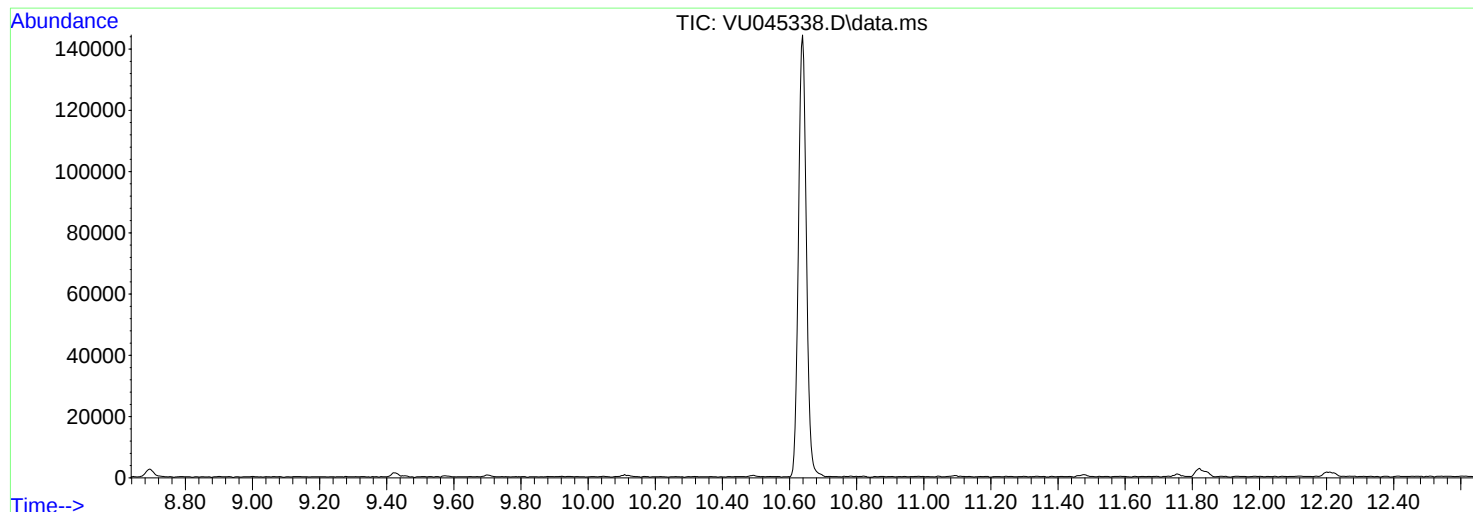

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	5844	PASS
75	95	30	80	52.5	15678	PASS
95	95	100	100	100.0	29859	PASS
96	95	5	9	6.8	2027	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.7	22005	PASS
175	174	5	9	7.0	1539	PASS
176	174	95	101	95.2	20939	PASS
177	176	5	9	6.3	1318	PASS