

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051468.D
 Acq On : 20 Oct 2022 13:34
 Operator : JC/MD
 Sample : VU1020WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK003

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M

Title : VOC Analysis

Signal : TIC: VU051468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	268015	300312	15.15%	1.967%
2	1.893	163	172	184	rBV	197081	274427	13.84%	1.797%
3	2.559	367	379	396	rVV	398390	651252	32.85%	4.265%
4	2.735	431	434	441	rVB4	394	395	0.02%	0.003%
5	2.790	441	451	459	rVV2	3868	7230	0.36%	0.047%
6	2.845	463	468	472	rVB3	652	667	0.03%	0.004%
7	3.044	515	530	543	rVB5	5349	10542	0.53%	0.069%
8	3.102	543	548	551	rBV	421	442	0.02%	0.003%
9	3.179	569	572	580	rVB3	1197	1395	0.07%	0.009%
10	3.256	593	596	600	rBV2	516	330	0.02%	0.002%
11	3.346	618	624	626	rBV4	1055	1024	0.05%	0.007%
12	3.481	663	666	671	rVV2	523	568	0.03%	0.004%
13	3.542	682	685	690	rVB2	436	350	0.02%	0.002%
14	3.568	690	693	699	rBV3	419	476	0.02%	0.003%
15	3.793	754	763	771	rVB2	563	897	0.05%	0.006%
16	3.980	811	821	826	rBV3	438	542	0.03%	0.004%
17	4.240	893	902	906	rBV2	362	449	0.02%	0.003%
18	4.449	961	967	971	rVB3	425	550	0.03%	0.004%
19	4.533	988	993	997	rVB2	410	454	0.02%	0.003%
20	4.562	997	1002	1004	rBV	426	345	0.02%	0.002%
21	4.616	1007	1019	1059	rBV	196898	484081	24.42%	3.170%
22	4.977	1128	1131	1136	rVB5	654	591	0.03%	0.004%
23	5.060	1136	1157	1179	rBV	355890	782538	39.47%	5.125%
24	5.282	1223	1226	1228	rBV3	828	657	0.03%	0.004%
25	5.317	1236	1237	1242	rBV2	460	329	0.02%	0.002%
26	5.722	1341	1363	1394	rBV2	732185	1982419	100.00%	12.983%
27	5.967	1436	1439	1446	rVB6	1351	1484	0.07%	0.010%
28	5.999	1447	1449	1452	rVB3	809	419	0.02%	0.003%
29	6.044	1460	1463	1477	rVB4	848	1380	0.07%	0.009%
30	6.099	1477	1480	1483	rBV3	648	504	0.03%	0.003%
31	6.118	1483	1486	1490	rVB2	584	436	0.02%	0.003%
32	6.247	1512	1526	1550	rBV	646268	1239857	62.54%	8.120%
33	6.533	1603	1615	1626	rVB	4102	8494	0.43%	0.056%
34	6.613	1637	1640	1644	rVB3	742	517	0.03%	0.003%
35	6.687	1644	1663	1682	rBV	456428	897594	45.28%	5.878%
36	6.886	1722	1725	1731	rVB5	493	522	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051468.D
 Acq On : 20 Oct 2022 13:34
 Operator : JC/MD
 Sample : VU1020WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK003

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

37	7.002	1755	1761	1766	rVB4	367	393	0.02%	0.003%
38	7.189	1810	1819	1829	rVV8	2100	4455	0.22%	0.029%
39	7.282	1844	1848	1852	rBV2	500	459	0.02%	0.003%
40	7.388	1876	1881	1885	rBV2	505	522	0.03%	0.003%
41	7.430	1888	1894	1899	rVB2	387	364	0.02%	0.002%
42	7.562	1922	1935	1958	rBV	229614	407409	20.55%	2.668%
43	7.697	1969	1977	1985	rVB5	1230	1806	0.09%	0.012%
44	7.793	2001	2007	2008	rBV3	2175	2007	0.10%	0.013%
45	7.896	2025	2039	2062	rBV	869834	1503603	75.85%	9.847%
46	8.176	2114	2126	2147	rBV	163117	275581	13.90%	1.805%
47	8.324	2166	2172	2176	rVB5	948	1224	0.06%	0.008%
48	8.346	2176	2179	2182	rBV2	840	541	0.03%	0.004%
49	8.398	2188	2195	2200	rVB4	981	1175	0.06%	0.008%
50	8.552	2233	2243	2248	rBV8	2481	3533	0.18%	0.023%
51	8.632	2255	2268	2301	rBV2	581397	1100874	55.53%	7.210%
52	8.918	2353	2357	2362	rBV3	884	790	0.04%	0.005%
53	9.050	2395	2398	2401	rVB5	535	354	0.02%	0.002%
54	9.108	2413	2416	2421	rVB3	372	355	0.02%	0.002%
55	9.137	2421	2425	2427	rBV	409	326	0.02%	0.002%
56	9.253	2458	2461	2465	rVB2	543	381	0.02%	0.002%
57	9.275	2465	2468	2474	rBV3	409	483	0.02%	0.003%
58	9.414	2498	2511	2539	rBV	916332	1534346	77.40%	10.048%
59	9.571	2555	2560	2568	rVB5	2541	3410	0.17%	0.022%
60	9.610	2568	2572	2576	rVB4	699	493	0.02%	0.003%
61	9.690	2589	2597	2599	rBV3	1828	1802	0.09%	0.012%
62	9.767	2616	2621	2626	rVB3	345	397	0.02%	0.003%
63	10.111	2719	2728	2736	rVV8	2280	4260	0.21%	0.028%
64	10.176	2741	2748	2753	rBV3	494	598	0.03%	0.004%
65	10.201	2753	2756	2761	rVB2	446	395	0.02%	0.003%
66	10.298	2778	2786	2788	rVV3	337	379	0.02%	0.002%
67	10.381	2808	2812	2817	rBV	483	446	0.02%	0.003%
68	10.414	2817	2822	2826	rVV3	414	427	0.02%	0.003%
69	10.488	2837	2845	2850	rVV4	1328	1681	0.08%	0.011%
70	10.674	2899	2903	2907	rBV2	330	347	0.02%	0.002%
71	10.754	2915	2928	2947	rBV	693101	1134448	57.23%	7.429%
72	10.886	2965	2969	2977	rVB3	793	765	0.04%	0.005%
73	10.986	2995	3000	3003	rBV2	481	482	0.02%	0.003%
74	11.092	3026	3033	3040	rVV4	1420	2400	0.12%	0.016%
75	11.124	3040	3043	3049	rVB2	565	646	0.03%	0.004%
76	11.304	3092	3099	3100	rBV	359	331	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051468.D
 Acq On : 20 Oct 2022 13:34
 Operator : JC/MD
 Sample : VU1020WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK003

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

77	11.471	3142	3151	3160	rVV3	2197	3034	0.15%	0.020%
78	11.748	3229	3237	3243	rBV6	4256	6499	0.33%	0.043%
79	11.809	3244	3256	3282	rBV	770975	1252345	63.17%	8.202%
80	12.053	3328	3332	3335	rBV2	549	365	0.02%	0.002%
81	12.192	3362	3375	3399	rBV	786935	1279896	64.56%	8.382%
82	12.655	3517	3519	3523	rVB	551	364	0.02%	0.002%
83	12.809	3564	3567	3569	rBV3	573	350	0.02%	0.002%
84	12.835	3572	3575	3581	rVV3	347	411	0.02%	0.003%
85	12.995	3621	3625	3634	rBV5	1283	1905	0.10%	0.012%
86	13.050	3637	3642	3646	rBV4	662	751	0.04%	0.005%
87	13.105	3656	3659	3662	rBV	884	766	0.04%	0.005%
88	13.172	3678	3680	3684	rBV	516	378	0.02%	0.002%
89	13.224	3688	3696	3712	rVB7	5626	10606	0.54%	0.069%
90	13.336	3727	3731	3734	rBV2	418	414	0.02%	0.003%
91	13.587	3803	3809	3816	rBV3	663	982	0.05%	0.006%
92	13.844	3879	3889	3904	rBV3	9151	15027	0.76%	0.098%
93	14.002	3935	3938	3942	rBV2	558	375	0.02%	0.002%
94	14.089	3956	3965	3978	rBV	14536	26220	1.32%	0.172%
95	14.179	3991	3993	3996	rBV4	588	390	0.02%	0.003%
96	14.333	4032	4041	4056	rVB2	9733	16408	0.83%	0.107%
97	14.529	4099	4102	4107	rBV3	553	516	0.03%	0.003%
98	15.195	4305	4309	4311	rBV2	776	704	0.04%	0.005%
99	15.532	4410	4414	4416	rBV2	1275	1078	0.05%	0.007%
100	16.028	4565	4568	4572	rBV4	990	687	0.03%	0.004%


Sum of corrected areas: 15269628

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051468.D
Acq On : 20 Oct 2022 13:34
Operator : JC/MD
Sample : VU1020WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

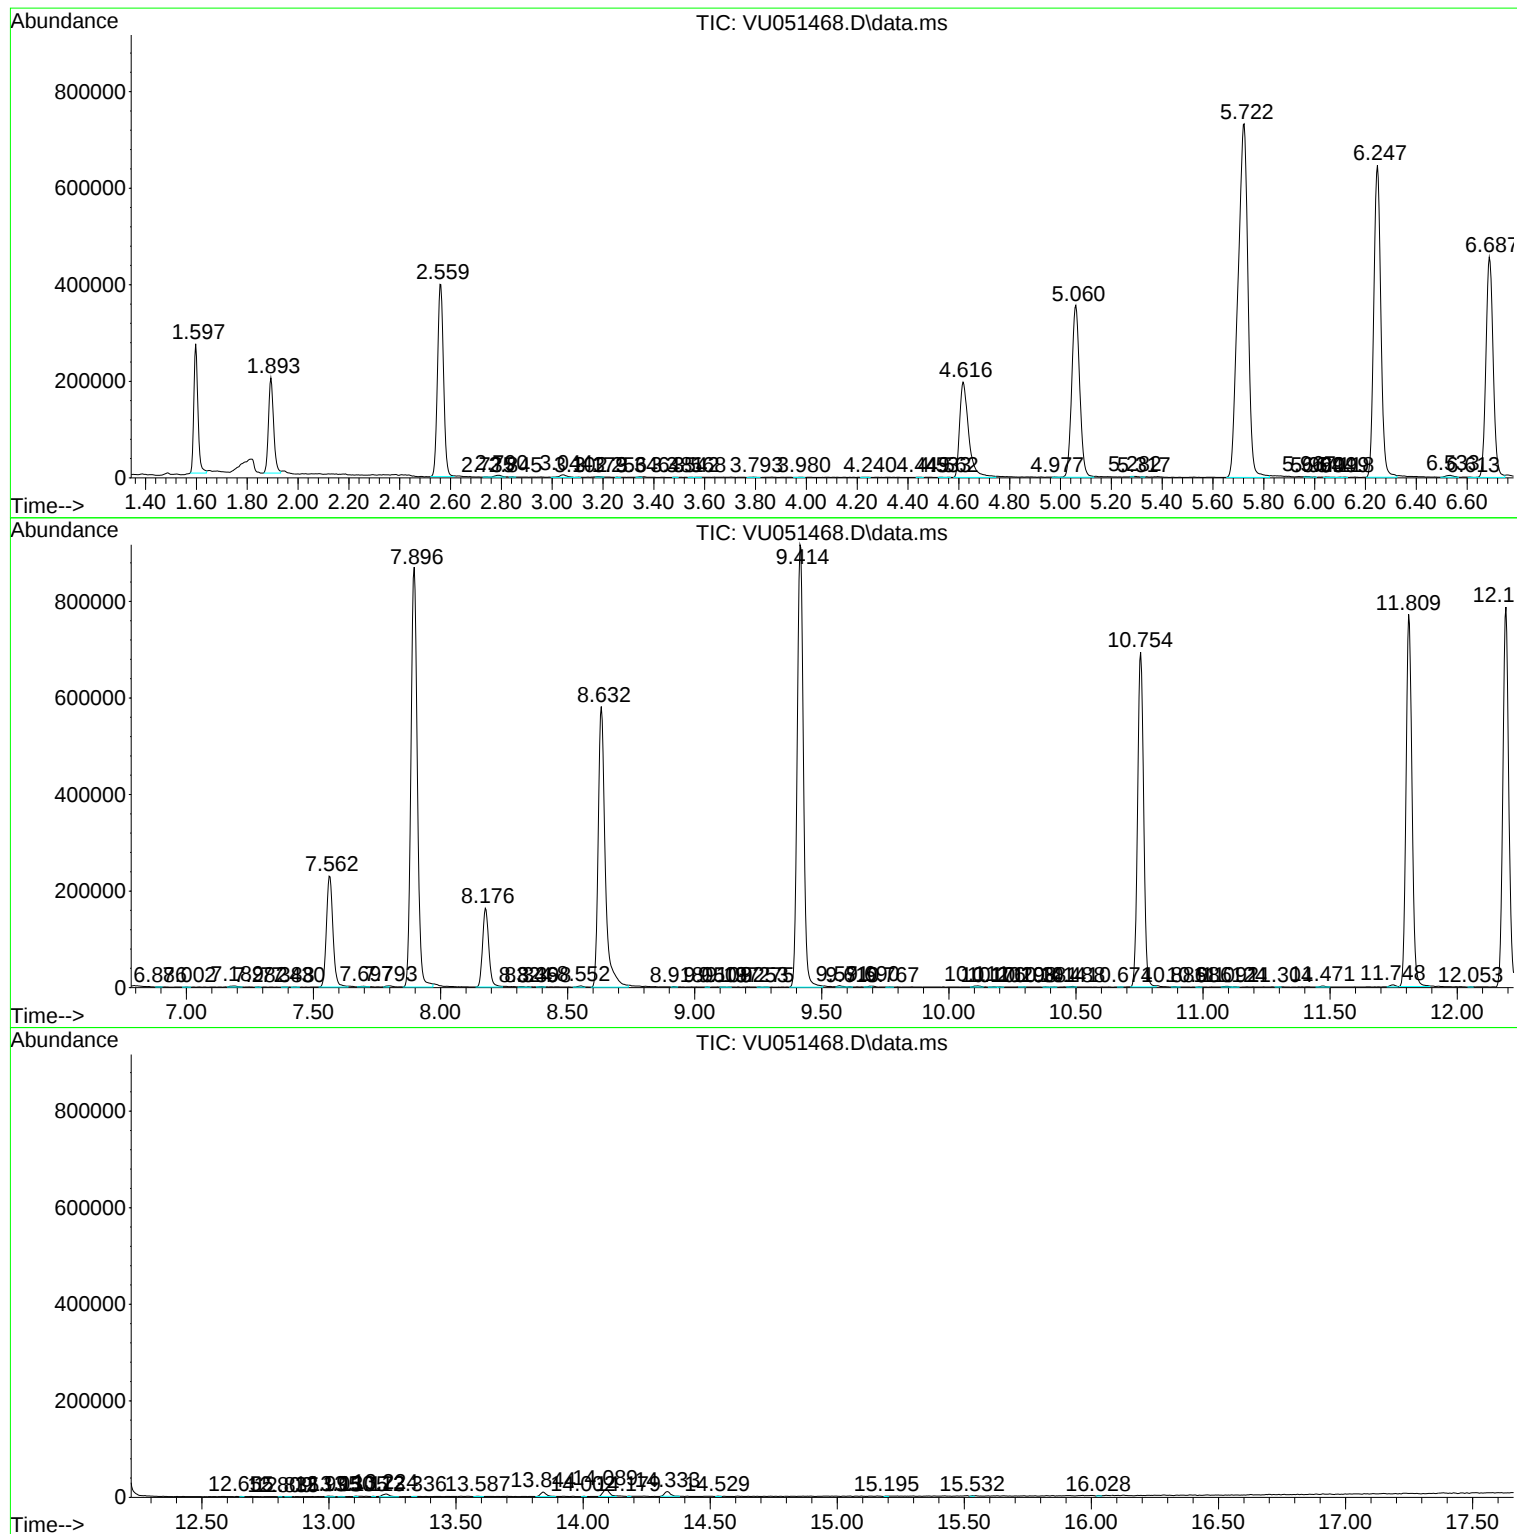

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051468.D
Acq On : 20 Oct 2022 13:34
Operator : JC/MD
Sample : VU1020WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051468.D
Acq On : 20 Oct 2022 13:34
Operator : JC/MD
Sample : VU1020WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK003

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc