

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051470.D
 Acq On : 20 Oct 2022 14:29
 Operator : JC/MD
 Sample : N5180-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0TF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

Signal : TIC: VU051470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	52	57	65	rVB	16994	19876	0.98%	0.132%
2	1.597	73	80	95	rBV	261997	304213	15.01%	2.015%
3	1.900	165	174	203	rVB	195981	288872	14.25%	1.914%
4	2.562	367	380	393	rBV	390450	635285	31.34%	4.208%
5	3.041	521	529	540	rBV5	1813	3683	0.18%	0.024%
6	3.179	561	572	589	rVB2	6811	15044	0.74%	0.100%
7	3.350	616	625	628	rBV5	868	1201	0.06%	0.008%
8	3.494	664	670	674	rBV3	370	391	0.02%	0.003%
9	3.723	734	741	743	rBV2	375	323	0.02%	0.002%
10	3.787	758	761	768	rBV3	340	392	0.02%	0.003%
11	3.906	795	798	802	rVB3	520	412	0.02%	0.003%
12	4.015	829	832	838	rVB3	348	381	0.02%	0.003%
13	4.305	918	922	931	rBV3	378	484	0.02%	0.003%
14	4.401	950	952	959	rVV2	399	330	0.02%	0.002%
15	4.433	959	962	967	rVB2	597	494	0.02%	0.003%
16	4.465	967	972	975	rBV3	520	493	0.02%	0.003%
17	4.616	1005	1019	1049	rBV	207003	508761	25.10%	3.370%
18	4.954	1121	1124	1128	rVB4	557	391	0.02%	0.003%
19	4.999	1132	1138	1140	rBV4	500	509	0.03%	0.003%
20	5.060	1141	1157	1184	rBV	364986	793699	39.15%	5.258%
21	5.285	1218	1227	1232	rBV6	1687	3070	0.15%	0.020%
22	5.369	1249	1253	1256	rBV3	732	676	0.03%	0.004%
23	5.443	1270	1276	1283	rBV3	304	428	0.02%	0.003%
24	5.723	1339	1363	1389	rBV2	743502	2027210	100.00%	13.429%
25	6.028	1454	1458	1463	rBV5	729	747	0.04%	0.005%
26	6.051	1463	1465	1470	rVB3	605	501	0.02%	0.003%
27	6.124	1486	1488	1492	rVB3	705	415	0.02%	0.003%
28	6.173	1500	1503	1506	rVB2	492	329	0.02%	0.002%
29	6.198	1506	1511	1512	rBV3	484	351	0.02%	0.002%
30	6.247	1512	1526	1550	rBV	596904	1130249	55.75%	7.487%
31	6.452	1587	1590	1592	rVB3	777	433	0.02%	0.003%
32	6.469	1592	1595	1599	rBV2	497	348	0.02%	0.002%
33	6.526	1604	1613	1627	rVB2	2929	6273	0.31%	0.042%
34	6.687	1649	1663	1682	rBV	480103	921650	45.46%	6.105%
35	6.967	1747	1750	1754	rVB3	513	358	0.02%	0.002%
36	7.070	1778	1782	1790	rVB3	545	841	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051470.D
 Acq On : 20 Oct 2022 14:29
 Operator : JC/MD
 Sample : N5180-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0TF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

37	7.179	1809	1816	1826	rBV10	2138	3861	0.19%	0.026%
38	7.388	1875	1881	1885	rBV3	395	403	0.02%	0.003%
39	7.501	1913	1916	1919	rBV	388	327	0.02%	0.002%
40	7.562	1922	1935	1952	rBV	230416	408593	20.16%	2.707%
41	7.694	1973	1976	1984	rVB5	1603	1921	0.09%	0.013%
42	7.758	1992	1996	2000	rBV2	356	373	0.02%	0.002%
43	7.790	2002	2006	2009	rVV3	659	538	0.03%	0.004%
44	7.896	2025	2039	2060	rBV	865070	1504837	74.23%	9.968%
45	8.176	2114	2126	2151	rVV	165067	283701	13.99%	1.879%
46	8.472	2207	2218	2227	rBV2	4220	7706	0.38%	0.051%
47	8.523	2231	2234	2238	rBV5	450	448	0.02%	0.003%
48	8.549	2238	2242	2250	rVB4	979	1250	0.06%	0.008%
49	8.629	2256	2267	2302	rBV2	591242	1126612	55.57%	7.463%
50	8.902	2348	2352	2355	rVB3	643	444	0.02%	0.003%
51	8.938	2360	2363	2367	rVB5	787	602	0.03%	0.004%
52	8.960	2367	2370	2373	rBV3	604	511	0.03%	0.003%
53	9.028	2388	2391	2398	rVB3	506	544	0.03%	0.004%
54	9.063	2398	2402	2403	rBV	363	319	0.02%	0.002%
55	9.195	2441	2443	2448	rVB3	417	345	0.02%	0.002%
56	9.414	2497	2511	2533	rBV	832203	1398015	68.96%	9.261%
57	9.562	2553	2557	2559	rBV4	952	785	0.04%	0.005%
58	9.594	2565	2567	2571	rVB3	578	343	0.02%	0.002%
59	9.700	2591	2600	2602	rBV4	1276	1651	0.08%	0.011%
60	9.899	2659	2662	2665	rBV2	431	319	0.02%	0.002%
61	10.099	2719	2724	2725	rBV3	817	640	0.03%	0.004%
62	10.118	2728	2730	2741	rVB4	1159	1172	0.06%	0.008%
63	10.250	2764	2771	2775	rBV2	603	706	0.03%	0.005%
64	10.314	2787	2791	2793	rBV	470	344	0.02%	0.002%
65	10.481	2838	2843	2845	rBV2	1196	986	0.05%	0.007%
66	10.690	2902	2908	2912	rBV3	441	502	0.02%	0.003%
67	10.755	2912	2928	2952	rBV	717826	1142293	56.35%	7.567%
68	10.890	2963	2970	2971	rBV5	2761	2806	0.14%	0.019%
69	10.996	2998	3003	3006	rBV3	536	541	0.03%	0.004%
70	11.153	3049	3052	3054	rBV2	409	320	0.02%	0.002%
71	11.198	3062	3066	3069	rVV2	445	376	0.02%	0.002%
72	11.279	3088	3091	3097	rVB3	585	458	0.02%	0.003%
73	11.372	3116	3120	3125	rBV2	562	523	0.03%	0.003%
74	11.414	3129	3133	3140	rBV4	566	565	0.03%	0.004%
75	11.468	3146	3150	3153	rBV2	942	987	0.05%	0.007%
76	11.594	3187	3189	3197	rVB2	570	494	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051470.D
 Acq On : 20 Oct 2022 14:29
 Operator : JC/MD
 Sample : N5180-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0TF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

77	11.636	3197	3202	3204	rBV3	564	482	0.02%	0.003%
78	11.687	3214	3218	3223	rVB2	577	559	0.03%	0.004%
79	11.719	3223	3228	3229	rBV2	429	395	0.02%	0.003%
80	11.748	3229	3237	3243	rBV5	2901	4179	0.21%	0.028%
81	11.809	3243	3256	3276	rBV	686701	1113367	54.92%	7.375%
82	11.989	3308	3312	3314	rBV3	410	360	0.02%	0.002%
83	12.066	3325	3336	3353	rBV3	13379	28569	1.41%	0.189%
84	12.192	3362	3375	3394	rBV	785104	1293255	63.79%	8.567%
85	12.385	3432	3435	3440	rBV4	759	572	0.03%	0.004%
86	12.761	3545	3552	3553	rBV2	946	1010	0.05%	0.007%
87	12.848	3574	3579	3582	rBV2	584	570	0.03%	0.004%
88	13.057	3640	3644	3647	rVV2	548	402	0.02%	0.003%
89	13.102	3655	3658	3661	rBV2	406	327	0.02%	0.002%
90	13.217	3684	3694	3703	rBV7	4931	8038	0.40%	0.053%
91	13.417	3752	3756	3759	rVB2	484	400	0.02%	0.003%
92	13.761	3860	3863	3865	rBV3	451	319	0.02%	0.002%
93	13.841	3880	3888	3900	rBV4	17348	28139	1.39%	0.186%
94	14.092	3956	3966	3973	rBV2	5303	8886	0.44%	0.059%
95	14.285	4023	4026	4030	rBV3	814	644	0.03%	0.004%
96	14.333	4030	4041	4053	rVV4	12318	21463	1.06%	0.142%
97	14.738	4160	4167	4176	rVV5	2678	4259	0.21%	0.028%
98	14.941	4227	4230	4231	rBV3	649	322	0.02%	0.002%
99	15.021	4251	4255	4259	rBV3	623	782	0.04%	0.005%
100	16.002	4552	4560	4576	rVB7	6286	11533	0.57%	0.076%




Sum of corrected areas: 15096106

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051470.D
Acq On : 20 Oct 2022 14:29
Operator : JC/MD
Sample : N5180-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0TF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

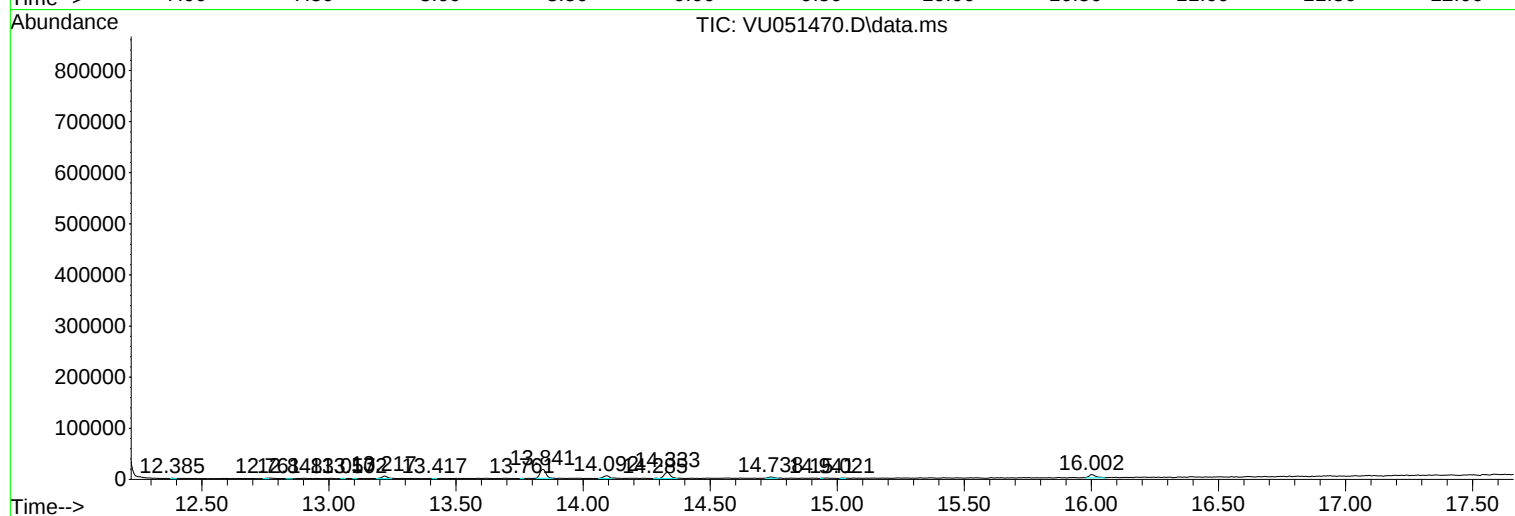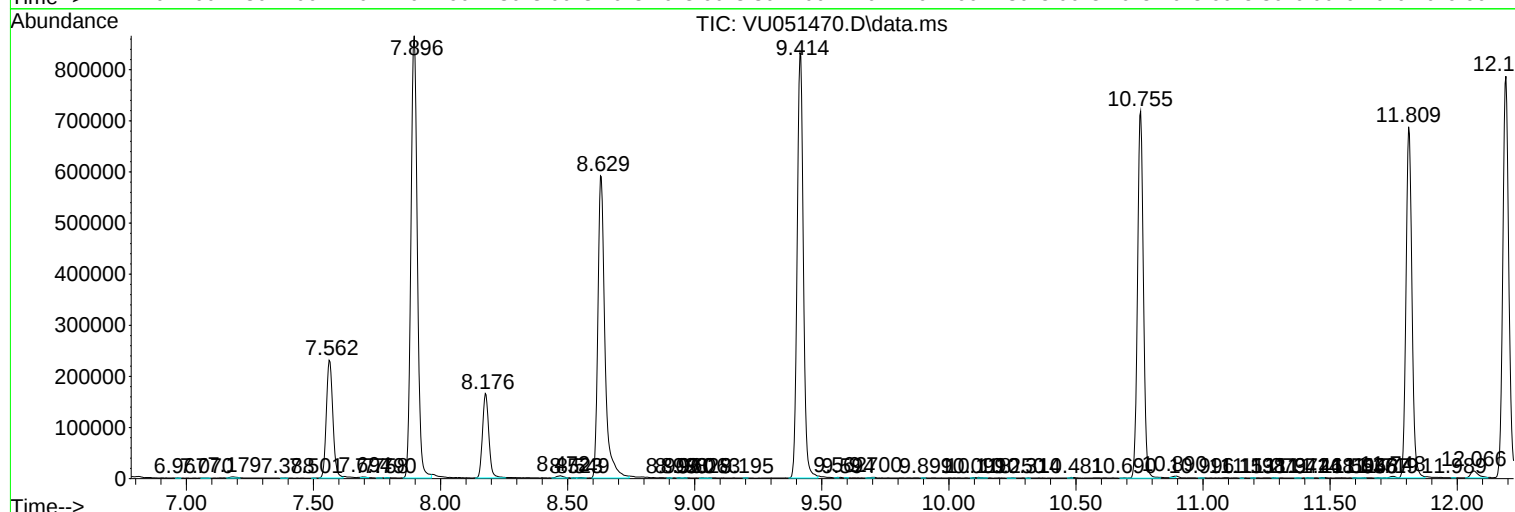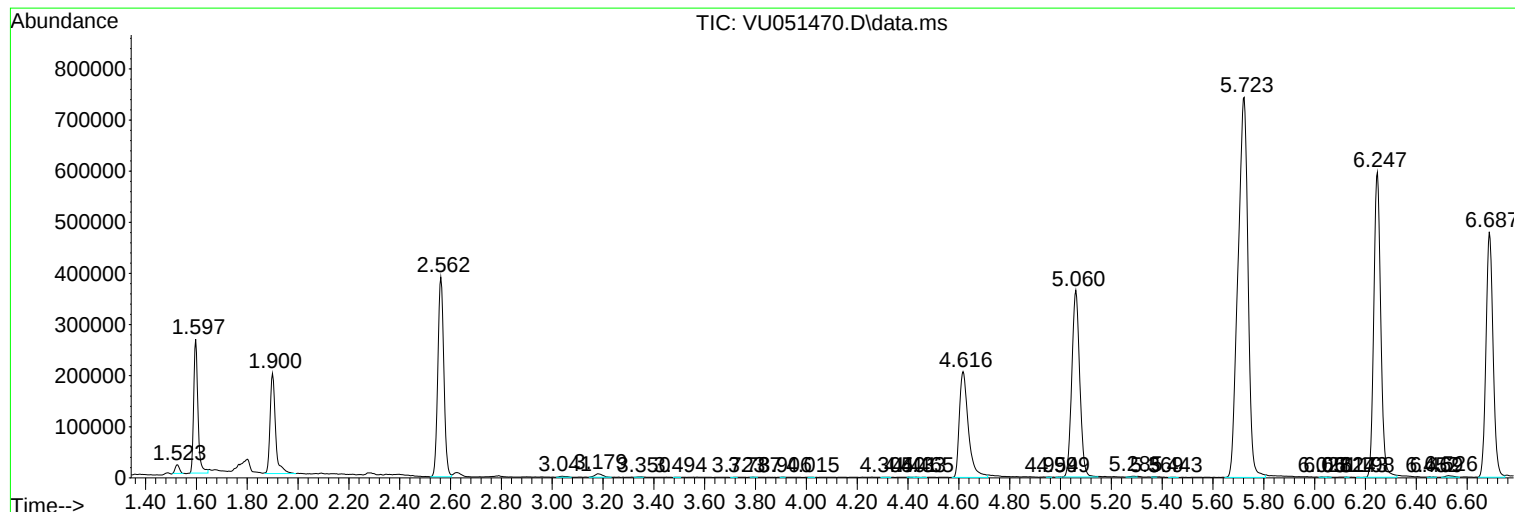

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051470.D
Acq On : 20 Oct 2022 14:29
Operator : JC/MD
Sample : N5180-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0TF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051470.D
Acq On : 20 Oct 2022 14:29
Operator : JC/MD
Sample : N5180-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0TF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc