

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051471.D
 Acq On : 20 Oct 2022 14:53
 Operator : JC/MD
 Sample : N5180-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

Signal : TIC: VU051471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	102	rVB	242816	270315	14.54%	1.941%
2	1.900	166	174	201	rVB	184470	265510	14.28%	1.906%
3	2.562	368	380	396	rBV	357774	582608	31.34%	4.183%
4	2.880	476	479	480	rBV	656	361	0.02%	0.003%
5	2.932	493	495	496	rBV	421	185	0.01%	0.001%
6	3.041	517	529	540	rBV6	1739	3566	0.19%	0.026%
7	3.121	550	554	556	rBV2	465	301	0.02%	0.002%
8	3.183	562	573	591	rVB2	15159	34698	1.87%	0.249%
9	3.253	591	595	598	rBV3	376	348	0.02%	0.002%
10	3.276	599	602	605	rVB2	336	215	0.01%	0.002%
11	3.424	646	648	649	rBV2	270	117	0.01%	0.001%
12	3.475	660	664	665	rBV	258	163	0.01%	0.001%
13	3.504	670	673	676	rVB2	277	141	0.01%	0.001%
14	3.530	678	681	685	rVV	414	348	0.02%	0.002%
15	3.578	692	696	698	rBV	388	302	0.02%	0.002%
16	3.642	713	716	719	rBV2	398	302	0.02%	0.002%
17	3.755	749	751	752	rBV	248	90	0.00%	0.001%
18	3.800	762	765	770	rBV2	384	396	0.02%	0.003%
19	3.890	791	793	798	rBV	187	127	0.01%	0.001%
20	3.932	804	806	809	rVB	362	182	0.01%	0.001%
21	3.957	809	814	817	rBV2	278	268	0.01%	0.002%
22	4.019	830	833	836	rBV2	242	170	0.01%	0.001%
23	4.038	836	839	841	rBV2	185	140	0.01%	0.001%
24	4.109	858	861	863	rBV	255	176	0.01%	0.001%
25	4.186	881	885	889	rBV2	326	333	0.02%	0.002%
26	4.228	895	898	901	rBV2	297	207	0.01%	0.001%
27	4.244	901	903	907	rVB2	403	280	0.02%	0.002%
28	4.269	908	911	913	rBV	173	92	0.00%	0.001%
29	4.305	918	922	924	rBV3	289	208	0.01%	0.001%
30	4.340	931	933	937	rBV2	375	217	0.01%	0.002%
31	4.424	956	959	963	rBV2	180	119	0.01%	0.001%
32	4.469	971	973	977	rBV3	282	221	0.01%	0.002%
33	4.617	1007	1019	1051	rBV	188393	467568	25.15%	3.357%
34	4.970	1125	1129	1133	rVB	773	579	0.03%	0.004%
35	5.060	1139	1157	1178	rBV	340486	742851	39.95%	5.334%
36	5.485	1284	1289	1291	rBV	474	425	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051471.D
 Acq On : 20 Oct 2022 14:53
 Operator : JC/MD
 Sample : N5180-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

37	5.520	1297	1300	1305	rVB3	421	380	0.02%	0.003%
38	5.546	1305	1308	1311	rBV2	252	161	0.01%	0.001%
39	5.581	1317	1319	1321	rBV	181	96	0.01%	0.001%
40	5.629	1331	1334	1336	rBV	241	148	0.01%	0.001%
41	5.723	1340	1363	1385	rBV2	684797	1859239	100.00%	13.349%
42	6.176	1501	1504	1507	rBV	472	249	0.01%	0.002%
43	6.247	1511	1526	1554	rBV	583467	1122027	60.35%	8.056%
44	6.530	1606	1614	1618	rBV5	1965	3159	0.17%	0.023%
45	6.565	1622	1625	1628	rBV3	378	265	0.01%	0.002%
46	6.687	1648	1663	1687	rBV	443984	855676	46.02%	6.144%
47	6.935	1737	1740	1744	rVB4	275	251	0.01%	0.002%
48	6.957	1744	1747	1749	rBV2	247	175	0.01%	0.001%
49	6.993	1755	1758	1759	rBV	254	130	0.01%	0.001%
50	7.031	1767	1770	1773	rBV2	196	150	0.01%	0.001%
51	7.051	1773	1776	1780	rVB2	453	272	0.01%	0.002%
52	7.083	1782	1786	1791	rBV	270	234	0.01%	0.002%
53	7.134	1796	1802	1806	rBV3	294	365	0.02%	0.003%
54	7.186	1806	1818	1825	rBV6	2381	4351	0.23%	0.031%
55	7.260	1839	1841	1846	rVB	310	204	0.01%	0.001%
56	7.292	1847	1851	1852	rBV	129	95	0.01%	0.001%
57	7.346	1865	1868	1869	rBV	170	92	0.00%	0.001%
58	7.401	1882	1885	1886	rBV2	183	91	0.00%	0.001%
59	7.456	1897	1902	1906	rVB2	307	317	0.02%	0.002%
60	7.481	1906	1910	1912	rBV2	309	231	0.01%	0.002%
61	7.562	1923	1935	1955	rBV	207367	375888	20.22%	2.699%
62	7.755	1992	1995	1997	rVB2	603	345	0.02%	0.002%
63	7.771	1997	2000	2003	rBV3	366	320	0.02%	0.002%
64	7.845	2019	2023	2025	rBV	491	456	0.02%	0.003%
65	7.896	2025	2039	2059	rBV	786292	1368451	73.60%	9.825%
66	8.176	2115	2126	2144	rBV	150100	255044	13.72%	1.831%
67	8.472	2206	2218	2230	rBV3	5432	9950	0.54%	0.071%
68	8.629	2255	2267	2296	rBV2	530459	1016306	54.66%	7.297%
69	8.854	2333	2337	2343	rBV5	834	880	0.05%	0.006%
70	9.141	2423	2426	2428	rBV	297	163	0.01%	0.001%
71	9.186	2437	2440	2442	rBV2	293	158	0.01%	0.001%
72	9.263	2461	2464	2466	rBV2	320	183	0.01%	0.001%
73	9.366	2491	2496	2498	rBV2	345	312	0.02%	0.002%
74	9.414	2498	2511	2550	rVV	814970	1375840	74.00%	9.878%
75	9.597	2566	2568	2569	rBV2	286	126	0.01%	0.001%
76	9.732	2607	2610	2613	rVB2	328	206	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051471.D
 Acq On : 20 Oct 2022 14:53
 Operator : JC/MD
 Sample : N5180-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

77	9.758	2615	2618	2622	rBV2	284	213	0.01%	0.002%
78	9.883	2654	2657	2662	rBV3	399	257	0.01%	0.002%
79	9.980	2683	2687	2690	rBV3	407	369	0.02%	0.003%
80	10.009	2694	2696	2700	rBV2	176	126	0.01%	0.001%
81	10.121	2726	2731	2734	rBV3	673	687	0.04%	0.005%
82	10.192	2750	2753	2760	rBV	461	454	0.02%	0.003%
83	10.250	2766	2771	2773	rBV2	270	263	0.01%	0.002%
84	10.333	2793	2797	2798	rBV2	379	250	0.01%	0.002%
85	10.446	2829	2832	2837	rBV3	441	414	0.02%	0.003%
86	10.645	2893	2894	2896	rBV	365	164	0.01%	0.001%
87	10.755	2915	2928	2947	rBV	649608	1049961	56.47%	7.539%
88	10.890	2963	2970	2981	rVB3	5212	9241	0.50%	0.066%
89	10.935	2982	2984	2987	rVB	318	146	0.01%	0.001%
90	11.005	3002	3006	3009	rVB2	518	359	0.02%	0.003%
91	11.185	3059	3062	3064	rBV	235	146	0.01%	0.001%
92	11.259	3083	3085	3089	rVB2	336	175	0.01%	0.001%
93	11.510	3161	3163	3166	rBV	457	300	0.02%	0.002%
94	11.661	3206	3210	3212	rBV	282	258	0.01%	0.002%
95	11.809	3243	3256	3284	rBV	644982	1052567	56.61%	7.557%
96	12.063	3326	3335	3352	rBV3	14357	28142	1.51%	0.202%
97	12.192	3362	3375	3404	rBV	686344	1145077	61.59%	8.222%
98	13.224	3692	3696	3704	rVB6	1571	1846	0.10%	0.013%
99	13.372	3739	3742	3745	rBV2	626	463	0.02%	0.003%
100	13.848	3881	3890	3898	rBV4	5494	8655	0.47%	0.062%




Sum of corrected areas: 13927648

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051471.D
Acq On : 20 Oct 2022 14:53
Operator : JC/MD
Sample : N5180-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

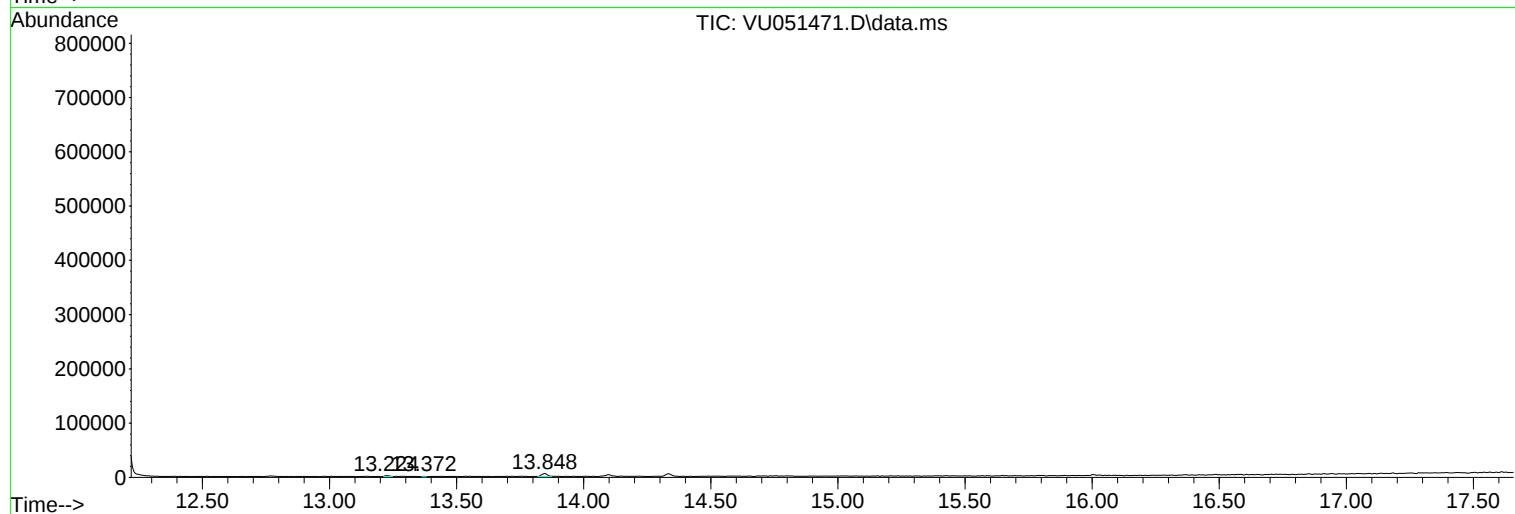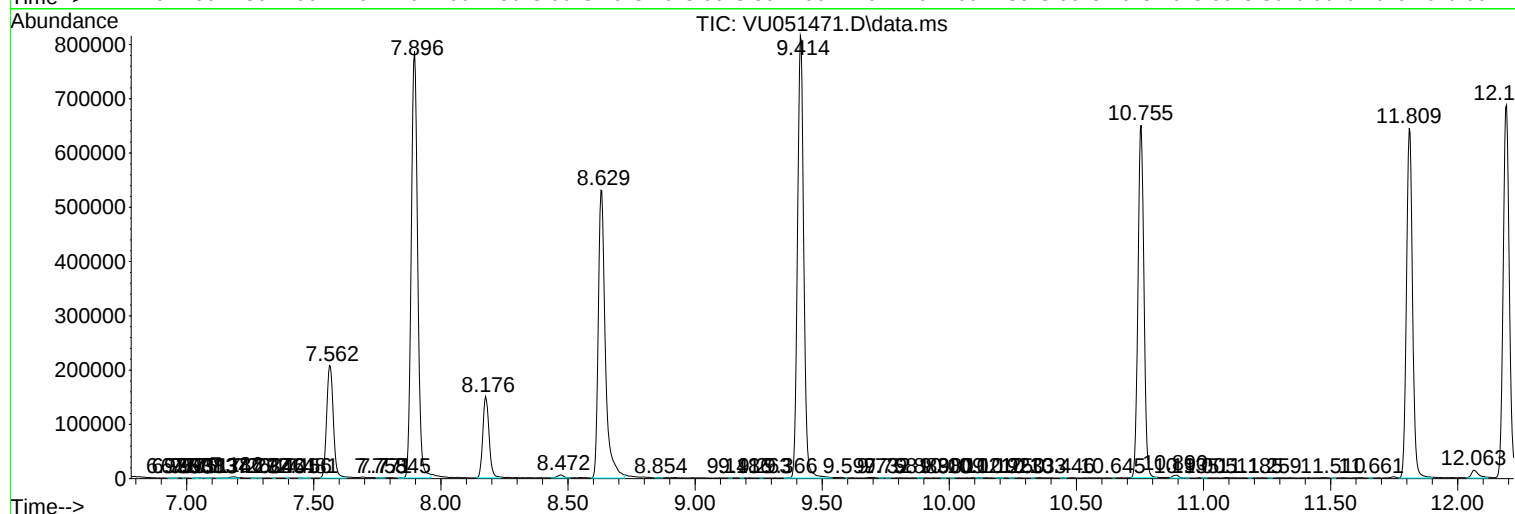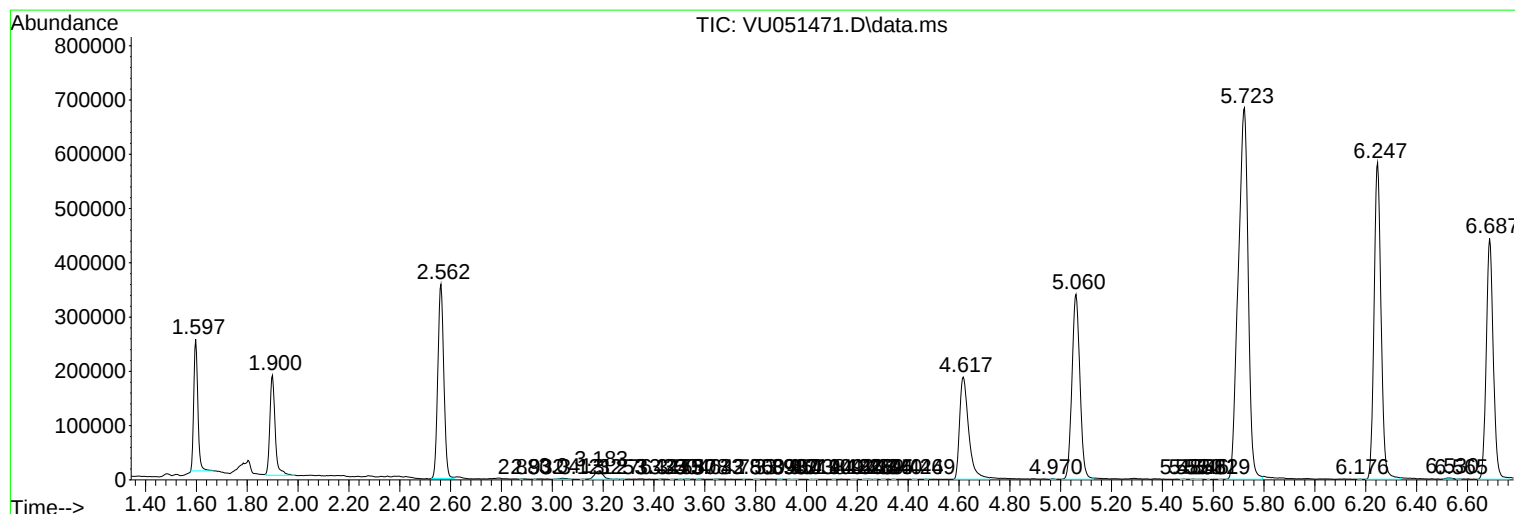

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051471.D
Acq On : 20 Oct 2022 14:53
Operator : JC/MD
Sample : N5180-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051471.D
Acq On : 20 Oct 2022 14:53
Operator : JC/MD
Sample : N5180-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------