

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051472.D
 Acq On : 20 Oct 2022 15:17
 Operator : JC/MD
 Sample : N5180-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M

Title : VOC Analysis

Signal : TIC: VU051472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	51	57	66	rBV	12008	15087	0.83%	0.110%
2	1.597	72	80	93	rBV	232241	278561	15.26%	2.038%
3	1.896	165	173	182	rBV	171464	231242	12.67%	1.692%
4	2.559	367	379	394	rBV	343559	561741	30.77%	4.110%
5	2.710	423	426	429	rVB2	606	418	0.02%	0.003%
6	2.761	438	442	444	rBV4	880	665	0.04%	0.005%
7	2.825	460	462	466	rVB2	619	321	0.02%	0.002%
8	2.883	477	480	484	rBV3	506	439	0.02%	0.003%
9	3.041	523	529	538	rVB4	2225	3276	0.18%	0.024%
10	3.112	547	551	555	rVV4	531	517	0.03%	0.004%
11	3.182	562	573	581	rVV5	3023	5832	0.32%	0.043%
12	3.356	622	627	629	rVV3	480	450	0.02%	0.003%
13	3.475	656	664	665	rBV2	487	591	0.03%	0.004%
14	3.510	670	675	677	rBV	408	392	0.02%	0.003%
15	3.632	708	713	719	rVB2	377	391	0.02%	0.003%
16	3.764	751	754	758	rVB2	413	340	0.02%	0.002%
17	3.800	758	765	769	rBV2	376	545	0.03%	0.004%
18	3.951	808	812	816	rBV2	388	375	0.02%	0.003%
19	4.202	884	890	896	rBV3	368	445	0.02%	0.003%
20	4.224	894	897	903	rVB3	366	352	0.02%	0.003%
21	4.314	920	925	927	rBV	377	327	0.02%	0.002%
22	4.475	969	975	982	rVB2	578	660	0.04%	0.005%
23	4.546	993	997	1001	rBV2	542	469	0.03%	0.003%
24	4.616	1007	1019	1046	rBV	184973	448338	24.56%	3.280%
25	5.060	1139	1157	1182	rBV	324357	718969	39.38%	5.260%
26	5.198	1195	1200	1205	rBV3	905	901	0.05%	0.007%
27	5.288	1219	1228	1235	rBV6	1156	1807	0.10%	0.013%
28	5.430	1269	1272	1280	rVB2	417	507	0.03%	0.004%
29	5.504	1292	1295	1300	rBV2	347	438	0.02%	0.003%
30	5.581	1316	1319	1324	rVV2	401	327	0.02%	0.002%
31	5.719	1337	1362	1384	rBV2	668024	1825739	100.00%	13.357%
32	6.044	1455	1463	1468	rVB4	743	1055	0.06%	0.008%
33	6.115	1480	1485	1490	rVV3	610	683	0.04%	0.005%
34	6.247	1511	1526	1544	rBV	563141	1073285	58.79%	7.852%
35	6.526	1605	1613	1625	rVB6	2807	4987	0.27%	0.036%
36	6.687	1648	1663	1685	rBV	427122	840403	46.03%	6.148%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051472.D
 Acq On : 20 Oct 2022 15:17
 Operator : JC/MD
 Sample : N5180-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

37	6.906	1726	1731	1732	rBV2	439	357	0.02%	0.003%
38	7.099	1788	1791	1795	rVB2	460	321	0.02%	0.002%
39	7.166	1807	1812	1813	rBV3	676	573	0.03%	0.004%
40	7.185	1813	1818	1827	rVB3	1957	2908	0.16%	0.021%
41	7.510	1916	1919	1922	rBV	585	368	0.02%	0.003%
42	7.562	1922	1935	1952	rBV	208722	367096	20.11%	2.686%
43	7.783	2000	2004	2006	rBV2	594	493	0.03%	0.004%
44	7.896	2023	2039	2059	rBV	779374	1353545	74.14%	9.902%
45	8.176	2114	2126	2143	rBV	149584	252815	13.85%	1.850%
46	8.391	2191	2193	2198	rVB3	690	525	0.03%	0.004%
47	8.427	2198	2204	2207	rBV3	528	520	0.03%	0.004%
48	8.472	2209	2218	2228	rVB3	4595	7842	0.43%	0.057%
49	8.542	2238	2240	2242	rBV3	864	490	0.03%	0.004%
50	8.632	2255	2268	2302	rBV2	539850	1031035	56.47%	7.543%
51	8.886	2344	2347	2351	rBV2	546	465	0.03%	0.003%
52	9.025	2388	2390	2394	rVB	607	396	0.02%	0.003%
53	9.147	2425	2428	2433	rVB3	579	473	0.03%	0.003%
54	9.169	2433	2435	2441	rBV3	524	543	0.03%	0.004%
55	9.262	2460	2464	2468	rBV	639	600	0.03%	0.004%
56	9.414	2498	2511	2532	rBV	810304	1350290	73.96%	9.879%
57	9.562	2551	2557	2564	rVB4	1028	1359	0.07%	0.010%
58	9.687	2592	2596	2598	rBV3	814	577	0.03%	0.004%
59	9.716	2603	2605	2611	rVB3	750	481	0.03%	0.004%
60	9.751	2611	2616	2619	rBV3	396	318	0.02%	0.002%
61	9.799	2628	2631	2634	rVB2	497	344	0.02%	0.003%
62	9.867	2646	2652	2655	rBV3	577	590	0.03%	0.004%
63	9.893	2655	2660	2663	rBV3	269	317	0.02%	0.002%
64	10.021	2696	2700	2705	rBV3	436	465	0.03%	0.003%
65	10.179	2746	2749	2753	rVB2	426	342	0.02%	0.003%
66	10.488	2838	2845	2851	rBV2	980	1040	0.06%	0.008%
67	10.635	2886	2891	2894	rVB2	385	359	0.02%	0.003%
68	10.754	2914	2928	2949	rBV	655175	1049051	57.46%	7.675%
69	10.893	2963	2971	2979	rVB4	3968	6255	0.34%	0.046%
70	10.957	2987	2991	2994	rBV2	346	325	0.02%	0.002%
71	11.092	3027	3033	3035	rBV4	735	751	0.04%	0.005%
72	11.237	3071	3078	3080	rBV2	253	316	0.02%	0.002%
73	11.253	3080	3083	3087	rVV3	539	401	0.02%	0.003%
74	11.349	3109	3113	3120	rVV3	525	551	0.03%	0.004%
75	11.471	3144	3151	3154	rBV3	655	783	0.04%	0.006%
76	11.526	3165	3168	3173	rVB2	416	386	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051472.D
 Acq On : 20 Oct 2022 15:17
 Operator : JC/MD
 Sample : N5180-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

77	11.725	3227	3230	3232	rBV2	635	429	0.02%	0.003%
78	11.745	3232	3236	3244	rVB4	1382	1335	0.07%	0.010%
79	11.809	3244	3256	3280	rBV	644918	1036575	56.78%	7.584%
80	12.066	3327	3336	3345	rBV2	10915	20302	1.11%	0.149%
81	12.192	3362	3375	3393	rBV	685247	1132183	62.01%	8.283%
82	12.426	3445	3448	3452	rBV2	401	334	0.02%	0.002%
83	12.767	3551	3554	3556	rBV2	663	398	0.02%	0.003%
84	12.876	3582	3588	3591	rBV3	478	622	0.03%	0.005%
85	13.066	3643	3647	3650	rVB2	498	361	0.02%	0.003%
86	13.085	3650	3653	3660	rBV4	365	434	0.02%	0.003%
87	13.156	3671	3675	3684	rBV2	1198	1448	0.08%	0.011%
88	13.224	3693	3696	3699	rVB4	920	621	0.03%	0.005%
89	13.320	3720	3726	3730	rBV4	622	759	0.04%	0.006%
90	13.423	3750	3758	3760	rBV3	726	1001	0.05%	0.007%
91	13.468	3769	3772	3775	rBV2	482	340	0.02%	0.002%
92	13.844	3885	3889	3901	rVB7	3416	4719	0.26%	0.035%
93	13.925	3912	3914	3921	rVB3	534	500	0.03%	0.004%
94	14.095	3958	3967	3977	rBV3	2311	3731	0.20%	0.027%
95	14.269	4019	4021	4026	rVB3	822	601	0.03%	0.004%
96	14.294	4027	4029	4033	rBV3	495	400	0.02%	0.003%
97	14.336	4036	4042	4046	rVV6	2018	2563	0.14%	0.019%
98	14.761	4172	4174	4176	rBV	773	347	0.02%	0.003%
99	14.886	4209	4213	4216	rBV2	651	571	0.03%	0.004%
100	15.246	4321	4325	4327	rBV3	849	688	0.04%	0.005%



Sum of corrected areas: 13668803

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051472.D
Acq On : 20 Oct 2022 15:17
Operator : JC/MD
Sample : N5180-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

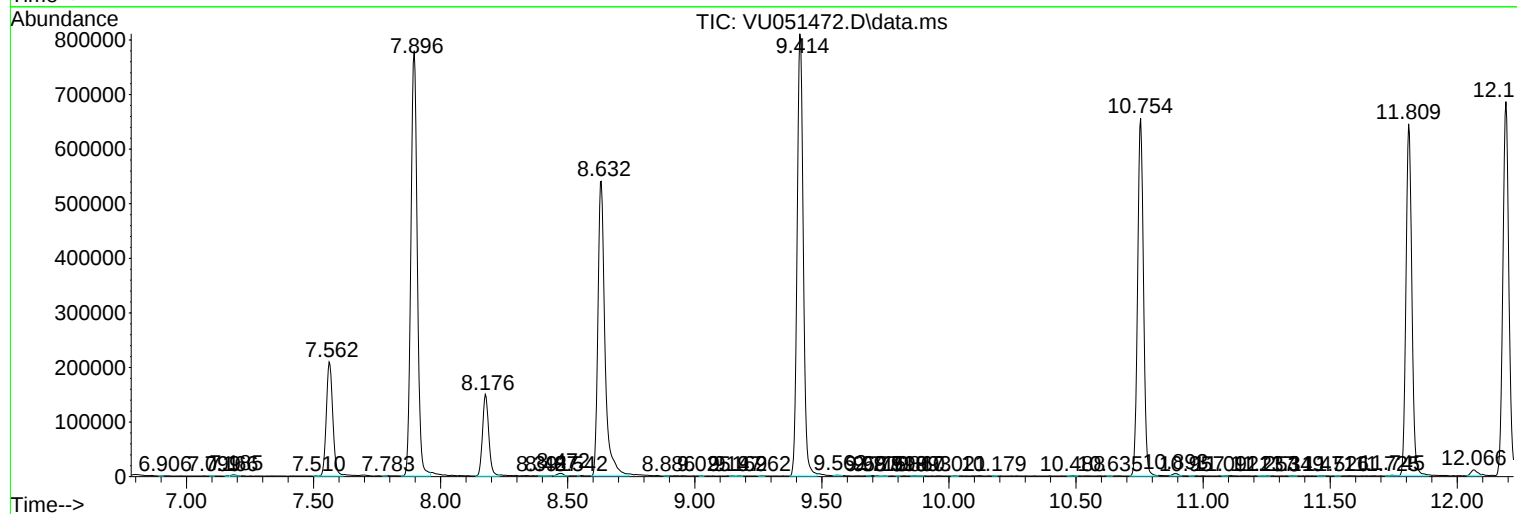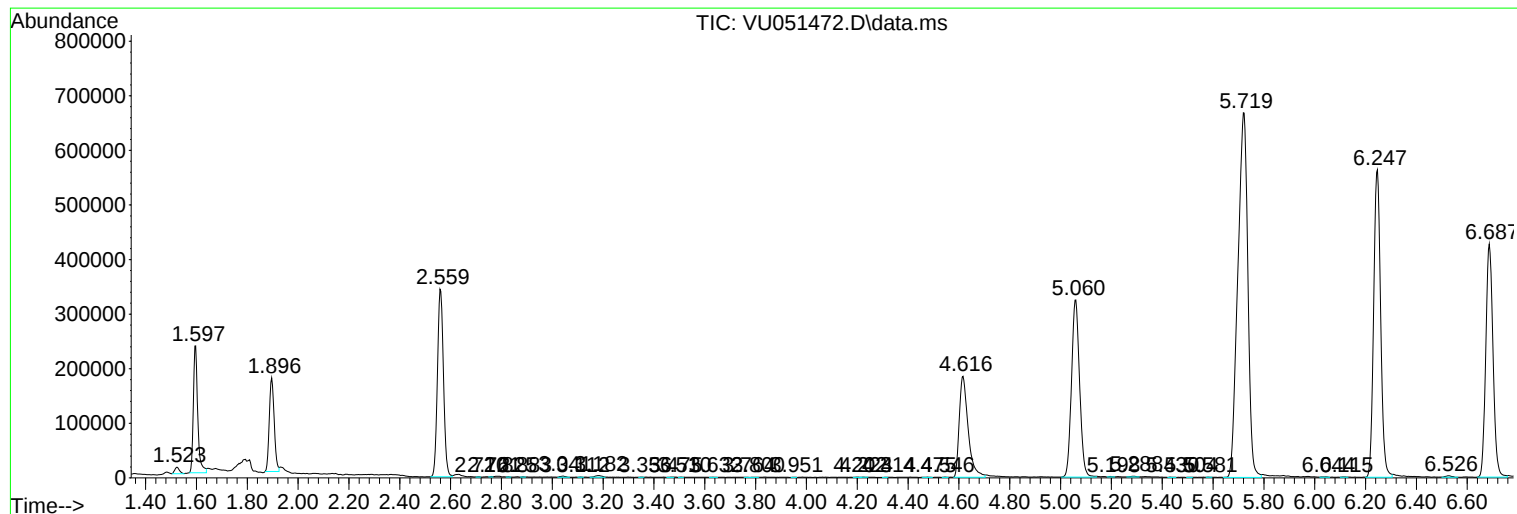

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051472.D
Acq On : 20 Oct 2022 15:17
Operator : JC/MD
Sample : N5180-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051472.D
Acq On : 20 Oct 2022 15:17
Operator : JC/MD
Sample : N5180-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
