

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051473.D
 Acq On : 20 Oct 2022 15:41
 Operator : JC/MD
 Sample : N5180-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M

Title : VOC Analysis

Signal : TIC: VU051473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	249919	281649	15.10%	2.046%
2	1.899	166	174	196	rVB	181537	262520	14.08%	1.907%
3	2.562	367	380	394	rBV	355415	581768	31.20%	4.227%
4	2.887	480	481	486	rVB2	506	341	0.02%	0.002%
5	2.922	486	492	495	rBV4	772	682	0.04%	0.005%
6	2.961	501	504	510	rBV4	545	516	0.03%	0.004%
7	3.044	523	530	538	rVB4	1567	2509	0.13%	0.018%
8	3.179	562	572	587	rBV6	2746	6400	0.34%	0.046%
9	3.243	587	592	598	rVB2	565	633	0.03%	0.005%
10	3.272	598	601	607	rBV2	337	322	0.02%	0.002%
11	3.324	611	617	619	rVB3	445	426	0.02%	0.003%
12	3.350	619	625	628	rBV3	751	851	0.05%	0.006%
13	3.639	713	715	720	rVV2	401	362	0.02%	0.003%
14	3.665	720	723	730	rVV2	520	501	0.03%	0.004%
15	3.758	748	752	756	rBV2	301	338	0.02%	0.002%
16	3.780	756	759	764	rVB3	382	337	0.02%	0.002%
17	4.092	853	856	860	rVV2	414	347	0.02%	0.003%
18	4.169	876	880	883	rVV2	527	452	0.02%	0.003%
19	4.346	930	935	937	rBV	451	343	0.02%	0.002%
20	4.526	988	991	997	rVB3	406	378	0.02%	0.003%
21	4.616	1007	1019	1053	rBV	185995	464276	24.90%	3.373%
22	4.890	1100	1104	1109	rVB2	460	521	0.03%	0.004%
23	5.060	1140	1157	1184	rVV	338452	738515	39.60%	5.365%
24	5.292	1220	1229	1235	rBV6	1781	2861	0.15%	0.021%
25	5.636	1331	1336	1340	rVB2	393	368	0.02%	0.003%
26	5.722	1340	1363	1392	rBV2	683307	1864825	100.00%	13.548%
27	5.948	1430	1433	1435	rBV4	569	438	0.02%	0.003%
28	6.018	1452	1455	1458	rBV3	494	378	0.02%	0.003%
29	6.073	1469	1472	1478	rVB2	453	440	0.02%	0.003%
30	6.105	1478	1482	1486	rBV3	727	704	0.04%	0.005%
31	6.247	1510	1526	1547	rBV	568326	1077643	57.79%	7.829%
32	6.430	1582	1583	1590	rVB3	719	515	0.03%	0.004%
33	6.484	1596	1600	1604	rVB3	594	599	0.03%	0.004%
34	6.523	1604	1612	1619	rBV10	2482	4111	0.22%	0.030%
35	6.587	1628	1632	1634	rBV2	320	321	0.02%	0.002%
36	6.620	1639	1642	1645	rVB2	672	431	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051473.D
 Acq On : 20 Oct 2022 15:41
 Operator : JC/MD
 Sample : N5180-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

37	6.687	1649	1663	1686	rBV	432764	851585	45.67%	6.187%
38	6.857	1712	1716	1722	rVB2	916	1038	0.06%	0.008%
39	7.160	1804	1810	1811	rBV	596	390	0.02%	0.003%
40	7.185	1814	1818	1819	rBV2	1291	887	0.05%	0.006%
41	7.446	1896	1899	1905	rVB2	452	381	0.02%	0.003%
42	7.565	1923	1936	1953	rBV	209542	374281	20.07%	2.719%
43	7.693	1973	1976	1984	rVV5	1370	1601	0.09%	0.012%
44	7.832	2016	2019	2021	rBV	494	334	0.02%	0.002%
45	7.896	2025	2039	2063	rBV	778443	1364427	73.17%	9.913%
46	8.176	2115	2126	2148	rBV	149220	256233	13.74%	1.862%
47	8.340	2175	2177	2186	rVB4	646	862	0.05%	0.006%
48	8.427	2201	2204	2206	rBV3	674	375	0.02%	0.003%
49	8.472	2208	2218	2227	rVB2	6108	10884	0.58%	0.079%
50	8.549	2239	2242	2245	rBV4	675	514	0.03%	0.004%
51	8.632	2254	2268	2302	rBV2	532634	1026986	55.07%	7.461%
52	8.838	2329	2332	2337	rVB4	635	483	0.03%	0.004%
53	9.015	2384	2387	2389	rBV2	545	353	0.02%	0.003%
54	9.031	2389	2392	2395	rBV2	904	790	0.04%	0.006%
55	9.092	2409	2411	2415	rVB2	501	336	0.02%	0.002%
56	9.166	2432	2434	2438	rVB2	624	331	0.02%	0.002%
57	9.195	2438	2443	2446	rBV3	603	440	0.02%	0.003%
58	9.414	2497	2511	2535	rBV	807429	1339025	71.80%	9.728%
59	9.619	2572	2575	2578	rVB3	630	435	0.02%	0.003%
60	9.655	2583	2586	2591	rVB2	450	338	0.02%	0.002%
61	9.693	2591	2598	2603	rBV3	944	1233	0.07%	0.009%
62	9.899	2656	2662	2665	rBV3	464	544	0.03%	0.004%
63	9.928	2669	2671	2678	rVV2	306	384	0.02%	0.003%
64	10.025	2697	2701	2703	rBV2	504	423	0.02%	0.003%
65	10.095	2716	2723	2725	rBV2	598	658	0.04%	0.005%
66	10.127	2731	2733	2736	rVB3	597	319	0.02%	0.002%
67	10.147	2736	2739	2742	rVB	543	334	0.02%	0.002%
68	10.169	2742	2746	2749	rBV2	418	348	0.02%	0.003%
69	10.369	2805	2808	2817	rVB	633	716	0.04%	0.005%
70	10.603	2877	2881	2885	rVV3	659	531	0.03%	0.004%
71	10.754	2914	2928	2956	rBV	647531	1051868	56.41%	7.642%
72	10.889	2963	2970	2982	rVB2	6818	10872	0.58%	0.079%
73	10.938	2983	2985	2992	rVB2	527	400	0.02%	0.003%
74	11.098	3027	3035	3039	rBV4	652	905	0.05%	0.007%
75	11.150	3049	3051	3058	rVB2	730	680	0.04%	0.005%
76	11.192	3058	3064	3067	rBV2	588	605	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051473.D
 Acq On : 20 Oct 2022 15:41
 Operator : JC/MD
 Sample : N5180-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

77	11.478	3146	3153	3156	rBV3	981	1100	0.06%	0.008%
78	11.748	3229	3237	3241	rBV4	1579	1769	0.09%	0.013%
79	11.809	3243	3256	3280	rBV	624502	1001711	53.72%	7.278%
80	12.063	3327	3335	3350	rBV3	8670	17230	0.92%	0.125%
81	12.192	3361	3375	3401	rBV	681736	1124344	60.29%	8.169%
82	12.561	3487	3490	3494	rBV3	538	499	0.03%	0.004%
83	12.684	3525	3528	3533	rBV2	547	531	0.03%	0.004%
84	12.732	3540	3543	3546	rVV3	626	432	0.02%	0.003%
85	12.774	3549	3556	3563	rVB3	1825	2676	0.14%	0.019%
86	12.832	3569	3574	3581	rBV2	540	619	0.03%	0.004%
87	12.925	3600	3603	3606	rVB2	625	398	0.02%	0.003%
88	12.967	3613	3616	3620	rVB2	489	327	0.02%	0.002%
89	13.021	3630	3633	3639	rVB3	588	571	0.03%	0.004%
90	13.230	3695	3698	3708	rVB3	1313	1539	0.08%	0.011%
91	13.317	3722	3725	3729	rBV3	421	382	0.02%	0.003%
92	13.494	3777	3780	3784	rBV	468	339	0.02%	0.002%
93	13.610	3813	3816	3820	rBV2	435	388	0.02%	0.003%
94	13.848	3886	3890	3898	rVB5	1609	2277	0.12%	0.017%
95	13.989	3932	3934	3941	rBV3	338	379	0.02%	0.003%
96	14.330	4035	4040	4041	rBV2	1615	1150	0.06%	0.008%
97	14.655	4138	4141	4149	rBV2	700	990	0.05%	0.007%
98	15.201	4308	4311	4314	rBV4	632	586	0.03%	0.004%
99	15.873	4517	4520	4523	rBV3	906	776	0.04%	0.006%
100	15.909	4528	4531	4533	rBV4	842	495	0.03%	0.004%




Sum of corrected areas: 13764258

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051473.D
Acq On : 20 Oct 2022 15:41
Operator : JC/MD
Sample : N5180-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

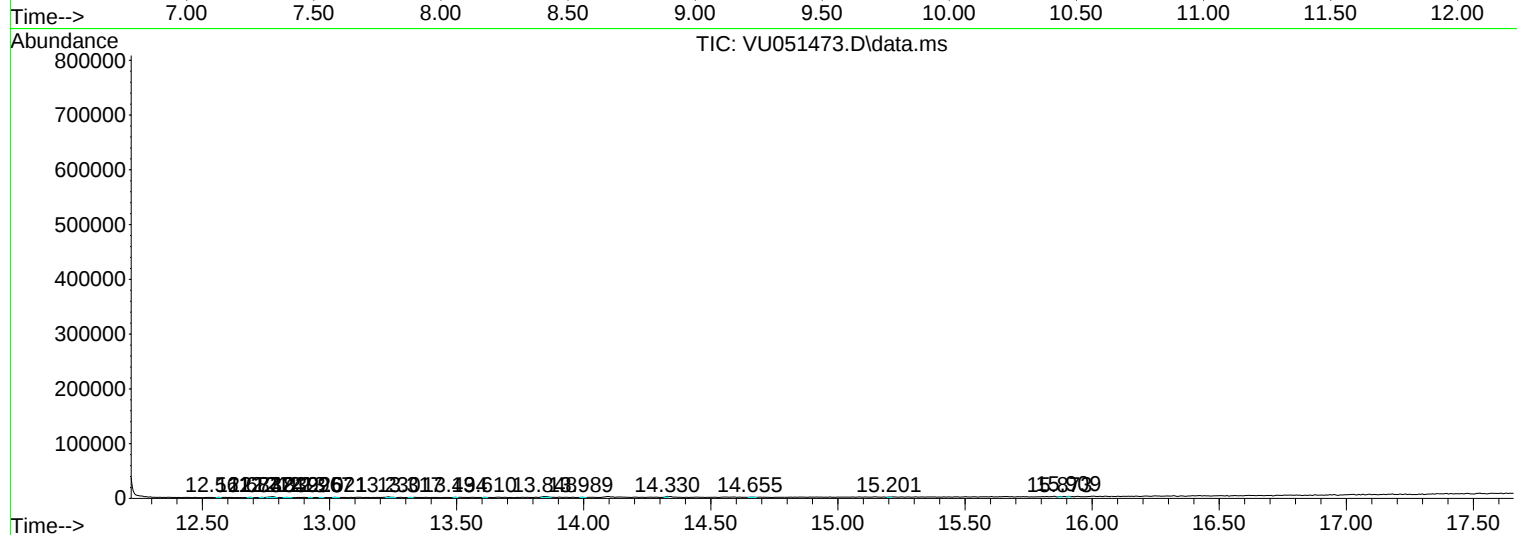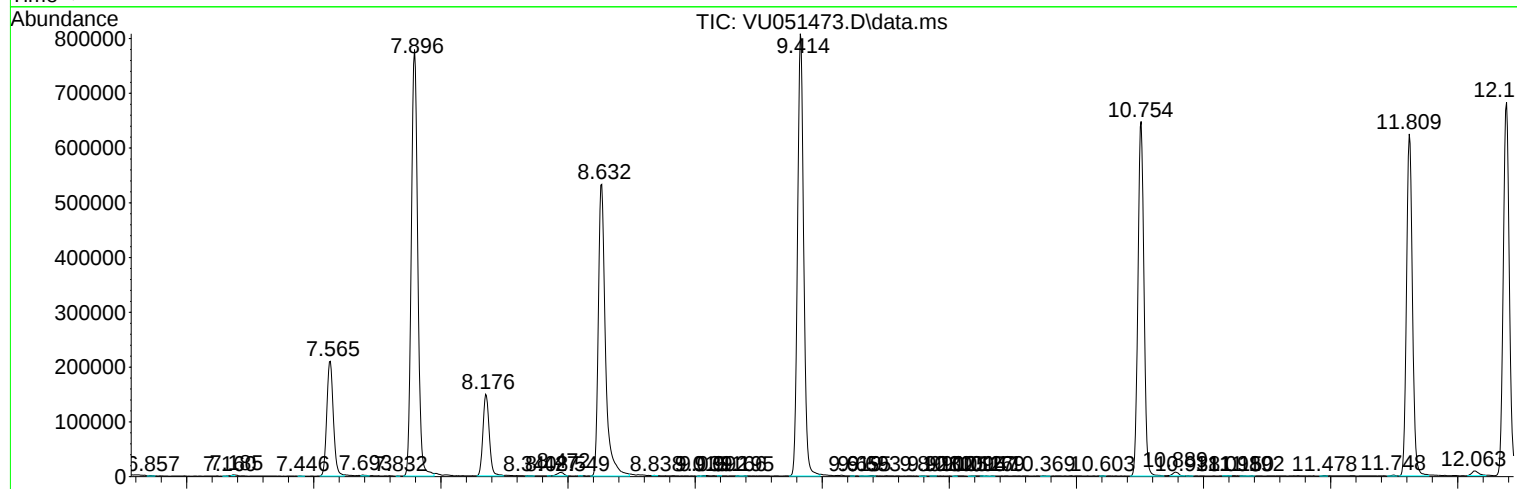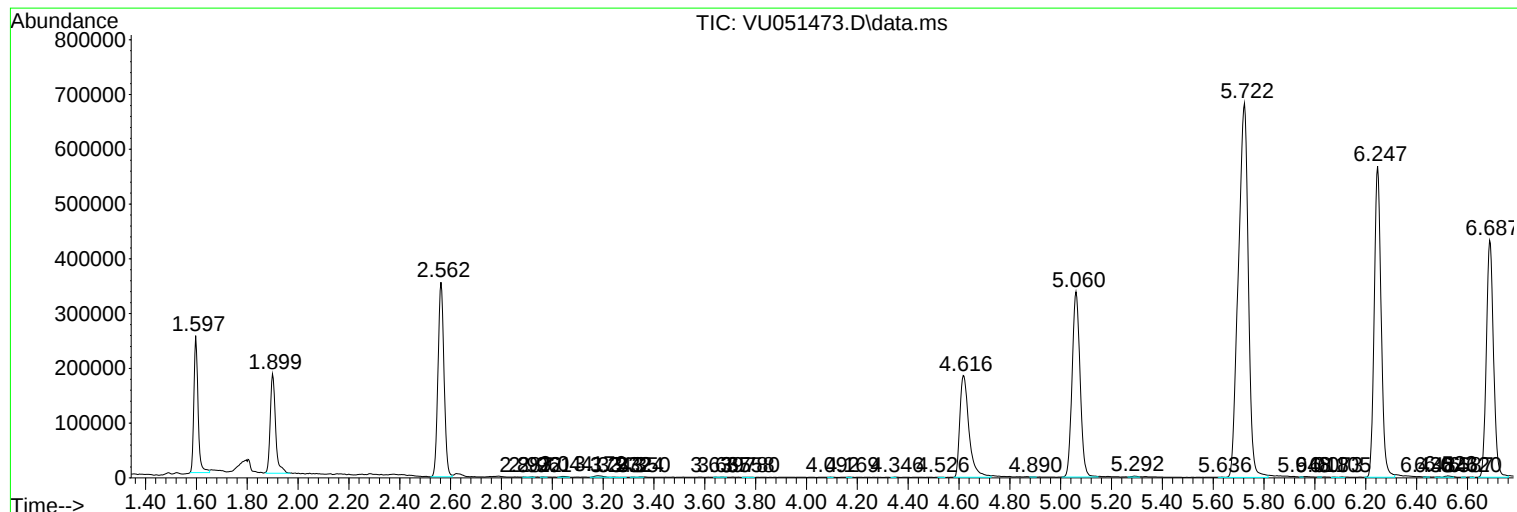

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051473.D
Acq On : 20 Oct 2022 15:41
Operator : JC/MD
Sample : N5180-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051473.D
Acq On : 20 Oct 2022 15:41
Operator : JC/MD
Sample : N5180-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc