

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051474.D
 Acq On : 20 Oct 2022 16:05
 Operator : JC/MD
 Sample : N5180-05DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M

Title : VOC Analysis

Signal : TIC: VU051474.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	99	rBV	252383	298724	13.96%	1.834%
2	1.896	165	173	199	rVB	184621	270421	12.64%	1.660%
3	2.562	367	380	396	rBV	372416	610946	28.56%	3.751%
4	2.755	437	440	442	rBV2	580	340	0.02%	0.002%
5	2.835	461	465	467	rBV3	587	499	0.02%	0.003%
6	3.041	519	529	543	rVB5	7521	15780	0.74%	0.097%
7	3.186	558	574	589	rVB2	10245	24286	1.14%	0.149%
8	3.298	603	609	612	rBV	359	312	0.01%	0.002%
9	3.350	622	625	628	rBV2	499	316	0.01%	0.002%
10	3.456	653	658	660	rBV	360	327	0.02%	0.002%
11	3.520	675	678	684	rVB2	485	484	0.02%	0.003%
12	3.559	684	690	692	rBV2	554	607	0.03%	0.004%
13	3.765	749	754	758	rBV2	253	305	0.01%	0.002%
14	4.337	929	932	938	rBV2	412	425	0.02%	0.003%
15	4.411	949	955	957	rBV	386	370	0.02%	0.002%
16	4.617	1006	1019	1058	rBV	188216	471019	22.02%	2.892%
17	4.784	1069	1071	1073	rBV	650	368	0.02%	0.002%
18	5.060	1136	1157	1183	rBV	340753	761092	35.58%	4.673%
19	5.276	1219	1224	1225	rBV3	977	713	0.03%	0.004%
20	5.330	1237	1241	1243	rBV2	695	475	0.02%	0.003%
21	5.366	1250	1252	1254	rBV	650	439	0.02%	0.003%
22	5.427	1267	1271	1275	rBV2	434	432	0.02%	0.003%
23	5.555	1308	1311	1318	rVB2	385	348	0.02%	0.002%
24	5.723	1340	1363	1375	rBV2	705679	1945833	90.95%	11.946%
25	5.964	1435	1438	1441	rBV3	848	539	0.03%	0.003%
26	6.038	1459	1461	1464	rBV2	556	345	0.02%	0.002%
27	6.070	1469	1471	1475	rVB3	544	345	0.02%	0.002%
28	6.134	1489	1491	1497	rVB3	609	396	0.02%	0.002%
29	6.192	1503	1509	1511	rBV3	456	390	0.02%	0.002%
30	6.247	1511	1526	1555	rBV	605629	1153637	53.92%	7.082%
31	6.530	1604	1614	1625	rVB9	3260	6542	0.31%	0.040%
32	6.687	1649	1663	1683	rBV	447708	871116	40.72%	5.348%
33	6.887	1721	1725	1730	rBV4	514	524	0.02%	0.003%
34	7.018	1761	1766	1767	rBV	419	319	0.01%	0.002%
35	7.099	1787	1791	1794	rBV2	525	365	0.02%	0.002%
36	7.144	1800	1805	1808	rBV3	371	299	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051474.D
 Acq On : 20 Oct 2022 16:05
 Operator : JC/MD
 Sample : N5180-05DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

37	7.186	1809	1818	1833	rVB8	2424	5027	0.23%	0.031%
38	7.562	1922	1935	1956	rBV	214434	381823	17.85%	2.344%
39	7.687	1972	1974	1987	rVB5	1781	2471	0.12%	0.015%
40	7.793	2000	2007	2011	rVV5	1001	1391	0.07%	0.009%
41	7.896	2025	2039	2062	rBV	821830	1421706	66.45%	8.728%
42	8.176	2112	2126	2144	rBV	154383	262916	12.29%	1.614%
43	8.395	2192	2194	2198	rVB3	607	396	0.02%	0.002%
44	8.469	2210	2217	2228	rVB4	3966	7077	0.33%	0.043%
45	8.510	2228	2230	2234	rVB2	775	569	0.03%	0.003%
46	8.536	2234	2238	2239	rBV	450	304	0.01%	0.002%
47	8.552	2239	2243	2245	rBV2	500	449	0.02%	0.003%
48	8.632	2248	2268	2303	rBV2	553791	1051999	49.17%	6.458%
49	8.909	2351	2354	2355	rBV	531	285	0.01%	0.002%
50	9.076	2403	2406	2410	rVB3	633	551	0.03%	0.003%
51	9.205	2443	2446	2449	rBV2	488	319	0.01%	0.002%
52	9.234	2449	2455	2461	rVV	644	750	0.04%	0.005%
53	9.279	2465	2469	2472	rBV2	387	347	0.02%	0.002%
54	9.304	2472	2477	2483	rBV3	514	670	0.03%	0.004%
55	9.414	2498	2511	2516	rBV	894064	1509340	70.55%	9.266%
56	9.665	2586	2589	2591	rBV2	404	317	0.01%	0.002%
57	9.690	2595	2597	2598	rBV2	540	288	0.01%	0.002%
58	9.761	2617	2619	2625	rVB2	365	291	0.01%	0.002%
59	9.890	2656	2659	2662	rVV2	506	367	0.02%	0.002%
60	9.909	2662	2665	2667	rVV2	456	312	0.01%	0.002%
61	9.996	2688	2692	2694	rBV2	393	322	0.02%	0.002%
62	10.105	2720	2726	2728	rBV3	806	695	0.03%	0.004%
63	10.272	2772	2778	2782	rVB2	627	531	0.02%	0.003%
64	10.333	2791	2797	2801	rVB3	348	436	0.02%	0.003%
65	10.485	2837	2844	2847	rBV2	612	769	0.04%	0.005%
66	10.684	2902	2906	2910	rVB2	514	363	0.02%	0.002%
67	10.755	2914	2928	2949	rBV	671838	1087882	50.85%	6.679%
68	10.886	2963	2969	2977	rVB4	4636	6676	0.31%	0.041%
69	11.005	3002	3006	3010	rBV2	566	523	0.02%	0.003%
70	11.050	3016	3020	3023	rVB2	374	289	0.01%	0.002%
71	11.092	3023	3033	3035	rBV4	739	1082	0.05%	0.007%
72	11.237	3072	3078	3079	rBV2	363	367	0.02%	0.002%
73	11.269	3084	3088	3091	rBV3	375	295	0.01%	0.002%
74	11.414	3128	3133	3140	rBV5	740	931	0.04%	0.006%
75	11.472	3148	3151	3155	rVV2	678	506	0.02%	0.003%
76	11.620	3194	3197	3200	rBV	426	324	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051474.D
 Acq On : 20 Oct 2022 16:05
 Operator : JC/MD
 Sample : N5180-05DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

77	11.690	3216	3219	3226	rVB3	505	332	0.02%	0.002%
78	11.745	3226	3236	3245	rBV	45279	70876	3.31%	0.435%
79	11.812	3245	3257	3284	rVV2	761639	1763103	82.41%	10.824%
80	12.076	3330	3339	3345	rBV7	1687	3223	0.15%	0.020%
81	12.195	3361	3376	3401	rBV2	925995	2139374	100.00%	13.134%
82	12.555	3485	3488	3491	rVB2	633	415	0.02%	0.003%
83	12.771	3547	3555	3560	rBV4	1141	1557	0.07%	0.010%
84	12.928	3601	3604	3607	rBV3	353	319	0.01%	0.002%
85	13.118	3659	3663	3667	rBV4	386	436	0.02%	0.003%
86	13.308	3716	3722	3724	rBV3	417	512	0.02%	0.003%
87	13.562	3798	3801	3805	rBV3	354	292	0.01%	0.002%
88	13.581	3805	3807	3813	rVB2	434	320	0.01%	0.002%
89	13.664	3826	3833	3835	rBV3	755	815	0.04%	0.005%
90	13.771	3861	3866	3868	rBV2	627	645	0.03%	0.004%
91	13.841	3877	3888	3904	rBV2	51450	87065	4.07%	0.535%
92	13.947	3917	3921	3928	rVB3	722	783	0.04%	0.005%
93	14.060	3953	3956	3960	rBV3	1058	837	0.04%	0.005%
94	14.092	3962	3966	3972	rVV3	1313	1770	0.08%	0.011%
95	14.291	4024	4028	4029	rBV	522	370	0.02%	0.002%
96	14.330	4032	4040	4057	rVB3	13208	21662	1.01%	0.133%
97	14.565	4110	4113	4115	rBV	666	479	0.02%	0.003%
98	14.697	4150	4154	4158	rBV4	834	800	0.04%	0.005%
99	15.166	4298	4300	4302	rBV	664	375	0.02%	0.002%
100	15.346	4354	4356	4360	rVB3	1087	620	0.03%	0.004%




Sum of corrected areas: 16288614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051474.D
Acq On : 20 Oct 2022 16:05
Operator : JC/MD
Sample : N5180-05DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

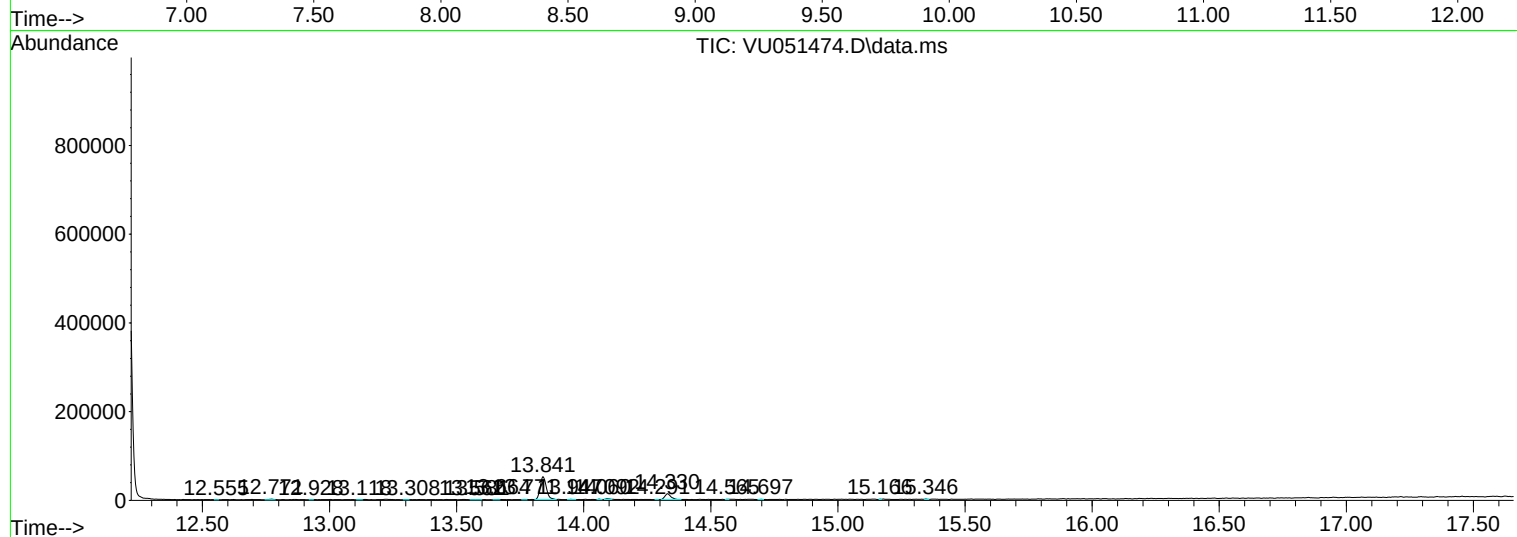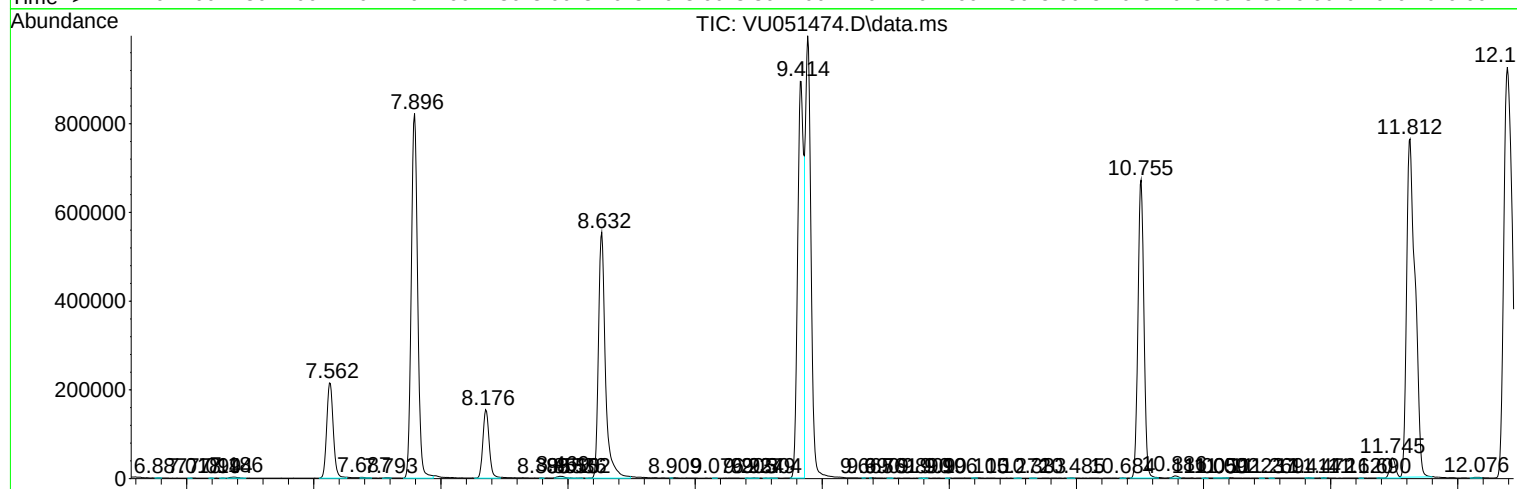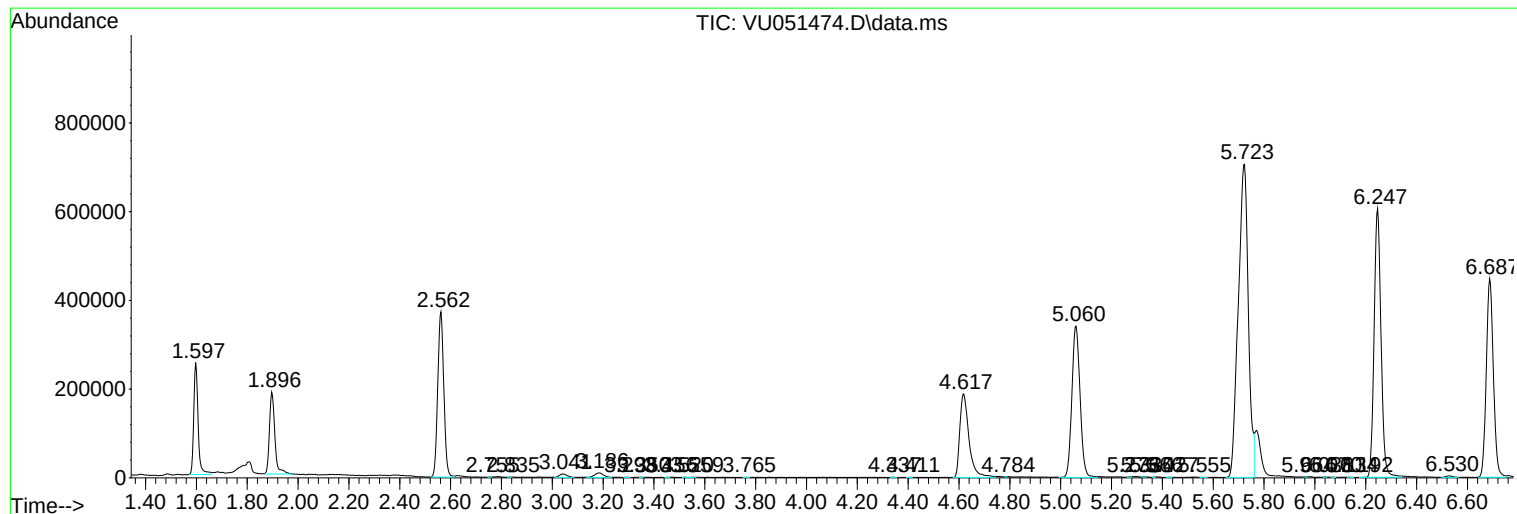

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051474.D
Acq On : 20 Oct 2022 16:05
Operator : JC/MD
Sample : N5180-05DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051474.D
Acq On : 20 Oct 2022 16:05
Operator : JC/MD
Sample : N5180-05DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------