

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051475.D
 Acq On : 20 Oct 2022 16:29
 Operator : JC/MD
 Sample : N5180-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M

Title : VOC Analysis

Signal : TIC: VU051475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	72	80	91	rBV	246402	283149	2.87%	0.876%
2	1.900	166	174	195	rVB	185351	264255	2.68%	0.817%
3	2.562	368	380	395	rBV	369869	603945	6.12%	1.867%
4	2.871	473	476	480	rBV2	572	444	0.00%	0.001%
5	3.044	522	530	540	rBV2	4304	7108	0.07%	0.022%
6	3.179	559	572	587	rVB	10114	22346	0.23%	0.069%
7	3.266	595	599	602	rBV2	451	382	0.00%	0.001%
8	3.331	617	619	623	rVB	527	346	0.00%	0.001%
9	3.414	639	645	646	rBV	359	322	0.00%	0.001%
10	3.462	655	660	663	rBV2	472	420	0.00%	0.001%
11	3.662	718	722	725	rBV2	455	358	0.00%	0.001%
12	3.713	732	738	745	rVB2	443	655	0.01%	0.002%
13	3.761	750	753	757	rVB2	530	333	0.00%	0.001%
14	3.880	783	790	793	rBV2	377	385	0.00%	0.001%
15	3.922	797	803	807	rBV3	424	459	0.00%	0.001%
16	3.996	819	826	828	rBV2	330	322	0.00%	0.001%
17	4.060	842	846	849	rVB3	414	310	0.00%	0.001%
18	4.080	849	852	855	rVB	548	320	0.00%	0.001%
19	4.260	905	908	915	rVV2	354	334	0.00%	0.001%
20	4.453	965	968	973	rVB2	425	340	0.00%	0.001%
21	4.485	973	978	981	rBV	438	438	0.00%	0.001%
22	4.523	981	990	991	rBV3	1787	1874	0.02%	0.006%
23	4.617	1004	1019	1063	rBV	187046	470175	4.76%	1.454%
24	4.845	1088	1090	1093	rBV3	645	387	0.00%	0.001%
25	4.974	1127	1130	1138	rBV3	578	745	0.01%	0.002%
26	5.060	1140	1157	1181	rBV	339795	753573	7.63%	2.330%
27	5.324	1235	1239	1240	rBV3	570	416	0.00%	0.001%
28	5.372	1250	1254	1255	rBV3	1023	767	0.01%	0.002%
29	5.523	1289	1301	1314	rVB5	3530	7420	0.08%	0.023%
30	5.610	1322	1328	1332	rVB	708	696	0.01%	0.002%
31	5.639	1332	1337	1340	rBV	440	417	0.00%	0.001%
32	5.723	1340	1363	1371	rBV2	700433	1893129	19.17%	5.854%
33	5.980	1441	1443	1445	rVB3	1092	506	0.01%	0.002%
34	6.035	1454	1460	1466	rVV6	1133	1310	0.01%	0.004%
35	6.131	1488	1490	1493	rVB	601	320	0.00%	0.001%
36	6.247	1510	1526	1560	rBV	626548	1199590	12.15%	3.709%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051475.D
 Acq On : 20 Oct 2022 16:29
 Operator : JC/MD
 Sample : N5180-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

37	6.494	1599	1603	1606	rBV3	393	305	0.00%	0.001%
38	6.517	1606	1610	1612	rBV2	2294	1904	0.02%	0.006%
39	6.594	1631	1634	1636	rBV3	609	381	0.00%	0.001%
40	6.687	1649	1663	1682	rBV	443734	866997	8.78%	2.681%
41	6.890	1722	1726	1728	rBV2	460	332	0.00%	0.001%
42	6.935	1736	1740	1742	rBV2	462	378	0.00%	0.001%
43	7.022	1764	1767	1770	rBV	524	309	0.00%	0.001%
44	7.099	1788	1791	1796	rBV	352	301	0.00%	0.001%
45	7.183	1811	1817	1819	rBV5	1769	1784	0.02%	0.006%
46	7.247	1832	1837	1842	rVB2	459	533	0.01%	0.002%
47	7.279	1842	1847	1848	rBV2	363	309	0.00%	0.001%
48	7.379	1871	1878	1882	rBV2	334	405	0.00%	0.001%
49	7.507	1910	1918	1920	rBV2	267	328	0.00%	0.001%
50	7.562	1920	1935	1958	rBV	218475	384820	3.90%	1.190%
51	7.729	1985	1987	1992	rVB2	555	413	0.00%	0.001%
52	7.896	2025	2039	2059	rBV	831340	1434063	14.52%	4.434%
53	8.121	2104	2109	2114	rBV3	355	360	0.00%	0.001%
54	8.176	2114	2126	2143	rBV	152611	257936	2.61%	0.798%
55	8.472	2209	2218	2226	rVV2	5022	8693	0.09%	0.027%
56	8.549	2237	2242	2247	rBV4	1193	1249	0.01%	0.004%
57	8.629	2253	2267	2307	rBV2	538893	1037618	10.51%	3.208%
58	8.851	2333	2336	2339	rBV2	685	374	0.00%	0.001%
59	8.973	2372	2374	2381	rVB4	720	523	0.01%	0.002%
60	9.022	2386	2389	2391	rBV2	569	313	0.00%	0.001%
61	9.073	2402	2405	2411	rVB	465	350	0.00%	0.001%
62	9.186	2436	2440	2443	rBV3	482	322	0.00%	0.001%
63	9.208	2443	2447	2450	rBV3	447	405	0.00%	0.001%
64	9.443	2498	2520	2558	rBV2	5183186	9874586	100.00%	30.532%
65	9.684	2592	2595	2597	rBV	717	564	0.01%	0.002%
66	9.787	2623	2627	2631	rBV5	491	373	0.00%	0.001%
67	9.928	2667	2671	2678	rVB4	898	1314	0.01%	0.004%
68	10.002	2692	2694	2698	rVB3	516	330	0.00%	0.001%
69	10.044	2705	2707	2716	rVB3	561	640	0.01%	0.002%
70	10.096	2717	2723	2727	rBV2	935	937	0.01%	0.003%
71	10.125	2727	2732	2737	rVB3	597	775	0.01%	0.002%
72	10.198	2749	2755	2759	rBV3	718	625	0.01%	0.002%
73	10.224	2759	2763	2766	rVB2	507	336	0.00%	0.001%
74	10.289	2780	2783	2788	rVB	371	308	0.00%	0.001%
75	10.317	2788	2792	2795	rBV2	508	356	0.00%	0.001%
76	10.340	2795	2799	2802	rVB3	389	313	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051475.D
 Acq On : 20 Oct 2022 16:29
 Operator : JC/MD
 Sample : N5180-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0KX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

77	10.475	2838	2841	2843	rBV2	486	339	0.00%	0.001%
78	10.552	2860	2865	2867	rBV2	315	311	0.00%	0.001%
79	10.755	2915	2928	2946	rBV	666494	1072407	10.86%	3.316%
80	10.893	2960	2971	2981	rBV3	5400	9005	0.09%	0.028%
81	10.989	2995	3001	3004	rBV2	629	578	0.01%	0.002%
82	11.198	3060	3066	3070	rVB3	646	671	0.01%	0.002%
83	11.350	3108	3113	3117	rBV2	379	426	0.00%	0.001%
84	11.600	3188	3191	3195	rBV	565	552	0.01%	0.002%
85	11.742	3224	3235	3245	rBV	236290	377323	3.82%	1.167%
86	11.832	3245	3263	3283	rVB2	2189669	4659390	47.19%	14.407%
87	12.079	3334	3340	3342	rBV4	837	885	0.01%	0.003%
88	12.208	3361	3380	3408	rBV2	3168079	6146882	62.25%	19.006%
89	12.456	3454	3457	3459	rBV2	479	379	0.00%	0.001%
90	12.768	3551	3554	3556	rBV3	710	533	0.01%	0.002%
91	12.864	3581	3584	3587	rBV2	566	352	0.00%	0.001%
92	12.915	3597	3600	3605	rBV2	497	495	0.01%	0.002%
93	12.973	3612	3618	3619	rBV3	1738	1449	0.01%	0.004%
94	13.227	3691	3697	3706	rVB5	1689	2602	0.03%	0.008%
95	13.838	3875	3887	3905	rBV	323139	533474	5.40%	1.650%
96	14.086	3959	3964	3974	rVB6	2271	3063	0.03%	0.009%
97	14.327	4029	4039	4054	rBV	74025	122516	1.24%	0.379%
98	14.549	4105	4108	4110	rBV	858	522	0.01%	0.002%
99	15.015	4250	4253	4256	rBV2	752	534	0.01%	0.002%
100	15.996	4554	4558	4569	rBV9	3336	5215	0.05%	0.016%




Sum of corrected areas: 32341361

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051475.D
Acq On : 20 Oct 2022 16:29
Operator : JC/MD
Sample : N5180-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

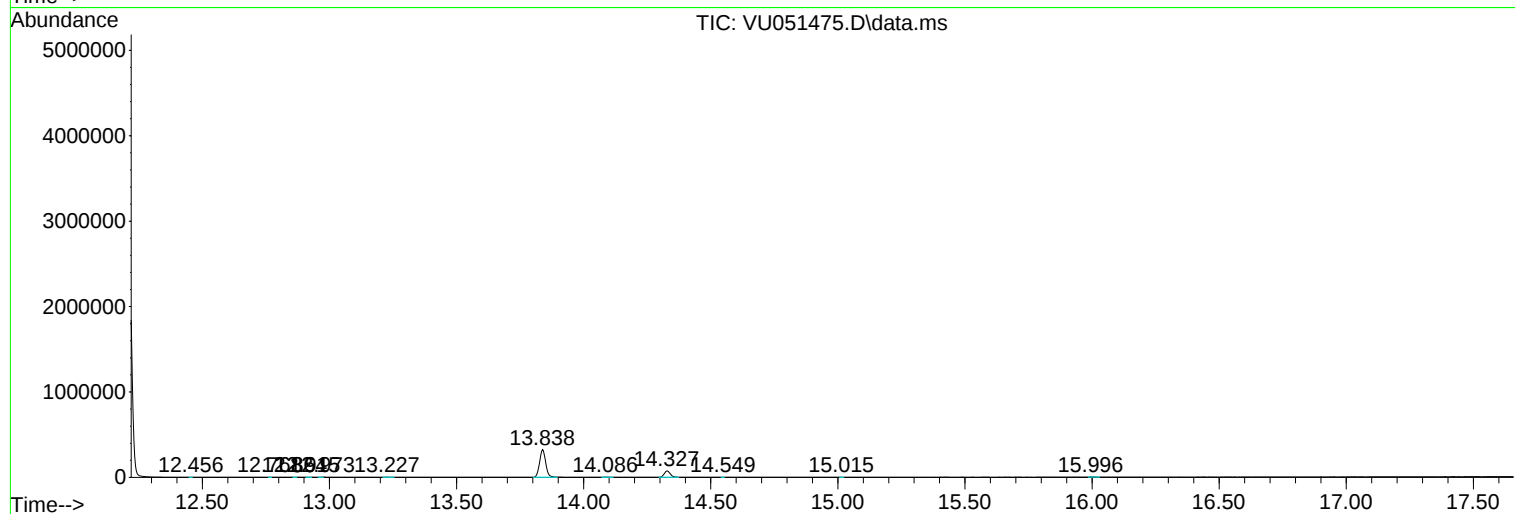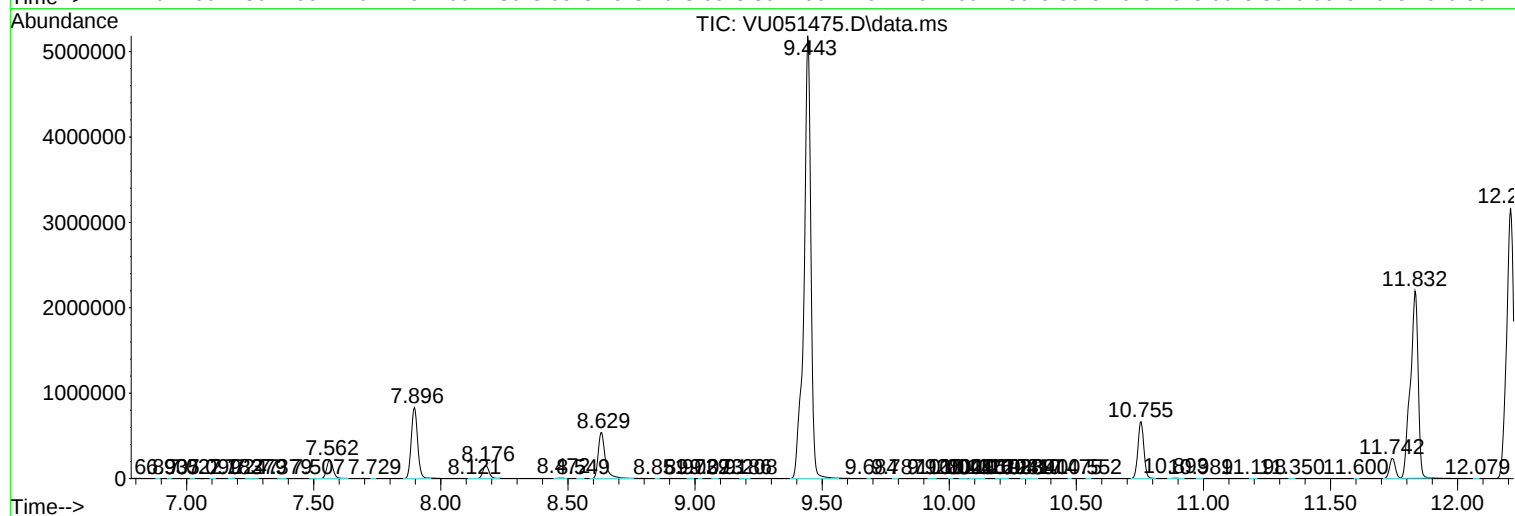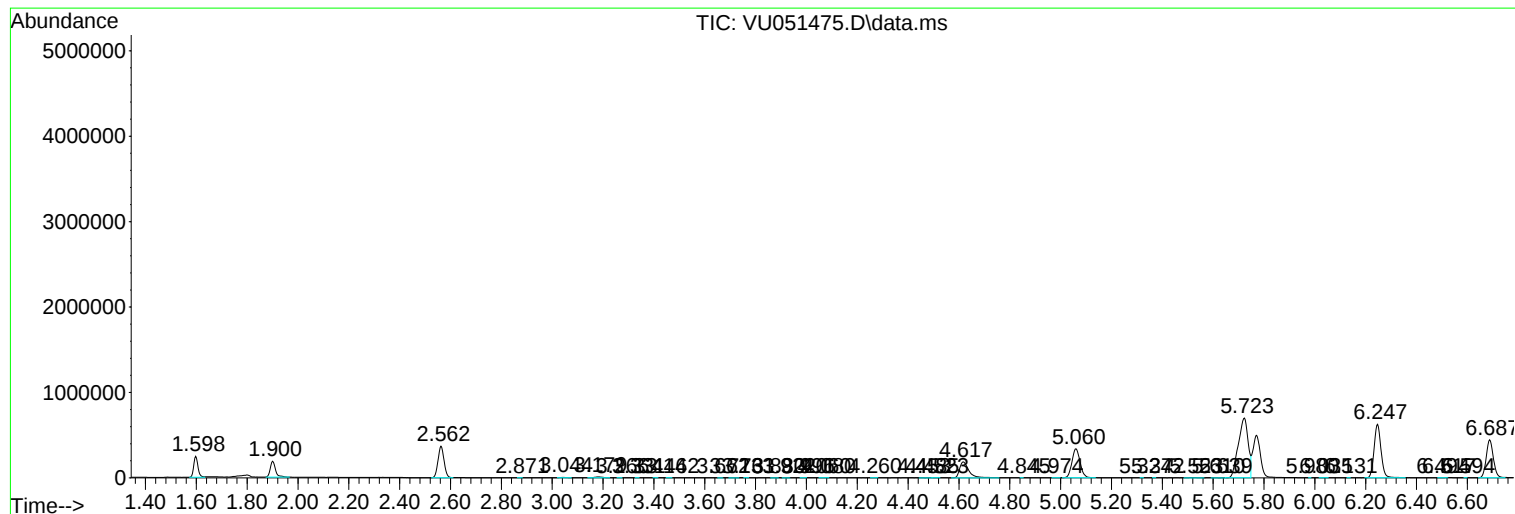

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051475.D
Acq On : 20 Oct 2022 16:29
Operator : JC/MD
Sample : N5180-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051475.D
Acq On : 20 Oct 2022 16:29
Operator : JC/MD
Sample : N5180-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0KX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc