

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051476.D
 Acq On : 20 Oct 2022 16:53
 Operator : JC/MD
 Sample : N5180-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M

Title : VOC Analysis

Signal : TIC: VU051476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	262935	301101	14.59%	1.987%
2	1.899	165	174	201	rVB	201512	297677	14.42%	1.964%
3	2.562	367	380	396	rBV	400762	650043	31.50%	4.289%
4	3.044	519	530	540	rVV5	3453	6780	0.33%	0.045%
5	3.124	552	555	560	rVB3	420	331	0.02%	0.002%
6	3.173	560	570	571	rBV3	1525	1862	0.09%	0.012%
7	3.375	630	633	639	rBV3	307	329	0.02%	0.002%
8	3.565	689	692	696	rVB2	381	281	0.01%	0.002%
9	3.597	696	702	705	rBV3	335	348	0.02%	0.002%
10	3.780	756	759	761	rVV2	458	297	0.01%	0.002%
11	3.838	770	777	782	rBV3	492	635	0.03%	0.004%
12	3.980	817	821	825	rVB2	361	341	0.02%	0.002%
13	4.002	825	828	830	rBV3	480	319	0.02%	0.002%
14	4.112	859	862	867	rVB2	512	347	0.02%	0.002%
15	4.481	971	977	983	rVB3	481	581	0.03%	0.004%
16	4.616	1005	1019	1058	rBV	205151	506453	24.54%	3.342%
17	4.980	1129	1132	1134	rBV	490	346	0.02%	0.002%
18	5.060	1140	1157	1179	rBV	377350	818293	39.65%	5.399%
19	5.369	1250	1253	1262	rBV6	1075	1342	0.07%	0.009%
20	5.504	1291	1295	1298	rBV	695	485	0.02%	0.003%
21	5.597	1320	1324	1326	rBV	345	292	0.01%	0.002%
22	5.722	1340	1363	1398	rBV2	762676	2063758	100.00%	13.617%
23	5.970	1436	1440	1446	rVB4	1361	1729	0.08%	0.011%
24	6.012	1446	1453	1459	rVB5	551	745	0.04%	0.005%
25	6.102	1477	1481	1483	rBV	652	484	0.02%	0.003%
26	6.115	1483	1485	1495	rVB4	793	1056	0.05%	0.007%
27	6.247	1508	1526	1550	rBV	587189	1122651	54.40%	7.408%
28	6.443	1584	1587	1590	rVB2	559	349	0.02%	0.002%
29	6.465	1590	1594	1597	rBV3	732	494	0.02%	0.003%
30	6.526	1605	1613	1623	rVB7	3677	6227	0.30%	0.041%
31	6.568	1623	1626	1629	rBV2	330	268	0.01%	0.002%
32	6.600	1634	1636	1645	rVB4	814	826	0.04%	0.005%
33	6.687	1648	1663	1681	rBV	474454	932326	45.18%	6.152%
34	6.896	1725	1728	1730	rBV	482	269	0.01%	0.002%
35	7.021	1764	1767	1771	rVB2	490	355	0.02%	0.002%
36	7.050	1771	1776	1778	rBV2	600	482	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051476.D
 Acq On : 20 Oct 2022 16:53
 Operator : JC/MD
 Sample : N5180-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

37	7.185	1809	1818	1827	rVV4	2884	4312	0.21%	0.028%
38	7.439	1894	1897	1900	rBV	505	420	0.02%	0.003%
39	7.565	1919	1936	1955	rBV	226837	409878	19.86%	2.705%
40	7.690	1969	1975	1978	rBV5	1166	1299	0.06%	0.009%
41	7.767	1997	1999	2005	rVB2	651	569	0.03%	0.004%
42	7.803	2005	2010	2014	rBV3	645	693	0.03%	0.005%
43	7.896	2024	2039	2066	rBV	880718	1527660	74.02%	10.080%
44	8.121	2107	2109	2112	rVB2	519	279	0.01%	0.002%
45	8.176	2114	2126	2149	rBV	164063	280253	13.58%	1.849%
46	8.439	2201	2208	2210	rBV3	537	650	0.03%	0.004%
47	8.468	2210	2217	2229	rVV4	2106	4030	0.20%	0.027%
48	8.632	2255	2268	2299	rBV2	588792	1115573	54.06%	7.361%
49	8.941	2361	2364	2370	rVB3	478	343	0.02%	0.002%
50	9.008	2383	2385	2389	rVB3	503	276	0.01%	0.002%
51	9.031	2389	2392	2396	rBV3	540	430	0.02%	0.003%
52	9.099	2408	2413	2416	rBV3	485	489	0.02%	0.003%
53	9.156	2427	2431	2433	rBV3	560	445	0.02%	0.003%
54	9.414	2498	2511	2541	rBV	833208	1419889	68.80%	9.369%
55	9.623	2573	2576	2578	rBV3	492	299	0.01%	0.002%
56	9.655	2582	2586	2589	rVB2	501	370	0.02%	0.002%
57	9.690	2590	2597	2600	rBV4	768	901	0.04%	0.006%
58	9.706	2600	2602	2611	rVB3	546	550	0.03%	0.004%
59	9.841	2641	2644	2647	rVB2	569	377	0.02%	0.002%
60	9.870	2647	2653	2656	rBV	474	470	0.02%	0.003%
61	9.893	2656	2660	2664	rBV2	309	348	0.02%	0.002%
62	10.227	2759	2764	2767	rBV2	392	321	0.02%	0.002%
63	10.385	2809	2813	2816	rBV2	419	391	0.02%	0.003%
64	10.478	2840	2842	2849	rVB2	351	297	0.01%	0.002%
65	10.555	2862	2866	2875	rVB3	504	734	0.04%	0.005%
66	10.671	2898	2902	2904	rBV2	431	367	0.02%	0.002%
67	10.754	2915	2928	2956	rBV	722989	1161237	56.27%	7.662%
68	10.854	2956	2959	2961	rVV2	769	492	0.02%	0.003%
69	10.893	2961	2971	2980	rVB5	2969	4401	0.21%	0.029%
70	10.934	2980	2984	2986	rBV	432	331	0.02%	0.002%
71	11.082	3027	3030	3033	rBV4	382	343	0.02%	0.002%
72	11.359	3113	3116	3119	rBV2	457	369	0.02%	0.002%
73	11.436	3136	3140	3144	rVB2	471	372	0.02%	0.002%
74	11.545	3167	3174	3176	rBV	660	667	0.03%	0.004%
75	11.668	3209	3212	3218	rBV3	383	331	0.02%	0.002%
76	11.696	3218	3221	3226	rBV2	414	311	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
 Data File : VU051476.D
 Acq On : 20 Oct 2022 16:53
 Operator : JC/MD
 Sample : N5180-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

77	11.748	3226	3237	3243	rBV7	3279	4944	0.24%	0.033%
78	11.809	3243	3256	3285	rBV	666744	1123075	54.42%	7.410%
79	11.992	3310	3313	3317	rVB4	505	322	0.02%	0.002%
80	12.076	3335	3339	3340	rBV	540	350	0.02%	0.002%
81	12.192	3361	3375	3398	rBV	794196	1328828	64.39%	8.768%
82	12.417	3442	3445	3446	rBV	668	316	0.02%	0.002%
83	12.741	3542	3546	3548	rBV	419	357	0.02%	0.002%
84	13.114	3658	3662	3665	rBV3	502	464	0.02%	0.003%
85	13.221	3691	3695	3696	rBV2	519	400	0.02%	0.003%
86	13.288	3712	3716	3721	rBV3	711	715	0.03%	0.005%
87	13.378	3741	3744	3748	rBV3	523	311	0.02%	0.002%
88	13.516	3782	3787	3791	rBV2	489	490	0.02%	0.003%
89	13.642	3822	3826	3830	rVB	937	844	0.04%	0.006%
90	13.667	3830	3834	3836	rBV2	465	291	0.01%	0.002%
91	13.687	3836	3840	3841	rBV2	478	388	0.02%	0.003%
92	13.732	3847	3854	3857	rBV3	840	1020	0.05%	0.007%
93	13.774	3863	3867	3872	rVB2	946	802	0.04%	0.005%
94	13.844	3881	3889	3902	rVB2	12822	20474	0.99%	0.135%
95	13.918	3909	3912	3916	rBV4	448	401	0.02%	0.003%
96	14.327	4034	4039	4049	rBV7	3631	6135	0.30%	0.040%
97	14.944	4225	4231	4234	rBV3	742	842	0.04%	0.006%
98	15.491	4399	4401	4403	rBV2	515	279	0.01%	0.002%
99	15.552	4418	4420	4423	rBV3	588	337	0.02%	0.002%
100	15.954	4543	4545	4549	rVB3	1004	574	0.03%	0.004%




Sum of corrected areas: 15155228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051476.D
Acq On : 20 Oct 2022 16:53
Operator : JC/MD
Sample : N5180-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

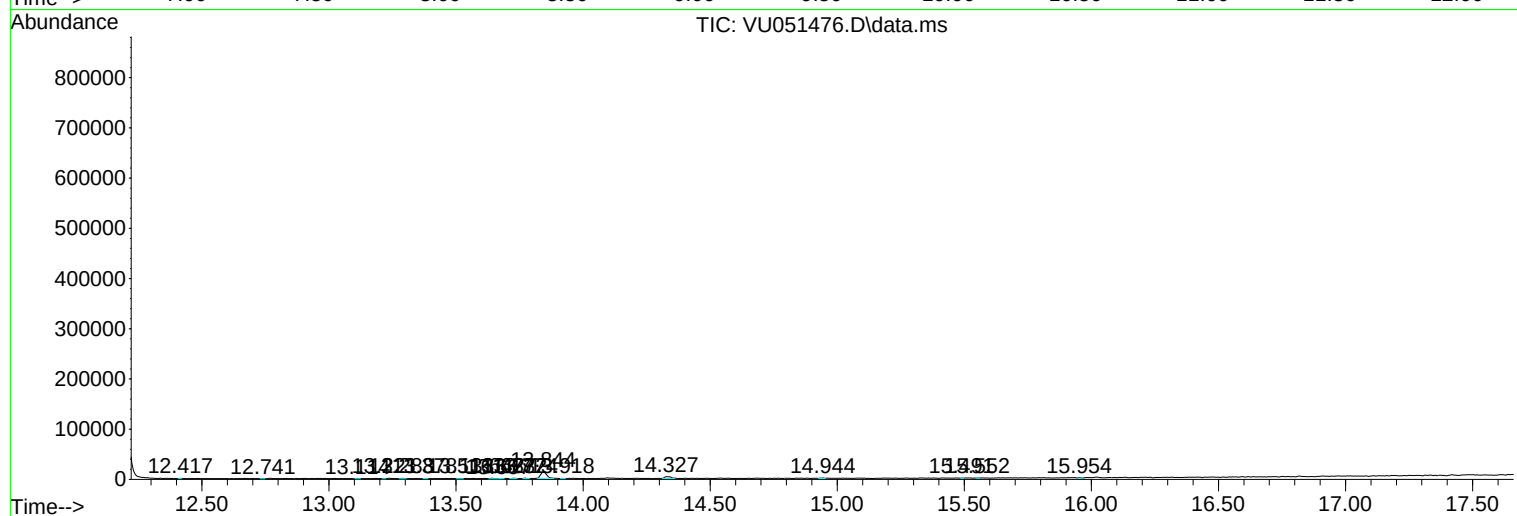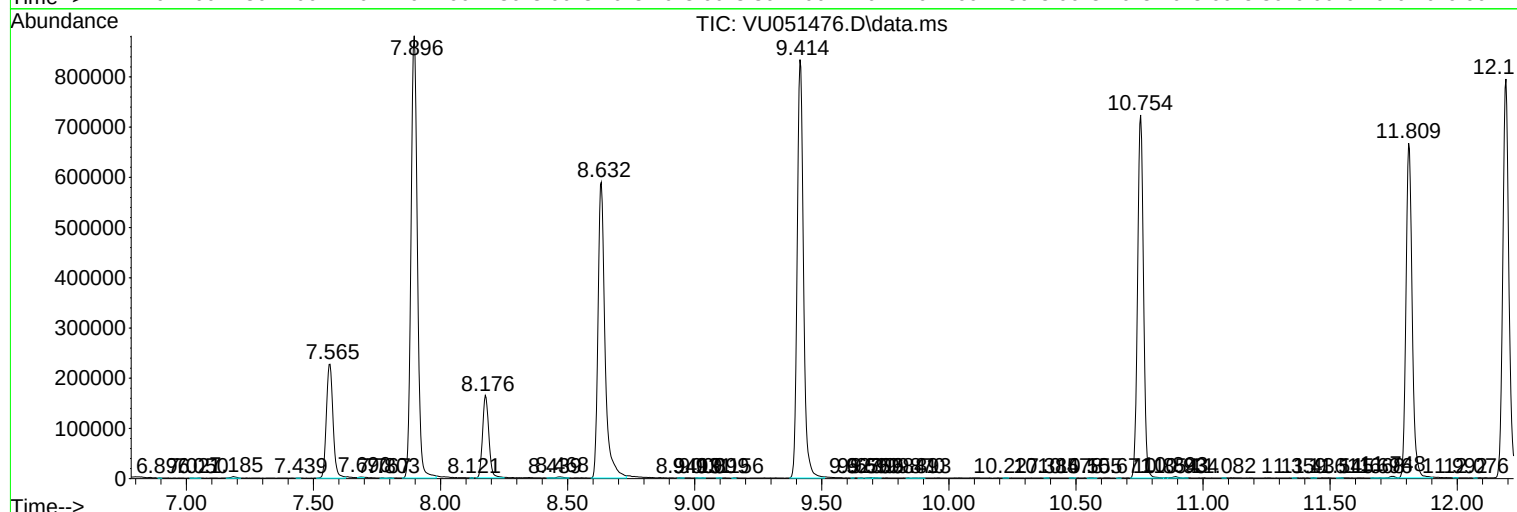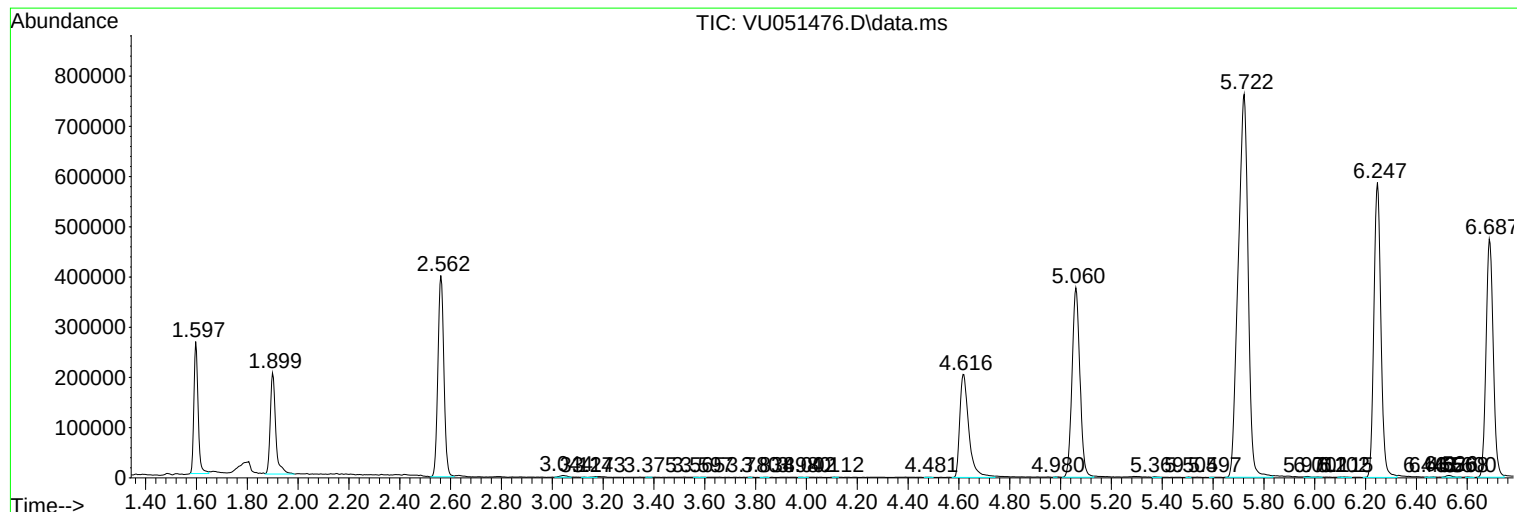

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051476.D
Acq On : 20 Oct 2022 16:53
Operator : JC/MD
Sample : N5180-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051476.D
Acq On : 20 Oct 2022 16:53
Operator : JC/MD
Sample : N5180-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------