


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102022\
Data File : VU051461.D
Acq On : 20 Oct 2022 09:18
Operator : JC/MD
Sample : BFB138
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB138

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Title : VOC Analysis
Last Update : Thu Oct 20 21:53:25 2022

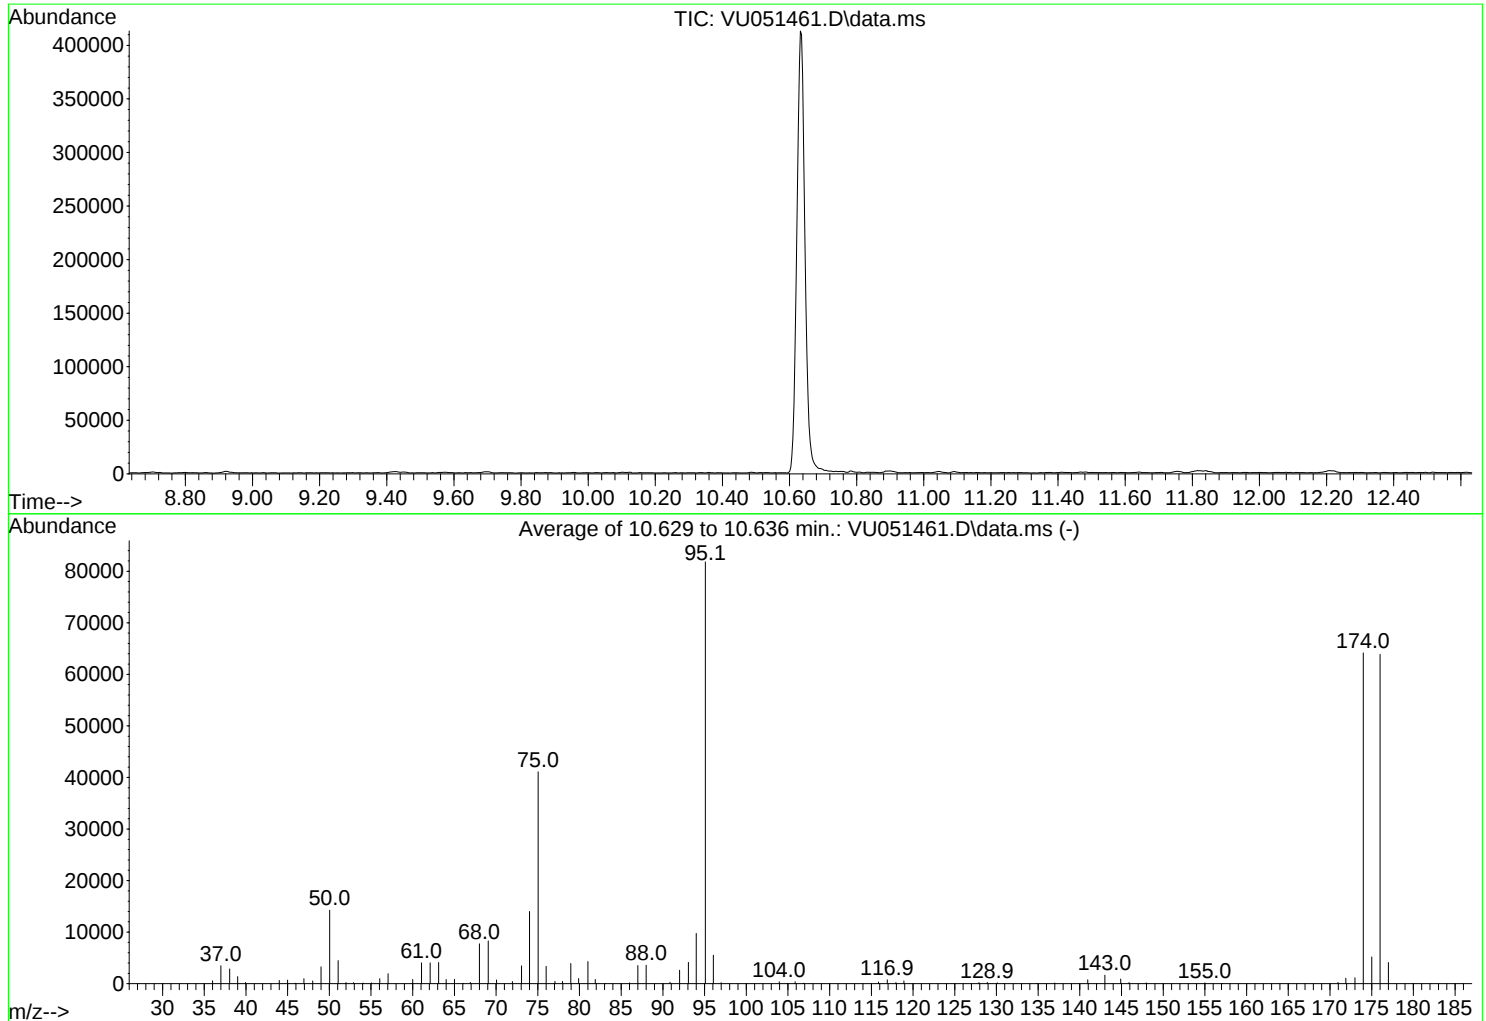

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.4	14256	PASS
75	95	30	80	50.2	41099	PASS
95	95	100	100	100.0	81827	PASS
96	95	5	9	6.7	5514	PASS
173	174	0.00	2	1.8	1167	PASS
174	95	50	120	78.4	64147	PASS
175	174	5	9	8.1	5194	PASS
176	174	95	101	99.6	63864	PASS
177	176	5	9	6.4	4095	PASS

Scan 2877 (10.591 min): VU051461.D\data.ms
BFB138

m/z	Abundance
39.90	598.0
44.00	318.0

Instrument :
MSVOA_U
ClientSampleId :
BFB138

m/z	Abundance
36.00	556.0
37.00	3216.0
38.00	2997.0
39.00	1333.0
40.00	843.0
44.00	893.0
45.00	670.0
45.90	157.0
46.90	1026.0
48.00	506.0
49.00	3241.0
50.00	13646.0
51.00	4502.0
52.00	180.0
52.90	151.0
54.10	113.0
55.00	167.0
56.00	1012.0
57.10	1801.0
60.00	870.0
61.00	4158.0
62.10	3741.0
63.10	3810.0
64.00	785.0
65.00	804.0
66.10	117.0
66.80	224.0
68.00	7316.0
69.10	8053.0
70.10	700.0
72.00	380.0
73.10	3453.0
74.00	13486.0
75.00	39192.0
76.00	3229.0
77.00	408.0
78.00	420.0
79.00	3653.0
79.90	869.0
81.00	3998.0
81.90	815.0
86.00	148.0
87.00	3503.0
88.00	3378.0
90.90	255.0
92.00	2546.0
93.10	4002.0
94.00	9504.0
95.10	78000.0
96.10	5283.0
97.00	135.0
104.00	351.0
104.90	119.0
105.80	331.0
106.90	133.0
115.90	248.0
116.90	771.0
117.90	211.0
118.90	560.0
127.90	246.0
128.90	241.0
130.10	151.0
137.00	124.0
141.00	661.0
142.00	112.0
143.00	1614.0
144.90	799.0
145.90	260.0
148.00	161.0
155.00	176.0
171.00	246.0
171.90	916.0
173.00	1071.0
174.00	59960.0
175.00	4947.0
176.00	59176.0
177.00	3881.0

Instrument :
MSVOA_U
ClientSampleId :
BFB138

m/z	Abundance
36.00	582.0
37.00	3560.0
38.10	2922.0
39.00	1418.0
40.00	802.0
44.00	974.0
45.00	714.0
45.90	141.0
46.90	962.0
48.00	552.0
49.00	3413.0
50.10	14684.0
51.00	4592.0
52.00	238.0
52.90	193.0
54.10	121.0
55.10	153.0
56.10	967.0
57.10	1978.0
60.00	834.0
61.00	4086.0
62.10	4165.0
63.10	4227.0
64.00	837.0
65.00	875.0
66.10	119.0
66.90	251.0
68.00	7996.0
69.00	8528.0
70.00	718.0
71.90	435.0
73.00	3518.0
74.00	14646.0
75.00	42440.0
76.00	3446.0
77.10	433.0
78.00	439.0
79.00	4068.0
79.90	1002.0
81.00	4407.0
81.90	850.0
86.00	137.0
87.00	3578.0
88.00	3666.0
90.80	272.0
92.00	2754.0
93.00	4341.0
94.00	9959.0
95.10	84192.0
96.10	5701.0
97.00	197.0
103.90	396.0
104.90	110.0
105.90	373.0
106.90	108.0
115.80	304.0
116.90	774.0
118.00	234.0
118.90	538.0
127.90	227.0
128.90	248.0
130.10	159.0
137.00	153.0
141.00	759.0
143.00	1685.0
144.90	961.0
145.90	241.0
147.90	171.0
155.00	152.0
170.90	268.0
171.90	1095.0
173.00	1196.0
174.00	65664.0
175.00	5397.0
176.00	65784.0
177.00	4242.0

Instrument :
MSVOA_U
ClientSampleId :
BFB138

m/z	Abundance
36.00	563.0
37.00	3676.0
38.00	2681.0
39.00	1366.0
40.00	834.0
44.00	973.0
45.00	631.0
47.00	871.0
48.00	534.0
49.00	3167.0
50.10	14438.0
51.10	4342.0
52.00	256.0
52.90	174.0
54.00	155.0
55.10	136.0
56.10	925.0
57.00	1974.0
60.00	748.0
61.10	3852.0
62.10	4179.0
63.10	4248.0
64.00	833.0
65.00	845.0
67.00	241.0
68.00	7845.0
69.00	8290.0
70.00	689.0
72.00	434.0
73.00	3369.0
74.00	13910.0
75.10	41664.0
76.00	3380.0
77.00	419.0
77.90	436.0
78.90	4056.0
79.90	1069.0
81.00	4470.0
81.90	786.0
83.10	103.0
86.00	147.0
87.00	3473.0
88.00	3627.0
90.80	304.0
92.00	2551.0
93.00	4025.0
94.00	9779.0
95.10	83288.0
96.00	5557.0
97.00	213.0
103.90	422.0
105.90	414.0
115.00	110.0
115.80	346.0
116.90	716.0
118.00	237.0
118.90	507.0
127.90	207.0
128.90	230.0
130.10	200.0
130.90	121.0
134.80	105.0
137.00	151.0
140.90	816.0
143.00	1675.0
144.90	937.0
145.90	194.0
147.90	182.0
155.00	154.0
157.10	130.0
170.90	278.0
171.90	1139.0
173.00	1235.0
174.00	66816.0
175.00	5237.0
176.00	66632.0
177.00	4161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB138