

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055820.D
 Acq On : 20 Oct 2023 09:58
 Operator : MD/SY
 Sample : VU1020MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	115	rBV	254584	304686	13.58%	1.809%
2	1.888	180	186	208	rVB	204282	294692	13.13%	1.750%
3	2.557	382	394	411	rBV	449018	739902	32.97%	4.393%
4	2.933	508	511	516	rBV3	541	574	0.03%	0.003%
5	3.039	535	544	555	rBV4	3866	6835	0.30%	0.041%
6	3.097	560	562	564	rBV	338	98	0.00%	0.001%
7	3.129	569	572	574	rBV2	292	173	0.01%	0.001%
8	3.242	605	607	610	rBV2	386	166	0.01%	0.001%
9	3.290	621	622	626	rBV	384	158	0.01%	0.001%
10	3.406	656	658	663	rBV2	177	179	0.01%	0.001%
11	3.502	685	688	690	rVB2	280	129	0.01%	0.001%
12	3.518	690	693	695	rBV	331	203	0.01%	0.001%
13	3.618	723	724	725	rBV	356	83	0.00%	0.000%
14	3.631	725	728	729	rBV	353	199	0.01%	0.001%
15	3.698	747	749	752	rBV2	327	190	0.01%	0.001%
16	3.743	757	763	764	rBV	203	207	0.01%	0.001%
17	3.811	782	784	787	rBV	182	101	0.00%	0.001%
18	3.904	811	813	816	rVB	324	149	0.01%	0.001%
19	3.972	833	834	839	rVB2	196	145	0.01%	0.001%
20	4.023	847	850	851	rBV2	259	105	0.00%	0.001%
21	4.033	851	853	858	rVB3	254	184	0.01%	0.001%
22	4.168	893	895	900	rVB2	313	221	0.01%	0.001%
23	4.190	900	902	904	rBV2	284	161	0.01%	0.001%
24	4.219	908	911	916	rBV2	198	207	0.01%	0.001%
25	4.287	930	932	933	rBV	185	84	0.00%	0.000%
26	4.332	945	946	947	rVB	348	67	0.00%	0.000%
27	4.390	959	964	969	rBV2	447	341	0.02%	0.002%
28	4.415	969	972	976	rBV2	332	238	0.01%	0.001%
29	4.557	1013	1016	1019	rVB2	251	160	0.01%	0.001%
30	4.576	1019	1022	1023	rBV	307	163	0.01%	0.001%
31	4.615	1023	1034	1072	rBV	172115	470042	20.95%	2.791%
32	4.978	1146	1147	1149	rBV	510	123	0.01%	0.001%
33	5.055	1156	1171	1195	rBV	402165	890326	39.68%	5.286%
34	5.383	1271	1273	1278	rBV2	250	221	0.01%	0.001%
35	5.409	1278	1281	1284	rVB3	358	207	0.01%	0.001%
36	5.454	1292	1295	1299	rBV2	511	337	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055820.D
 Acq On : 20 Oct 2023 09:58
 Operator : MD/SY
 Sample : VU1020MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	5.505	1309	1311	1312	rBV	63	25	0.00%	0.000%
38	5.525	1312	1317	1319	rBV2	716	496	0.02%	0.003%
39	5.576	1330	1333	1334	rBV	168	94	0.00%	0.001%
40	5.621	1344	1347	1349	rBV2	240	134	0.01%	0.001%
41	5.718	1356	1377	1404	rBV2	815522	2243920	100.00%	13.322%
42	6.030	1471	1474	1476	rBV	582	372	0.02%	0.002%
43	6.110	1495	1499	1501	rBV3	778	558	0.02%	0.003%
44	6.142	1508	1509	1512	rVB2	289	125	0.01%	0.001%
45	6.174	1516	1519	1522	rBV	503	238	0.01%	0.001%
46	6.187	1522	1523	1524	rBV	329	110	0.00%	0.001%
47	6.245	1528	1541	1581	rVV	605689	1195438	53.27%	7.097%
48	6.528	1617	1629	1645	rBV2	26557	53265	2.37%	0.316%
49	6.685	1664	1678	1705	rBV	504429	1003692	44.73%	5.959%
50	6.898	1741	1744	1747	rBV2	404	194	0.01%	0.001%
51	6.914	1747	1749	1751	rBV2	378	223	0.01%	0.001%
52	6.991	1769	1773	1774	rBV2	328	191	0.01%	0.001%
53	7.065	1794	1796	1800	rBV2	298	206	0.01%	0.001%
54	7.103	1804	1808	1810	rBV2	307	228	0.01%	0.001%
55	7.187	1823	1834	1850	rBV3	7828	16594	0.74%	0.099%
56	7.332	1877	1879	1885	rVB2	432	447	0.02%	0.003%
57	7.367	1885	1890	1893	rBV2	327	276	0.01%	0.002%
58	7.467	1914	1921	1923	rBV	478	523	0.02%	0.003%
59	7.502	1930	1932	1934	rBV2	233	120	0.01%	0.001%
60	7.560	1938	1950	1979	rBV2	258552	479764	21.38%	2.848%
61	7.795	2015	2023	2024	rBV3	2375	2278	0.10%	0.014%
62	7.840	2035	2037	2041	rBV3	664	374	0.02%	0.002%
63	7.894	2041	2054	2091	rVV	998352	1761430	78.50%	10.458%
64	8.177	2129	2142	2163	rBV	185004	325082	14.49%	1.930%
65	8.409	2212	2214	2217	rBV2	298	152	0.01%	0.001%
66	8.544	2253	2256	2258	rBV2	1031	794	0.04%	0.005%
67	8.592	2267	2271	2272	rBV	270	195	0.01%	0.001%
68	8.634	2272	2284	2323	rBV4	415062	1058732	47.18%	6.286%
69	8.920	2369	2373	2374	rBV2	676	498	0.02%	0.003%
70	9.036	2407	2409	2411	rBV2	295	177	0.01%	0.001%
71	9.078	2420	2422	2425	rBV	326	211	0.01%	0.001%
72	9.094	2425	2427	2428	rBV	435	153	0.01%	0.001%
73	9.177	2452	2453	2455	rVB	856	192	0.01%	0.001%
74	9.213	2462	2464	2466	rBV2	290	121	0.01%	0.001%
75	9.245	2472	2474	2475	rBV	123	53	0.00%	0.000%
76	9.415	2513	2527	2563	rBV	898585	1520532	67.76%	9.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055820.D
 Acq On : 20 Oct 2023 09:58
 Operator : MD/SY
 Sample : VU1020MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	9.753	2630	2632	2635	rBV2	458	271	0.01%	0.002%
78	9.885	2669	2673	2674	rBV2	383	290	0.01%	0.002%
79	9.943	2687	2691	2694	rBV2	281	272	0.01%	0.002%
80	10.110	2735	2743	2746	rBV4	1805	2357	0.11%	0.014%
81	10.332	2810	2812	2815	rBV	294	128	0.01%	0.001%
82	10.402	2833	2834	2835	rBV	152	51	0.00%	0.000%
83	10.486	2855	2860	2865	rBV4	2195	2145	0.10%	0.013%
84	10.544	2876	2878	2879	rBV	299	127	0.01%	0.001%
85	10.631	2903	2905	2906	rBV	564	216	0.01%	0.001%
86	10.647	2907	2910	2916	rVB4	1808	1801	0.08%	0.011%
87	10.682	2916	2921	2925	rBV4	450	517	0.02%	0.003%
88	10.753	2930	2943	2965	rBV	760918	1257937	56.06%	7.469%
89	11.087	3043	3047	3051	rBV4	2030	2220	0.10%	0.013%
90	11.148	3062	3066	3067	rBV2	588	412	0.02%	0.002%
91	11.242	3093	3095	3099	rVB2	615	390	0.02%	0.002%
92	11.315	3116	3118	3121	rBV	363	287	0.01%	0.002%
93	11.473	3160	3167	3174	rBV4	3232	4893	0.22%	0.029%
94	11.746	3246	3252	3259	rBV5	3490	5101	0.23%	0.030%
95	11.811	3260	3272	3307	rVV	900641	1489481	66.38%	8.843%
96	12.190	3377	3390	3418	rBV	974399	1626045	72.46%	9.654%
97	13.849	3897	3906	3918	rBV3	13581	22443	1.00%	0.133%
98	14.097	3974	3983	4006	rVB2	21375	45553	2.03%	0.270%




Sum of corrected areas: 16843200

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055820.D
Acq On : 20 Oct 2023 09:58
Operator : MD/SY
Sample : VU1020MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

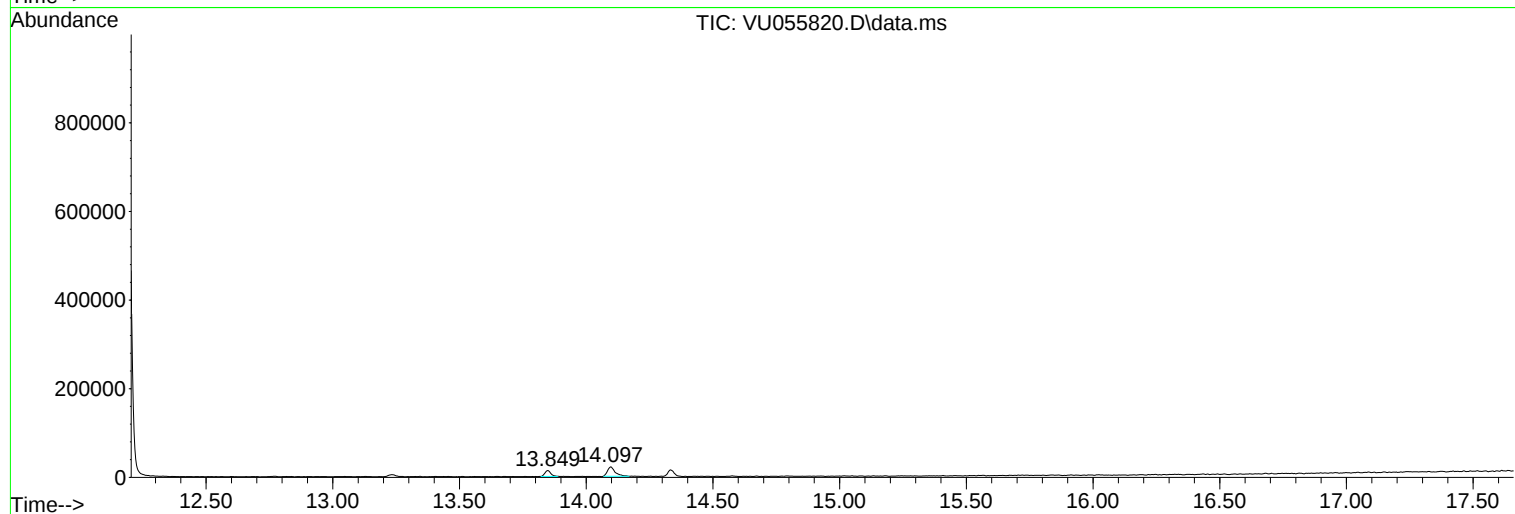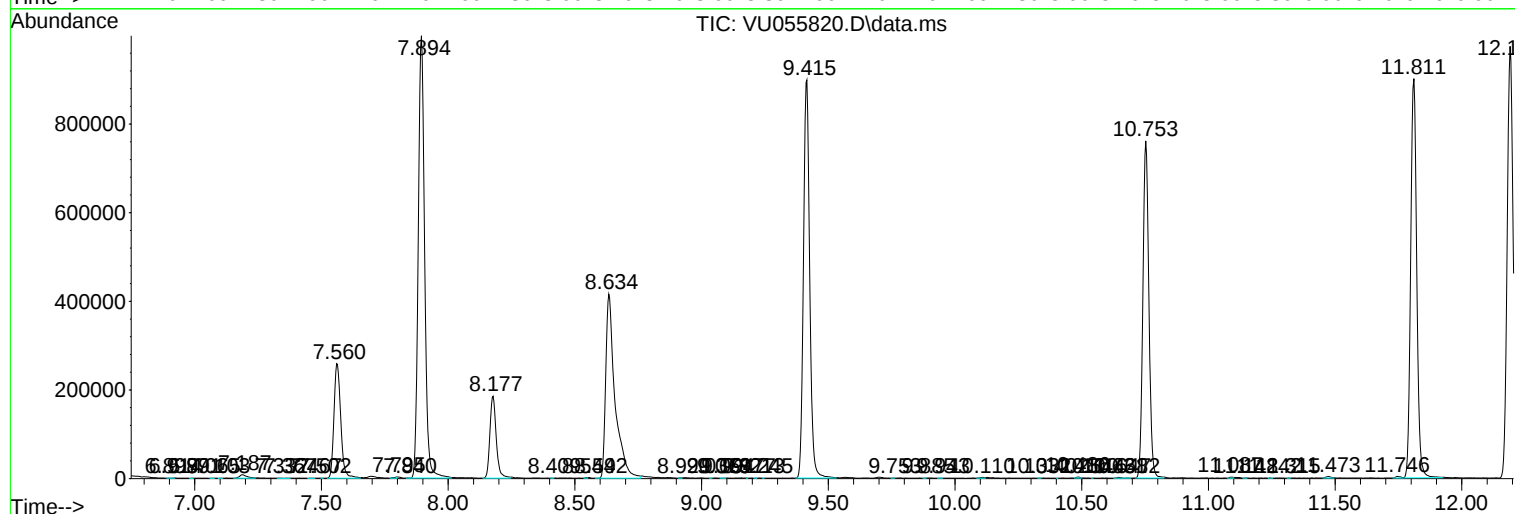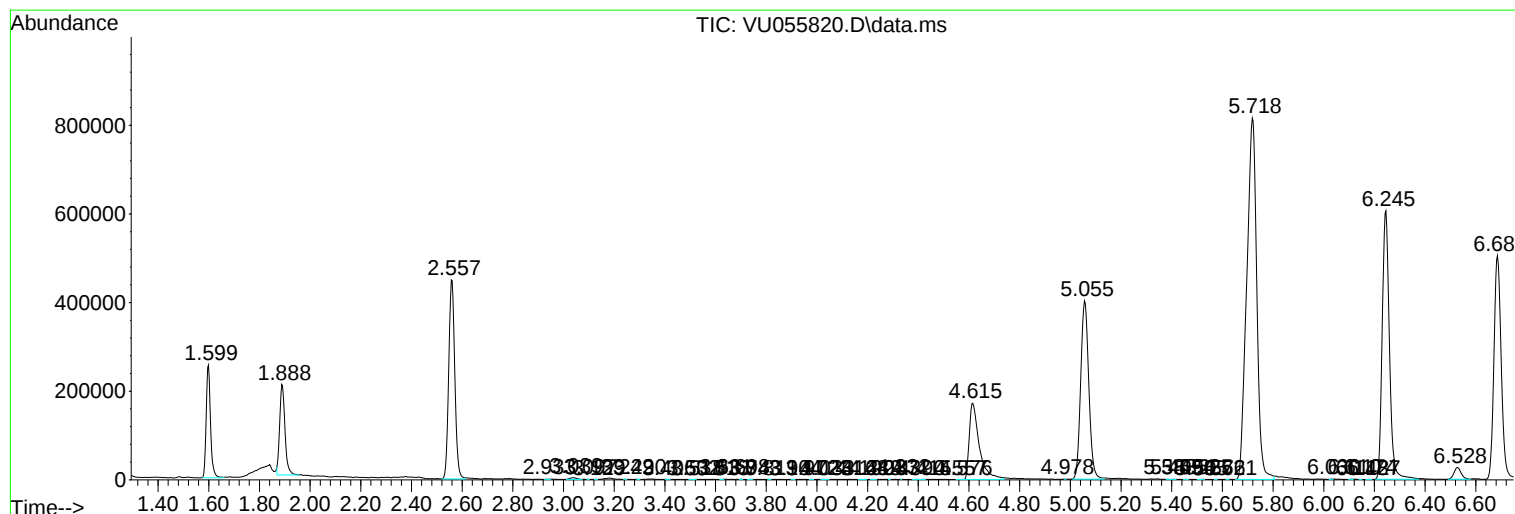

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055820.D
Acq On : 20 Oct 2023 09:58
Operator : MD/SY
Sample : VU1020MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055820.D
Acq On : 20 Oct 2023 09:58
Operator : MD/SY
Sample : VU1020MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------