

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055827.D
 Acq On : 20 Oct 2023 13:02
 Operator : MD/SY
 Sample : 04947-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	111	rBV	229509	279271	13.59%	1.777%
2	1.888	179	186	203	rVB	185559	265925	12.94%	1.693%
3	2.560	383	395	410	rBV	408040	669111	32.56%	4.259%
4	2.734	446	449	450	rBV2	705	414	0.02%	0.003%
5	2.875	488	493	495	rBV4	516	478	0.02%	0.003%
6	2.920	505	507	511	rBV2	513	310	0.02%	0.002%
7	3.039	534	544	553	rVB5	3366	6374	0.31%	0.041%
8	3.178	574	587	600	rBV2	6570	15575	0.76%	0.099%
9	3.345	636	639	640	rBV3	649	359	0.02%	0.002%
10	3.522	692	694	700	rBV2	386	348	0.02%	0.002%
11	3.628	725	727	732	rVV4	509	317	0.02%	0.002%
12	3.660	732	737	743	rVV3	314	420	0.02%	0.003%
13	3.834	785	791	794	rBV3	407	412	0.02%	0.003%
14	4.107	871	876	882	rVB	309	316	0.02%	0.002%
15	4.174	895	897	906	rVB2	483	481	0.02%	0.003%
16	4.522	1002	1005	1009	rVB2	359	302	0.01%	0.002%
17	4.557	1012	1016	1020	rVB3	386	296	0.01%	0.002%
18	4.615	1023	1034	1073	rBV2	157354	460862	22.42%	2.933%
19	4.997	1149	1153	1154	rBV	594	407	0.02%	0.003%
20	5.055	1155	1171	1195	rVV	384533	849268	41.32%	5.405%
21	5.322	1248	1254	1255	rBV4	659	657	0.03%	0.004%
22	5.448	1290	1293	1298	rVB2	422	330	0.02%	0.002%
23	5.477	1298	1302	1305	rVB2	455	348	0.02%	0.002%
24	5.509	1305	1312	1314	rBV2	420	447	0.02%	0.003%
25	5.605	1336	1342	1346	rVB2	539	563	0.03%	0.004%
26	5.718	1357	1377	1400	rBV2	748591	2055199	100.00%	13.081%
27	5.975	1451	1457	1464	rVB7	1004	1327	0.06%	0.008%
28	6.033	1471	1475	1478	rBV5	801	602	0.03%	0.004%
29	6.049	1478	1480	1485	rVB3	636	417	0.02%	0.003%
30	6.113	1496	1500	1504	rBV3	1117	1168	0.06%	0.007%
31	6.245	1526	1541	1564	rBV	593456	1149741	55.94%	7.318%
32	6.403	1588	1590	1595	rVB3	973	571	0.03%	0.004%
33	6.534	1618	1631	1648	rBV4	30680	71909	3.50%	0.458%
34	6.685	1663	1678	1702	rBV	470862	930096	45.26%	5.920%
35	6.856	1729	1731	1734	rBV3	637	349	0.02%	0.002%
36	7.030	1783	1785	1789	rVB	685	375	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055827.D
 Acq On : 20 Oct 2023 13:02
 Operator : MD/SY
 Sample : 04947-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.052	1789	1792	1797	rBV3	618	558	0.03%	0.004%
38	7.187	1822	1834	1850	rBV6	6496	16689	0.81%	0.106%
39	7.370	1890	1891	1896	rVB	574	305	0.01%	0.002%
40	7.444	1911	1914	1919	rBV2	438	350	0.02%	0.002%
41	7.493	1926	1929	1934	rBV3	486	466	0.02%	0.003%
42	7.560	1934	1950	1966	rBV	242446	440530	21.43%	2.804%
43	7.695	1986	1992	2006	rVB4	3531	6455	0.31%	0.041%
44	7.804	2024	2026	2035	rVB5	940	926	0.05%	0.006%
45	7.894	2040	2054	2076	rBV	910487	1602315	77.96%	10.198%
46	8.177	2130	2142	2162	rBV	172880	299567	14.58%	1.907%
47	8.470	2231	2233	2236	rVB	568	351	0.02%	0.002%
48	8.550	2248	2258	2271	rBV3	30913	55198	2.69%	0.351%
49	8.634	2273	2284	2327	rBV3	382365	970152	47.20%	6.175%
50	8.901	2359	2367	2372	rVB6	1183	1867	0.09%	0.012%
51	8.962	2382	2386	2390	rBV4	516	416	0.02%	0.003%
52	9.126	2433	2437	2442	rVV3	675	712	0.03%	0.005%
53	9.206	2458	2462	2463	rBV2	689	400	0.02%	0.003%
54	9.367	2509	2512	2514	rBV3	457	288	0.01%	0.002%
55	9.415	2514	2527	2564	rVV	877562	1471364	71.59%	9.365%
56	9.599	2582	2584	2588	rVB3	1161	554	0.03%	0.004%
57	9.637	2592	2596	2598	rBV	489	296	0.01%	0.002%
58	9.698	2613	2615	2617	rBV3	757	371	0.02%	0.002%
59	9.878	2668	2671	2676	rBV2	442	347	0.02%	0.002%
60	10.177	2760	2764	2767	rVB2	552	434	0.02%	0.003%
61	10.242	2781	2784	2789	rBV2	361	299	0.01%	0.002%
62	10.283	2793	2797	2801	rBV2	399	338	0.02%	0.002%
63	10.312	2801	2806	2812	rBV3	690	640	0.03%	0.004%
64	10.386	2824	2829	2833	rBV2	462	448	0.02%	0.003%
65	10.483	2856	2859	2861	rVV2	557	293	0.01%	0.002%
66	10.573	2883	2887	2890	rBV2	442	397	0.02%	0.003%
67	10.753	2926	2943	2963	rBV	705390	1170146	56.94%	7.448%
68	10.875	2979	2981	2982	rBV2	661	324	0.02%	0.002%
69	10.949	3001	3004	3008	rVB2	592	392	0.02%	0.002%
70	11.107	3048	3053	3055	rBV	682	561	0.03%	0.004%
71	11.226	3085	3090	3093	rVB2	729	586	0.03%	0.004%
72	11.254	3093	3099	3100	rBV2	540	576	0.03%	0.004%
73	11.383	3136	3139	3142	rVB2	498	319	0.02%	0.002%
74	11.406	3142	3146	3147	rBV3	663	446	0.02%	0.003%
75	11.460	3161	3163	3167	rBV2	619	479	0.02%	0.003%
76	11.502	3173	3176	3182	rVB3	584	549	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055827.D
 Acq On : 20 Oct 2023 13:02
 Operator : MD/SY
 Sample : 04947-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45K0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.637	3214	3218	3219	rBV	480	319	0.02%	0.002%
78	11.734	3244	3248	3252	rBV3	820	603	0.03%	0.004%
79	11.811	3259	3272	3296	rBV	865922	1402275	68.23%	8.925%
80	12.094	3350	3360	3368	rBV9	4289	10254	0.50%	0.065%
81	12.190	3377	3390	3415	rBV	890571	1473733	71.71%	9.380%
82	12.425	3461	3463	3467	rBV3	628	568	0.03%	0.004%
83	12.486	3478	3482	3486	rVB4	625	600	0.03%	0.004%
84	12.563	3500	3506	3507	rBV3	664	510	0.02%	0.003%
85	12.663	3535	3537	3540	rVB3	736	396	0.02%	0.003%
86	12.724	3552	3556	3558	rBV2	599	450	0.02%	0.003%
87	12.753	3561	3565	3569	rVV4	840	764	0.04%	0.005%
88	12.772	3569	3571	3577	rVB4	1002	935	0.05%	0.006%
89	12.843	3591	3593	3598	rBV3	627	418	0.02%	0.003%
90	12.894	3605	3609	3613	rBV3	778	673	0.03%	0.004%
91	12.917	3613	3616	3621	rBV5	829	868	0.04%	0.006%
92	12.942	3622	3624	3627	rVB2	716	412	0.02%	0.003%
93	13.103	3672	3674	3680	rVB2	764	577	0.03%	0.004%
94	13.155	3687	3690	3692	rBV2	611	429	0.02%	0.003%
95	13.650	3839	3844	3846	rBV2	530	531	0.03%	0.003%
96	13.766	3876	3880	3881	rBV2	607	461	0.02%	0.003%
97	14.245	4026	4029	4034	rBV3	736	652	0.03%	0.004%
98	14.524	4112	4116	4120	rBV2	723	821	0.04%	0.005%
99	14.618	4142	4145	4147	rBV2	776	563	0.03%	0.004%
100	15.293	4351	4355	4356	rBV3	1272	969	0.05%	0.006%


Sum of corrected areas: 15711830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055827.D
Acq On : 20 Oct 2023 13:02
Operator : MD/SY
Sample : 04947-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

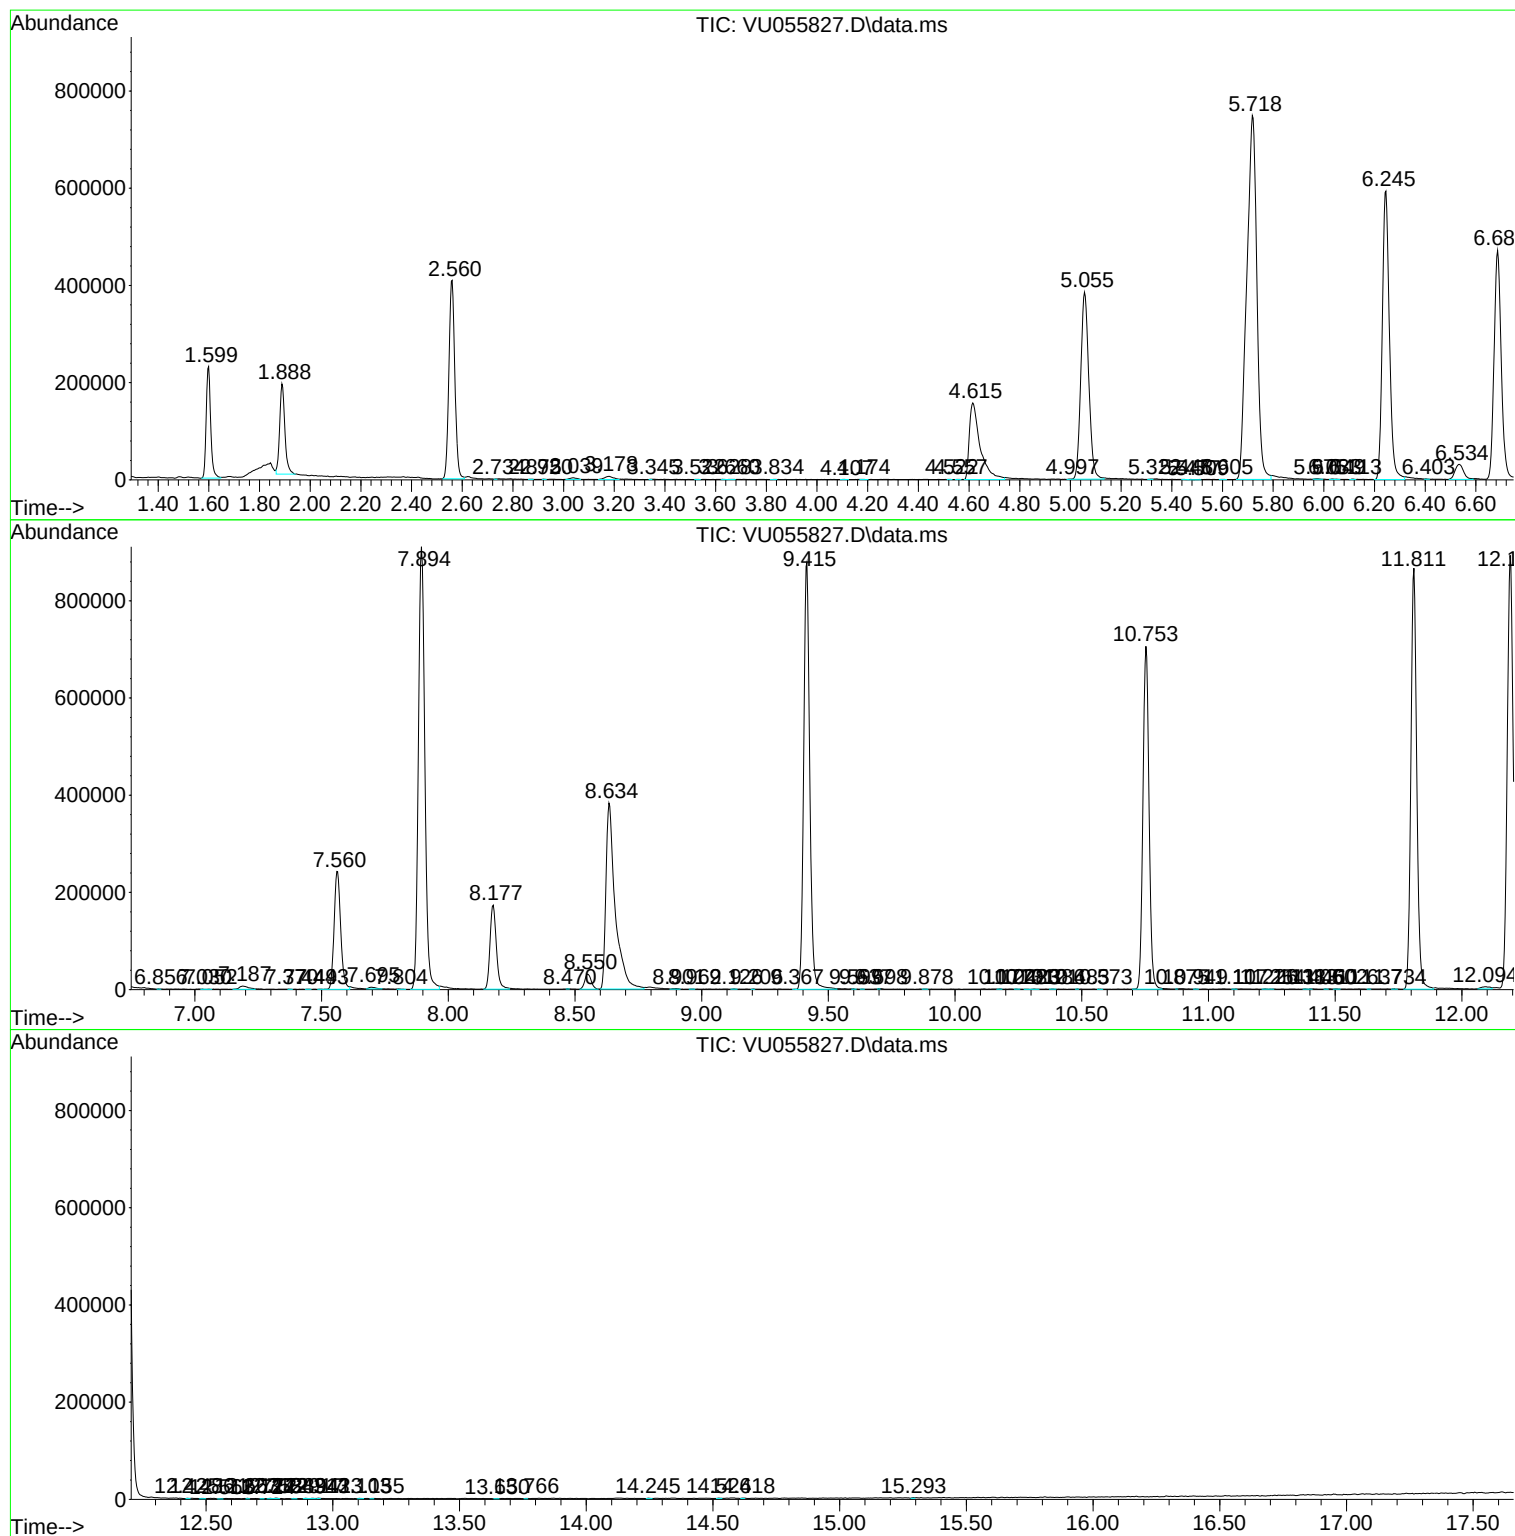

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055827.D
Acq On : 20 Oct 2023 13:02
Operator : MD/SY
Sample : 04947-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055827.D
Acq On : 20 Oct 2023 13:02
Operator : MD/SY
Sample : 04947-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45K0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------