

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055833.D
 Acq On : 20 Oct 2023 15:27
 Operator : MD/SY
 Sample : 04947-08 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

Signal : TIC: VU055833.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	110	rBV	234152	271785	12.94%	1.634%
2	1.888	179	186	204	rVB	193085	277503	13.21%	1.669%
3	2.560	382	395	426	rVB	403243	671616	31.97%	4.038%
4	2.911	502	504	509	rBV3	675	650	0.03%	0.004%
5	3.036	532	543	550	rBV5	11897	24117	1.15%	0.145%
6	3.177	576	587	602	rVB2	28232	62068	2.95%	0.373%
7	3.351	628	641	656	rVB5	6588	15619	0.74%	0.094%
8	3.637	727	730	736	rVB	546	413	0.02%	0.002%
9	3.669	736	740	742	rBV3	806	595	0.03%	0.004%
10	3.702	742	750	757	rVB5	1675	2957	0.14%	0.018%
11	3.875	797	804	808	rVB2	583	507	0.02%	0.003%
12	4.087	865	870	872	rBV3	572	473	0.02%	0.003%
13	4.103	872	875	879	rVV2	510	408	0.02%	0.002%
14	4.287	928	932	937	rBV4	739	729	0.03%	0.004%
15	4.431	971	977	987	rVB3	1161	1778	0.08%	0.011%
16	4.525	993	1006	1019	rVB5	8865	20928	1.00%	0.126%
17	4.615	1022	1034	1075	rBV	167942	482759	22.98%	2.903%
18	5.055	1154	1171	1193	rBV	385012	850649	40.49%	5.115%
19	5.290	1242	1244	1249	rBV2	355	384	0.02%	0.002%
20	5.316	1249	1252	1255	rBV3	596	512	0.02%	0.003%
21	5.338	1257	1259	1262	rVV3	850	471	0.02%	0.003%
22	5.386	1262	1274	1285	rVB5	8536	18625	0.89%	0.112%
23	5.444	1285	1292	1293	rBV4	1893	1783	0.08%	0.011%
24	5.592	1329	1338	1341	rBV5	2518	3660	0.17%	0.022%
25	5.718	1357	1377	1405	rBV2	768197	2100873	100.00%	12.632%
26	5.984	1451	1460	1472	rVB7	6430	12394	0.59%	0.075%
27	6.045	1477	1479	1485	rVB3	828	623	0.03%	0.004%
28	6.097	1490	1495	1497	rBV2	627	410	0.02%	0.002%
29	6.242	1526	1540	1564	rBV	610185	1199188	57.08%	7.211%
30	6.435	1597	1600	1603	rVB3	530	380	0.02%	0.002%
31	6.454	1603	1606	1610	rBV3	409	373	0.02%	0.002%
32	6.531	1617	1630	1644	rBV3	26410	54229	2.58%	0.326%
33	6.685	1663	1678	1695	rBV	482352	945913	45.02%	5.688%
34	6.975	1758	1768	1771	rBV5	1507	2054	0.10%	0.012%
35	7.068	1794	1797	1802	rVB4	1169	1048	0.05%	0.006%
36	7.193	1823	1836	1850	rBV4	7287	17529	0.83%	0.105%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055833.D
 Acq On : 20 Oct 2023 15:27
 Operator : MD/SY
 Sample : 04947-08 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.303	1867	1870	1876	rVB3	788	676	0.03%	0.004%
38	7.373	1888	1892	1894	rBV3	773	566	0.03%	0.003%
39	7.409	1901	1903	1905	rBV3	714	384	0.02%	0.002%
40	7.463	1917	1920	1923	rBV	585	394	0.02%	0.002%
41	7.502	1928	1932	1935	rVB3	685	490	0.02%	0.003%
42	7.560	1937	1950	1975	rBV	249756	459724	21.88%	2.764%
43	7.695	1984	1992	2005	rBV6	3630	7153	0.34%	0.043%
44	7.785	2016	2020	2023	rBV5	726	797	0.04%	0.005%
45	7.894	2034	2054	2088	rBV	936963	1649973	78.54%	9.921%
46	8.177	2126	2142	2157	rBV	171385	301680	14.36%	1.814%
47	8.354	2191	2197	2199	rBV5	1562	1681	0.08%	0.010%
48	8.409	2207	2214	2218	rBV6	720	1005	0.05%	0.006%
49	8.550	2246	2258	2272	rVB3	13237	23481	1.12%	0.141%
50	8.634	2272	2284	2323	rBV3	405947	1031116	49.08%	6.200%
51	8.862	2348	2355	2363	rVB7	2526	3849	0.18%	0.023%
52	8.920	2366	2373	2374	rBV5	1180	1134	0.05%	0.007%
53	9.020	2402	2404	2409	rVB4	606	444	0.02%	0.003%
54	9.106	2427	2431	2434	rBV2	854	704	0.03%	0.004%
55	9.161	2445	2448	2451	rVB4	815	481	0.02%	0.003%
56	9.415	2513	2527	2552	rBV	909249	1542794	73.44%	9.277%
57	9.618	2586	2590	2593	rVB4	625	436	0.02%	0.003%
58	9.688	2607	2612	2613	rBV2	1154	995	0.05%	0.006%
59	10.245	2780	2785	2786	rBV4	1812	1617	0.08%	0.010%
60	10.357	2811	2820	2825	rBV5	2584	3629	0.17%	0.022%
61	10.393	2829	2831	2832	rBV	948	408	0.02%	0.002%
62	10.483	2853	2859	2860	rBV2	1849	1696	0.08%	0.010%
63	10.624	2895	2903	2911	rVB7	3042	4515	0.21%	0.027%
64	10.688	2921	2923	2929	rBV	567	415	0.02%	0.002%
65	10.753	2930	2943	2963	rBV	735979	1206170	57.41%	7.253%
66	10.910	2981	2992	3002	rBV3	4961	8337	0.40%	0.050%
67	11.003	3016	3021	3023	rBV4	872	723	0.03%	0.004%
68	11.106	3049	3053	3055	rBV3	939	740	0.04%	0.004%
69	11.235	3088	3093	3096	rBV4	543	523	0.02%	0.003%
70	11.306	3106	3115	3122	rBV9	2847	4683	0.22%	0.028%
71	11.373	3127	3136	3139	rBV6	2863	3926	0.19%	0.024%
72	11.412	3141	3148	3160	rVB5	19875	30223	1.44%	0.182%
73	11.566	3188	3196	3201	rBV6	3971	5970	0.28%	0.036%
74	11.608	3206	3209	3212	rVV4	2848	2578	0.12%	0.016%
75	11.637	3212	3218	3231	rVB4	6324	11448	0.54%	0.069%
76	11.708	3231	3240	3248	rBV4	3076	5980	0.28%	0.036%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055833.D
 Acq On : 20 Oct 2023 15:27
 Operator : MD/SY
 Sample : 04947-08 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.811	3257	3272	3288	rBV	956795	1559932	74.25%	9.380%
78	12.097	3353	3361	3370	rVB7	8913	13402	0.64%	0.081%
79	12.190	3376	3390	3417	rBV	958622	1609230	76.60%	9.676%
80	12.376	3442	3448	3462	rVB3	8766	17220	0.82%	0.104%
81	12.534	3492	3497	3503	rBV7	4464	5900	0.28%	0.035%
82	12.576	3504	3510	3516	rVB	8733	10708	0.51%	0.064%
83	12.669	3532	3539	3547	rBV	7087	12257	0.58%	0.074%
84	12.762	3566	3568	3569	rBV2	908	444	0.02%	0.003%
85	12.878	3596	3604	3611	rBV9	1790	3036	0.14%	0.018%
86	12.942	3614	3624	3625	rBV9	4449	5704	0.27%	0.034%
87	13.032	3650	3652	3654	rBV2	1036	596	0.03%	0.004%
88	13.190	3698	3701	3704	rVV5	1245	1000	0.05%	0.006%
89	13.251	3716	3720	3728	rVB7	2993	3277	0.16%	0.020%
90	13.293	3728	3733	3740	rBV5	1806	2320	0.11%	0.014%
91	13.418	3769	3772	3773	rBV2	890	520	0.02%	0.003%
92	13.447	3775	3781	3783	rBV5	6774	6635	0.32%	0.040%
93	13.740	3867	3872	3875	rBV4	954	983	0.05%	0.006%
94	13.846	3896	3905	3910	rBV10	1909	2889	0.14%	0.017%
95	13.891	3915	3919	3923	rBV3	905	916	0.04%	0.006%
96	13.958	3938	3940	3946	rVB3	623	530	0.03%	0.003%
97	14.119	3981	3990	3992	rBV5	1792	2676	0.13%	0.016%
98	14.187	4009	4011	4015	rBV5	857	419	0.02%	0.003%
99	14.441	4088	4090	4093	rBV3	619	430	0.02%	0.003%
100	14.463	4095	4097	4100	rVB3	1036	453	0.02%	0.003%




Sum of corrected areas: 16631018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055833.D
Acq On : 20 Oct 2023 15:27
Operator : MD/SY
Sample : 04947-08 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

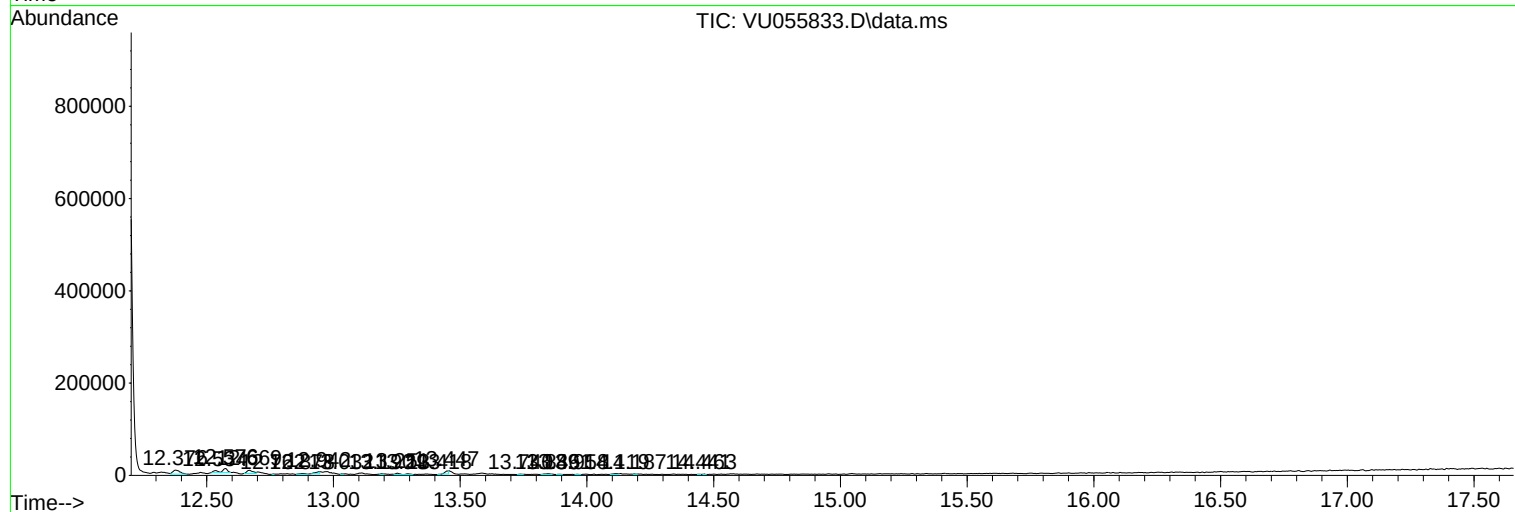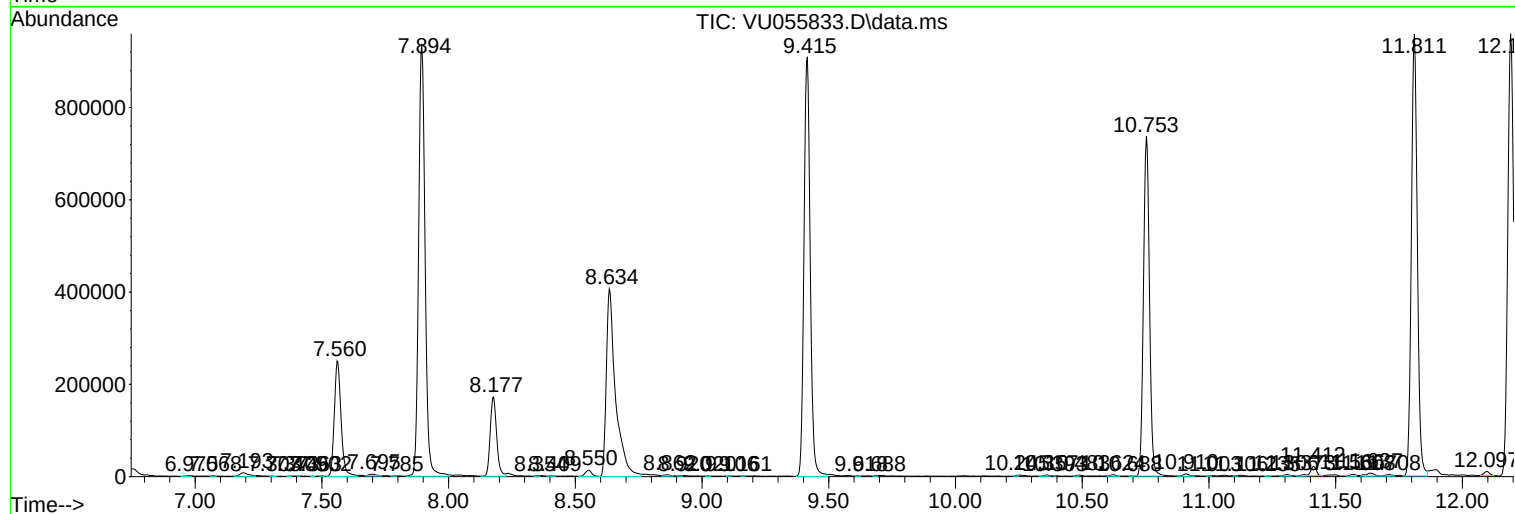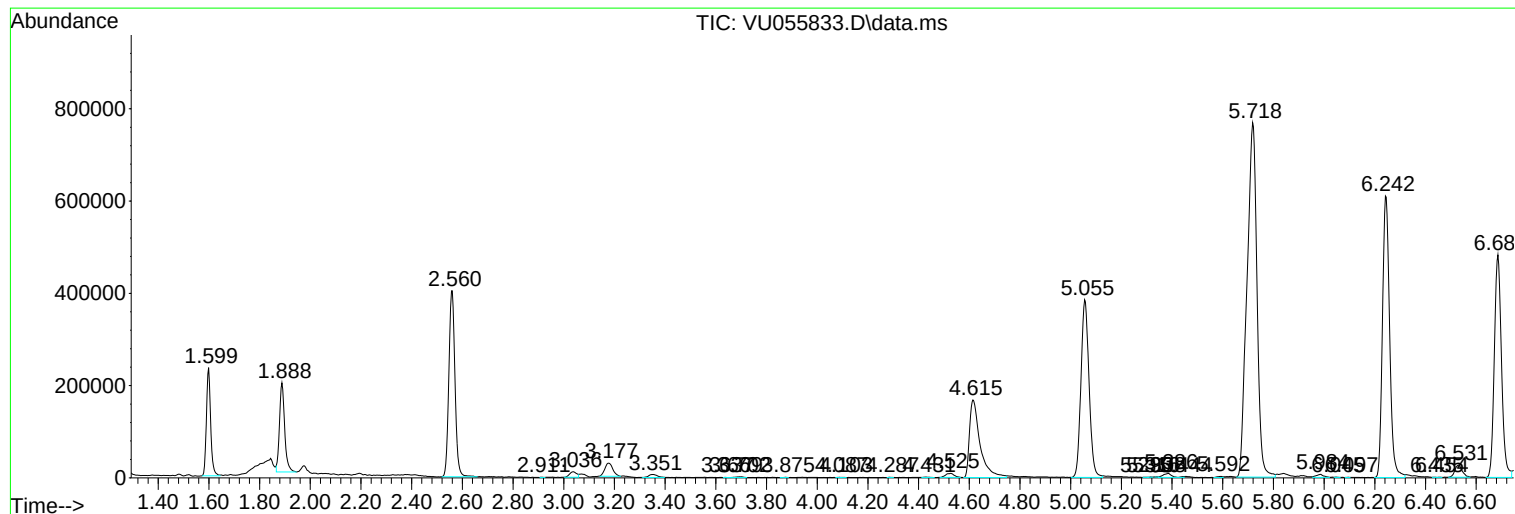

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055833.D
Acq On : 20 Oct 2023 15:27
Operator : MD/SY
Sample : 04947-08 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055833.D
Acq On : 20 Oct 2023 15:27
Operator : MD/SY
Sample : 04947-08 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------