

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055834.D
 Acq On : 20 Oct 2023 15:51
 Operator : MD/SY
 Sample : 04947-10 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

Signal : TIC: VU055834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.483	56	60	66	rVB3	4785	4277	0.20%	0.026%
2	1.599	88	96	114	rVB	216056	273147	12.94%	1.658%
3	1.882	178	184	208	rVB	185691	282267	13.37%	1.713%
4	2.557	382	394	411	rBV	408559	669921	31.73%	4.066%
5	2.718	442	444	447	rVB2	1271	622	0.03%	0.004%
6	2.785	463	465	471	rVB4	747	606	0.03%	0.004%
7	2.872	487	492	496	rBV3	470	506	0.02%	0.003%
8	2.898	498	500	507	rVB3	719	480	0.02%	0.003%
9	2.988	525	528	533	rVB2	522	402	0.02%	0.002%
10	3.036	533	543	554	rBV4	7652	14194	0.67%	0.086%
11	3.178	568	587	602	rBV	38435	88552	4.19%	0.537%
12	3.342	634	638	641	rBV4	903	806	0.04%	0.005%
13	3.641	726	731	736	rBV3	599	580	0.03%	0.004%
14	3.698	742	749	752	rBV4	489	639	0.03%	0.004%
15	3.776	768	773	777	rVB2	431	390	0.02%	0.002%
16	4.071	862	865	871	rVB2	602	467	0.02%	0.003%
17	4.145	884	888	893	rVB	559	458	0.02%	0.003%
18	4.178	893	898	904	rBV2	314	451	0.02%	0.003%
19	4.509	995	1001	1004	rBV3	389	368	0.02%	0.002%
20	4.615	1023	1034	1073	rBV	168151	528389	25.03%	3.207%
21	4.920	1124	1129	1132	rBV2	484	494	0.02%	0.003%
22	5.055	1150	1171	1192	rBV	380143	849577	40.24%	5.156%
23	5.300	1244	1247	1249	rBV3	541	377	0.02%	0.002%
24	5.319	1249	1253	1255	rVV2	1005	841	0.04%	0.005%
25	5.341	1258	1260	1267	rVB4	2002	1577	0.07%	0.010%
26	5.386	1272	1274	1277	rVV3	437	352	0.02%	0.002%
27	5.403	1277	1279	1282	rVB	838	427	0.02%	0.003%
28	5.718	1356	1377	1409	rBV2	773713	2111343	100.00%	12.814%
29	5.968	1449	1455	1456	rBV4	828	801	0.04%	0.005%
30	5.994	1461	1463	1467	rVB4	1067	752	0.04%	0.005%
31	6.116	1498	1501	1506	rVB3	637	372	0.02%	0.002%
32	6.184	1516	1522	1526	rBV2	408	467	0.02%	0.003%
33	6.242	1526	1540	1565	rBV	628449	1212059	57.41%	7.356%
34	6.528	1617	1629	1645	rBV7	24978	51066	2.42%	0.310%
35	6.685	1663	1678	1698	rBV	480586	949087	44.95%	5.760%
36	7.029	1783	1785	1790	rVB2	826	490	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055834.D
 Acq On : 20 Oct 2023 15:51
 Operator : MD/SY
 Sample : 04947-10 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.187	1824	1834	1853	rBV4	7490	18391	0.87%	0.112%
38	7.319	1871	1875	1877	rVV2	577	435	0.02%	0.003%
39	7.560	1938	1950	1982	rBV	255719	458274	21.71%	2.781%
40	7.698	1985	1993	2001	rBV4	3430	5982	0.28%	0.036%
41	7.808	2024	2027	2031	rVB2	698	558	0.03%	0.003%
42	7.894	2040	2054	2077	rBV	923996	1638490	77.60%	9.944%
43	8.177	2130	2142	2162	rBV	174501	307174	14.55%	1.864%
44	8.348	2193	2195	2198	rVB3	955	501	0.02%	0.003%
45	8.554	2248	2259	2269	rBV3	12653	21043	1.00%	0.128%
46	8.634	2272	2284	2320	rBV3	405729	1039236	49.22%	6.307%
47	8.923	2370	2374	2379	rBV5	946	988	0.05%	0.006%
48	8.975	2386	2390	2391	rBV2	754	496	0.02%	0.003%
49	9.004	2396	2399	2403	rVB3	571	431	0.02%	0.003%
50	9.062	2411	2417	2419	rBV3	880	767	0.04%	0.005%
51	9.100	2423	2429	2431	rBV3	595	600	0.03%	0.004%
52	9.116	2431	2434	2437	rVB	715	401	0.02%	0.002%
53	9.370	2507	2513	2514	rBV	483	429	0.02%	0.003%
54	9.415	2514	2527	2550	rBV	924287	1565143	74.13%	9.499%
55	9.708	2610	2618	2620	rVB6	1044	1073	0.05%	0.007%
56	9.814	2650	2651	2656	rBV	556	377	0.02%	0.002%
57	9.930	2683	2687	2691	rBV2	484	378	0.02%	0.002%
58	9.955	2692	2695	2702	rVB2	415	468	0.02%	0.003%
59	10.164	2757	2760	2764	rBV2	741	509	0.02%	0.003%
60	10.251	2781	2787	2791	rVV3	1029	1168	0.06%	0.007%
61	10.361	2813	2821	2825	rBV4	957	1318	0.06%	0.008%
62	10.393	2825	2831	2834	rVV2	436	457	0.02%	0.003%
63	10.467	2850	2854	2856	rBV	592	477	0.02%	0.003%
64	10.483	2856	2859	2865	rVB4	672	539	0.03%	0.003%
65	10.570	2884	2886	2891	rVB4	770	516	0.02%	0.003%
66	10.595	2891	2894	2897	rBV	471	352	0.02%	0.002%
67	10.621	2897	2902	2911	rVB5	1299	1644	0.08%	0.010%
68	10.753	2929	2943	2962	rBV	731939	1219696	57.77%	7.403%
69	10.907	2984	2991	2999	rBV6	1949	2943	0.14%	0.018%
70	11.113	3051	3055	3066	rVB7	1097	1656	0.08%	0.010%
71	11.309	3112	3116	3118	rBV4	925	746	0.04%	0.005%
72	11.373	3129	3136	3140	rBV5	1823	2246	0.11%	0.014%
73	11.412	3140	3148	3159	rVB5	9380	14825	0.70%	0.090%
74	11.473	3163	3167	3168	rBV2	996	636	0.03%	0.004%
75	11.566	3190	3196	3197	rBV2	1660	1398	0.07%	0.008%
76	11.637	3215	3218	3226	rVB3	2520	2754	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055834.D
 Acq On : 20 Oct 2023 15:51
 Operator : MD/SY
 Sample : 04947-10 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.688	3231	3234	3235	rBV	621	350	0.02%	0.002%
78	11.811	3259	3272	3292	rBV	927056	1522153	72.09%	9.238%
79	12.097	3354	3361	3362	rBV4	1487	1589	0.08%	0.010%
80	12.190	3377	3390	3423	rBV	927350	1558507	73.82%	9.459%
81	12.312	3424	3428	3433	rBV7	1445	1616	0.08%	0.010%
82	12.483	3479	3481	3488	rVB6	1779	1596	0.08%	0.010%
83	12.531	3488	3496	3504	rBV9	3724	7149	0.34%	0.043%
84	12.669	3531	3539	3546	rBV8	3464	4870	0.23%	0.030%
85	12.801	3577	3580	3583	rBV2	781	452	0.02%	0.003%
86	12.817	3583	3585	3588	rVB3	972	475	0.02%	0.003%
87	12.836	3588	3591	3594	rBV3	961	672	0.03%	0.004%
88	12.881	3597	3605	3608	rBV5	1379	1898	0.09%	0.012%
89	13.119	3672	3679	3682	rBV4	1078	1251	0.06%	0.008%
90	13.306	3731	3737	3739	rBV3	707	898	0.04%	0.005%
91	13.460	3777	3785	3789	rBV8	2266	3078	0.15%	0.019%
92	13.579	3816	3822	3824	rBV3	1002	1183	0.06%	0.007%
93	13.978	3944	3946	3949	rBV2	519	375	0.02%	0.002%
94	14.061	3969	3972	3975	rBV2	985	537	0.03%	0.003%
95	14.110	3985	3987	3989	rBV2	743	444	0.02%	0.003%
96	14.402	4075	4078	4082	rBV4	621	612	0.03%	0.004%
97	14.557	4124	4126	4128	rBV	772	406	0.02%	0.002%
98	14.573	4128	4131	4136	rVV5	1708	1362	0.06%	0.008%
99	14.627	4145	4148	4153	rBV4	1021	907	0.04%	0.006%
100	15.052	4278	4280	4284	rBV2	1389	1059	0.05%	0.006%


Sum of corrected areas: 16476558

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055834.D
Acq On : 20 Oct 2023 15:51
Operator : MD/SY
Sample : 04947-10 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

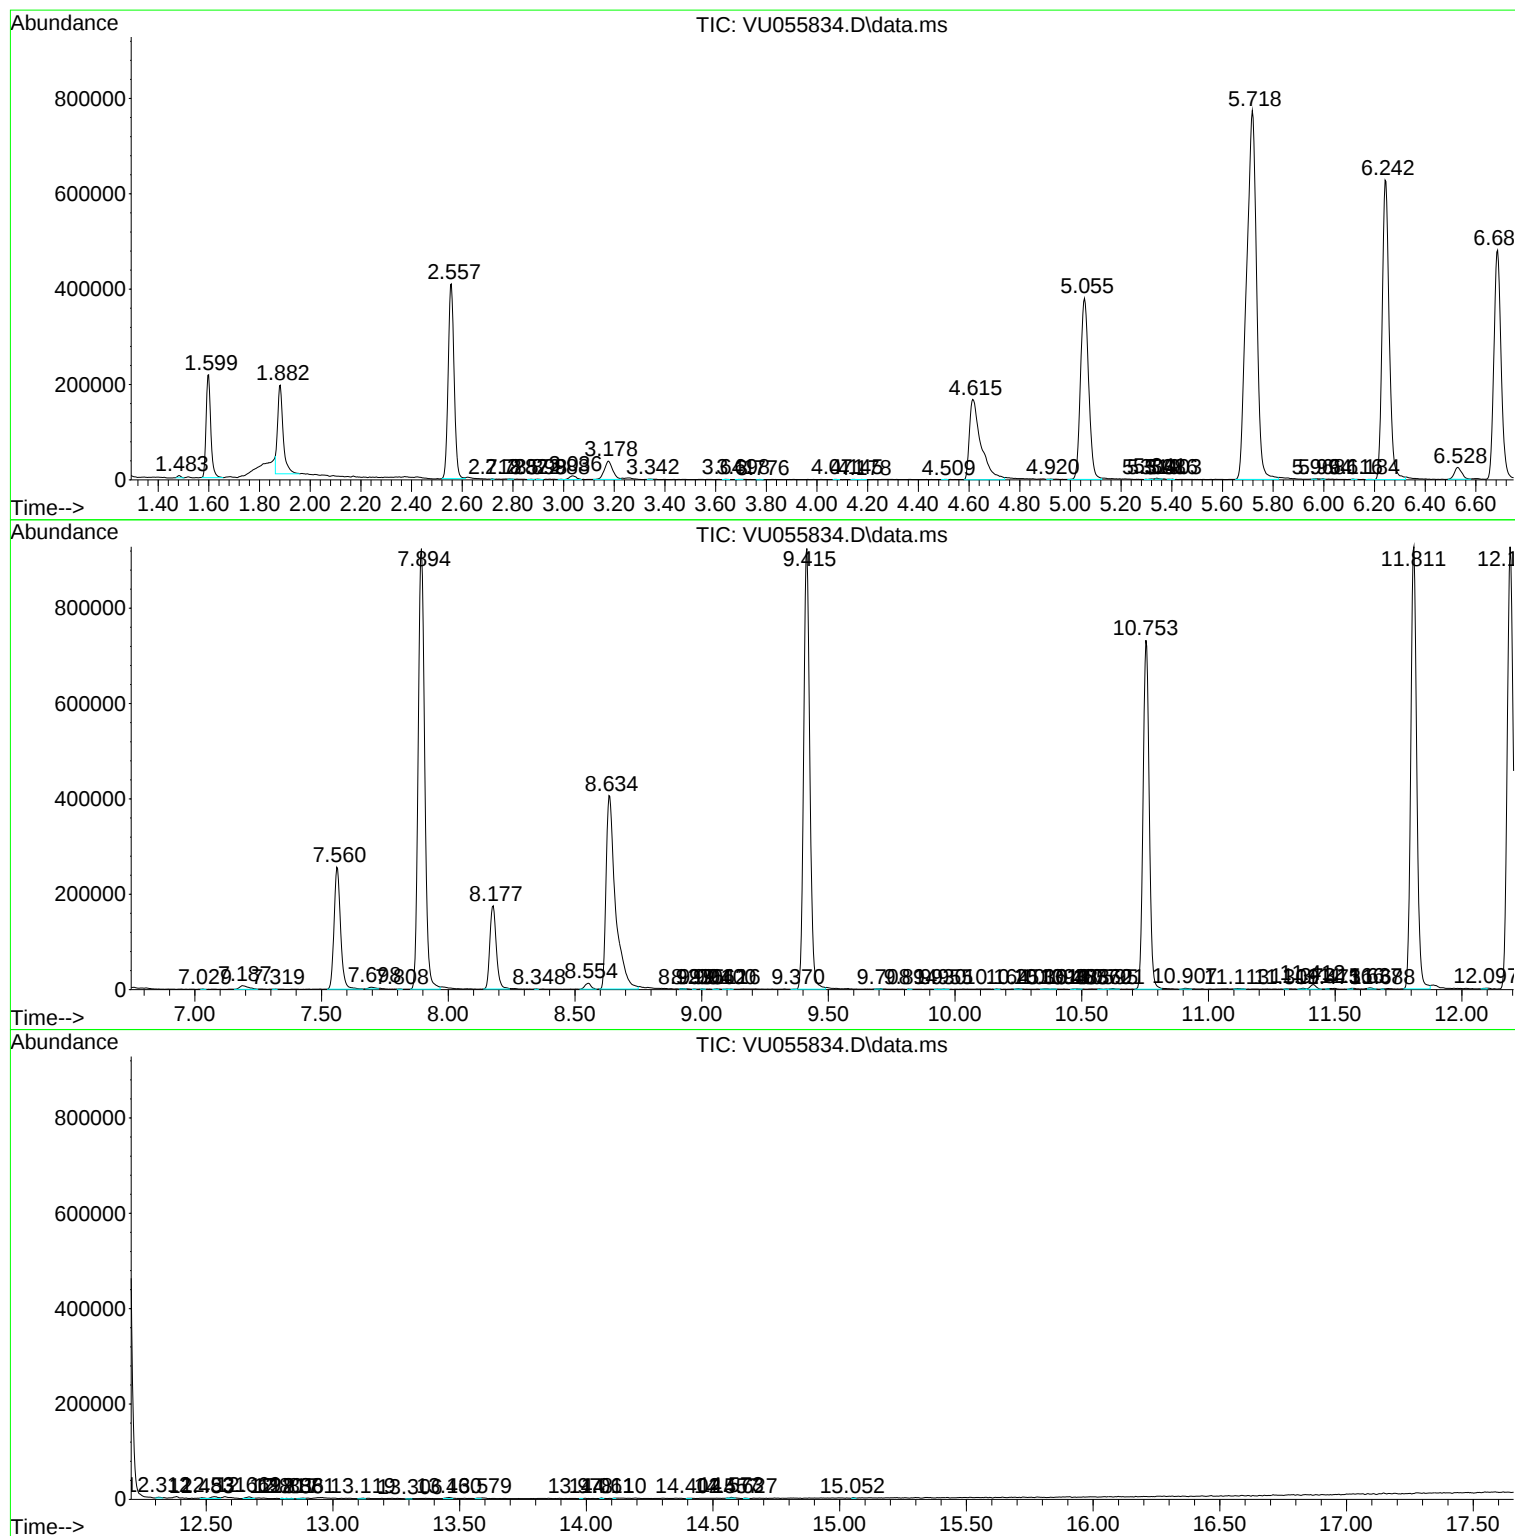

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055834.D
Acq On : 20 Oct 2023 15:51
Operator : MD/SY
Sample : 04947-10 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055834.D
Acq On : 20 Oct 2023 15:51
Operator : MD/SY
Sample : 04947-10 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------