

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055835.D
 Acq On : 20 Oct 2023 16:15
 Operator : MD/SY
 Sample : 04947-11 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	111	rBV	228674	273632	13.43%	1.722%
2	1.888	178	186	206	rVB	181027	267531	13.13%	1.684%
3	2.560	382	395	412	rBV	393440	649482	31.88%	4.087%
4	2.853	484	486	488	rVV2	651	392	0.02%	0.002%
5	3.039	533	544	555	rBV3	7909	14714	0.72%	0.093%
6	3.084	556	558	564	rVB2	513	367	0.02%	0.002%
7	3.119	564	569	571	rBV3	460	400	0.02%	0.003%
8	3.177	571	587	619	rVB	37801	97975	4.81%	0.617%
9	3.332	631	635	637	rBV2	523	336	0.02%	0.002%
10	3.454	671	673	678	rVB	463	337	0.02%	0.002%
11	3.563	705	707	712	rVB3	420	305	0.01%	0.002%
12	3.618	718	724	727	rBV2	571	504	0.02%	0.003%
13	3.656	731	736	738	rBV2	399	308	0.02%	0.002%
14	4.229	912	914	919	rVB2	430	334	0.02%	0.002%
15	4.390	963	964	971	rVB2	485	373	0.02%	0.002%
16	4.541	1008	1011	1015	rBV3	544	500	0.02%	0.003%
17	4.615	1023	1034	1064	rBV	176513	496626	24.38%	3.125%
18	4.926	1128	1131	1136	rVB3	620	620	0.03%	0.004%
19	5.055	1154	1171	1197	rBV	372664	824172	40.45%	5.187%
20	5.332	1249	1257	1264	rBV5	1434	2529	0.12%	0.016%
21	5.390	1272	1275	1280	rVB2	676	443	0.02%	0.003%
22	5.717	1356	1377	1410	rBV2	738939	2037313	100.00%	12.821%
23	5.962	1448	1453	1454	rBV4	850	693	0.03%	0.004%
24	6.126	1500	1504	1509	rBV2	747	811	0.04%	0.005%
25	6.245	1526	1541	1566	rBV	599924	1166537	57.26%	7.341%
26	6.476	1609	1613	1614	rBV2	457	313	0.02%	0.002%
27	6.528	1618	1629	1644	rVV5	24364	49467	2.43%	0.311%
28	6.685	1663	1678	1699	rBV	460304	915522	44.94%	5.762%
29	6.856	1728	1731	1735	rVB2	436	321	0.02%	0.002%
30	6.939	1751	1757	1764	rBV2	461	566	0.03%	0.004%
31	6.971	1764	1767	1772	rBV3	412	318	0.02%	0.002%
32	7.000	1773	1776	1780	rVB	564	424	0.02%	0.003%
33	7.135	1814	1818	1822	rBV2	460	329	0.02%	0.002%
34	7.187	1826	1834	1856	rVB4	7529	16298	0.80%	0.103%
35	7.325	1873	1877	1880	rBV3	524	426	0.02%	0.003%
36	7.563	1938	1951	1968	rBV	241729	438496	21.52%	2.760%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055835.D
 Acq On : 20 Oct 2023 16:15
 Operator : MD/SY
 Sample : 04947-11 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.695	1988	1992	1997	rBV5	2991	3246	0.16%	0.020%
38	7.762	2011	2013	2017	rVB4	984	568	0.03%	0.004%
39	7.795	2017	2023	2025	rBV4	995	993	0.05%	0.006%
40	7.807	2025	2027	2034	rVB3	875	739	0.04%	0.005%
41	7.894	2041	2054	2100	rBV	884976	1574023	77.26%	9.906%
42	8.123	2123	2125	2129	rVB2	588	320	0.02%	0.002%
43	8.177	2129	2142	2165	rBV	170614	295263	14.49%	1.858%
44	8.299	2174	2180	2181	rBV3	467	330	0.02%	0.002%
45	8.364	2196	2200	2208	rVB4	562	626	0.03%	0.004%
46	8.418	2213	2217	2220	rBV2	548	337	0.02%	0.002%
47	8.450	2223	2227	2230	rVB3	523	423	0.02%	0.003%
48	8.499	2238	2242	2248	rBV3	358	401	0.02%	0.003%
49	8.550	2248	2258	2271	rVB4	10566	18728	0.92%	0.118%
50	8.634	2271	2284	2324	rBV3	403892	1038929	51.00%	6.538%
51	8.865	2353	2356	2359	rBV3	798	451	0.02%	0.003%
52	8.891	2362	2364	2368	rVB4	678	437	0.02%	0.003%
53	8.913	2369	2371	2379	rVB5	931	839	0.04%	0.005%
54	8.949	2379	2382	2387	rVB3	512	458	0.02%	0.003%
55	9.071	2416	2420	2422	rBV2	631	435	0.02%	0.003%
56	9.126	2434	2437	2440	rVB	632	398	0.02%	0.003%
57	9.303	2485	2492	2497	rVB	389	459	0.02%	0.003%
58	9.331	2497	2501	2503	rBV2	623	321	0.02%	0.002%
59	9.415	2512	2527	2562	rBV	867165	1481233	72.71%	9.322%
60	9.656	2597	2602	2606	rBV3	466	433	0.02%	0.003%
61	9.698	2612	2615	2619	rBV4	966	621	0.03%	0.004%
62	9.942	2687	2691	2693	rBV	558	350	0.02%	0.002%
63	10.032	2716	2719	2724	rVB2	381	353	0.02%	0.002%
64	10.068	2724	2730	2732	rBV2	422	386	0.02%	0.002%
65	10.113	2739	2744	2747	rBV4	343	404	0.02%	0.003%
66	10.386	2826	2829	2833	rBV	431	372	0.02%	0.002%
67	10.479	2856	2858	2863	rVV3	578	485	0.02%	0.003%
68	10.621	2900	2902	2907	rVV4	892	444	0.02%	0.003%
69	10.753	2930	2943	2963	rVV	709619	1180621	57.95%	7.430%
70	10.965	3004	3009	3012	rBV2	413	407	0.02%	0.003%
71	11.010	3019	3023	3026	rBV3	710	568	0.03%	0.004%
72	11.061	3036	3039	3046	rBV6	840	1030	0.05%	0.006%
73	11.113	3053	3055	3062	rVB5	1015	1001	0.05%	0.006%
74	11.174	3070	3074	3078	rBV	582	420	0.02%	0.003%
75	11.274	3100	3105	3106	rBV2	591	465	0.02%	0.003%
76	11.415	3140	3149	3162	rVB6	6476	9562	0.47%	0.060%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055835.D
 Acq On : 20 Oct 2023 16:15
 Operator : MD/SY
 Sample : 04947-11 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.473	3163	3167	3168	rBV3	753	475	0.02%	0.003%
78	11.624	3211	3214	3216	rVV3	637	465	0.02%	0.003%
79	11.637	3216	3218	3226	rVB4	1565	1682	0.08%	0.011%
80	11.711	3239	3241	3244	rVB2	1102	659	0.03%	0.004%
81	11.810	3256	3272	3294	rBV	906261	1483140	72.80%	9.334%
82	12.042	3342	3344	3347	rBV3	572	379	0.02%	0.002%
83	12.077	3353	3355	3358	rBV3	611	387	0.02%	0.002%
84	12.190	3374	3390	3414	rBV	900017	1510319	74.13%	9.505%
85	12.380	3443	3449	3460	rVB8	3114	4729	0.23%	0.030%
86	12.450	3468	3471	3474	rBV4	764	684	0.03%	0.004%
87	12.531	3490	3496	3505	rVB7	1574	2354	0.12%	0.015%
88	12.572	3505	3509	3511	rBV4	1734	1389	0.07%	0.009%
89	12.791	3573	3577	3581	rBV2	562	497	0.02%	0.003%
90	12.843	3590	3593	3595	rBV	628	452	0.02%	0.003%
91	12.917	3613	3616	3619	rBV3	691	512	0.03%	0.003%
92	13.042	3653	3655	3658	rBV3	680	448	0.02%	0.003%
93	13.109	3673	3676	3679	rBV3	959	648	0.03%	0.004%
94	13.244	3715	3718	3721	rBV3	435	354	0.02%	0.002%
95	13.450	3779	3782	3783	rBV2	878	439	0.02%	0.003%
96	13.585	3821	3824	3825	rBV3	613	325	0.02%	0.002%
97	13.659	3845	3847	3852	rBV3	555	425	0.02%	0.003%
98	13.701	3858	3860	3864	rBV	450	319	0.02%	0.002%
99	14.135	3992	3995	3998	rBV2	758	615	0.03%	0.004%
100	14.894	4228	4231	4234	rVB4	1060	638	0.03%	0.004%




Sum of corrected areas: 15889927

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055835.D
Acq On : 20 Oct 2023 16:15
Operator : MD/SY
Sample : 04947-11 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

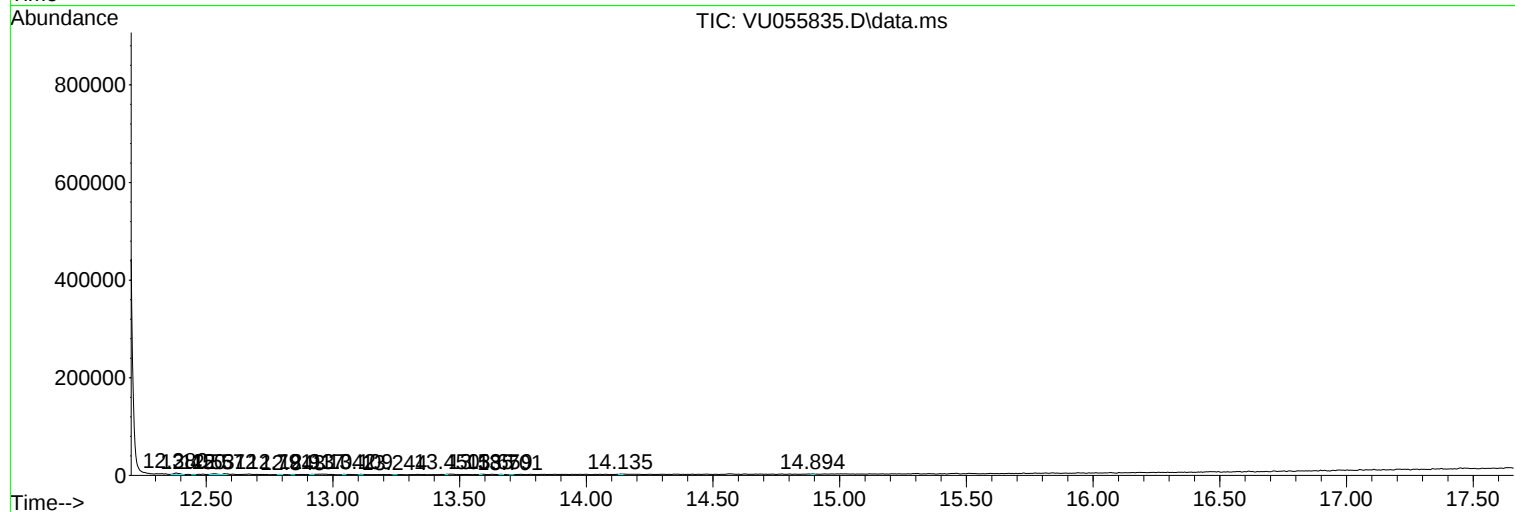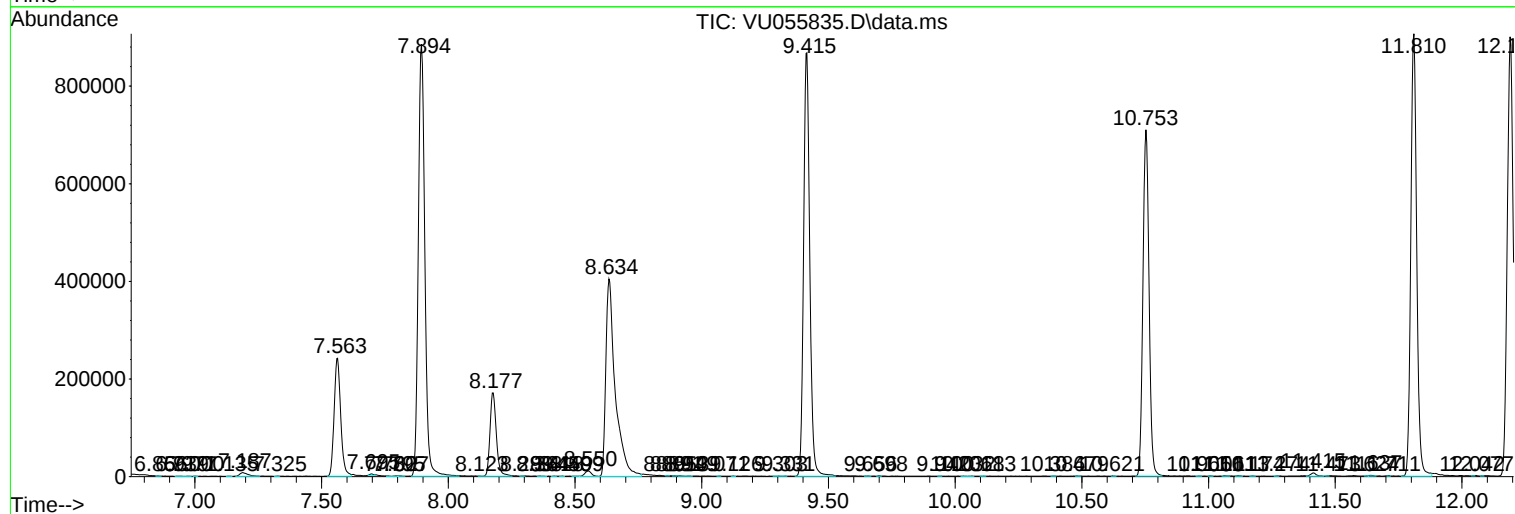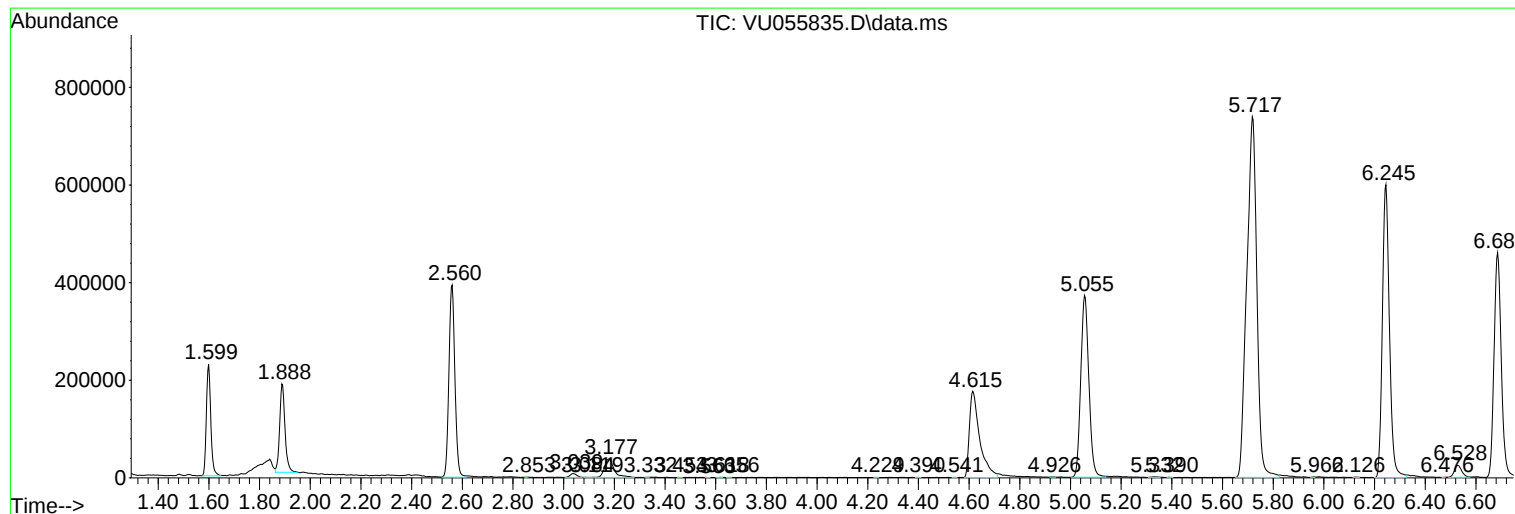

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055835.D
Acq On : 20 Oct 2023 16:15
Operator : MD/SY
Sample : 04947-11 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055835.D
Acq On : 20 Oct 2023 16:15
Operator : MD/SY
Sample : 04947-11 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------