

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055836.D
 Acq On : 20 Oct 2023 16:39
 Operator : MD/SY
 Sample : 04947-12 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.515	66	70	77	rBV4	3425	3344	0.07%	0.015%
2	1.599	87	96	113	rBV	231541	280665	6.20%	1.287%
3	1.882	178	184	204	rVB	181923	271147	5.99%	1.244%
4	2.557	382	394	413	rBV	399037	649800	14.35%	2.980%
5	2.715	440	443	448	rVB4	934	721	0.02%	0.003%
6	2.785	462	465	471	rVB4	1037	1194	0.03%	0.005%
7	2.814	471	474	477	rBV3	458	380	0.01%	0.002%
8	2.933	504	511	512	rBV2	561	555	0.01%	0.003%
9	3.036	533	543	555	rBV5	7404	13672	0.30%	0.063%
10	3.178	572	587	606	rBV	32573	78191	1.73%	0.359%
11	3.348	628	640	653	rVB5	5633	11651	0.26%	0.053%
12	3.464	674	676	683	rVB2	503	410	0.01%	0.002%
13	3.518	689	693	697	rBV3	521	491	0.01%	0.002%
14	3.695	745	748	753	rBV3	561	571	0.01%	0.003%
15	3.727	756	758	765	rVB2	493	363	0.01%	0.002%
16	4.007	843	845	849	rVV	452	339	0.01%	0.002%
17	4.055	855	860	862	rVV	416	427	0.01%	0.002%
18	4.081	866	868	872	rVV2	484	444	0.01%	0.002%
19	4.113	876	878	882	rVV2	725	587	0.01%	0.003%
20	4.149	885	889	892	rVB2	446	397	0.01%	0.002%
21	4.219	908	911	918	rVB2	466	449	0.01%	0.002%
22	4.251	918	921	923	rBV2	459	337	0.01%	0.002%
23	4.419	968	973	976	rBV	415	357	0.01%	0.002%
24	4.618	1023	1035	1037	rBV	178633	283591	6.26%	1.301%
25	4.965	1139	1143	1147	rVB3	744	560	0.01%	0.003%
26	5.055	1155	1171	1195	rBV	374862	832746	18.40%	3.819%
27	5.200	1213	1216	1218	rBV3	783	467	0.01%	0.002%
28	5.255	1231	1233	1236	rVB3	727	394	0.01%	0.002%
29	5.306	1245	1249	1251	rBV3	623	583	0.01%	0.003%
30	5.329	1252	1256	1263	rVB5	1701	1966	0.04%	0.009%
31	5.718	1355	1377	1406	rBV2	746891	2057533	45.45%	9.437%
32	5.972	1448	1456	1459	rBV4	1451	1952	0.04%	0.009%
33	6.039	1473	1477	1483	rVB5	830	814	0.02%	0.004%
34	6.097	1490	1495	1497	rBV3	617	545	0.01%	0.002%
35	6.242	1527	1540	1564	rBV	595332	1162299	25.68%	5.331%
36	6.473	1609	1612	1615	rBV3	607	514	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055836.D
 Acq On : 20 Oct 2023 16:39
 Operator : MD/SY
 Sample : 04947-12 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.538	1617	1632	1661	rVV	787041	1521459	33.61%	6.978%
38	6.685	1664	1678	1697	rVV	465662	910490	20.11%	4.176%
39	6.894	1740	1743	1746	rBV2	492	352	0.01%	0.002%
40	7.187	1826	1834	1848	rBV5	7128	15634	0.35%	0.072%
41	7.283	1862	1864	1869	rVB3	713	432	0.01%	0.002%
42	7.357	1885	1887	1891	rVB2	648	427	0.01%	0.002%
43	7.470	1915	1922	1926	rBV3	590	775	0.02%	0.004%
44	7.560	1938	1950	1980	rBV	244671	448579	9.91%	2.057%
45	7.698	1986	1993	2004	rVB4	3771	6362	0.14%	0.029%
46	7.808	2024	2027	2032	rVB3	824	633	0.01%	0.003%
47	7.837	2032	2036	2037	rBV2	512	385	0.01%	0.002%
48	7.894	2041	2054	2083	rBV	911166	1595799	35.25%	7.319%
49	8.081	2109	2112	2116	rVB2	772	554	0.01%	0.003%
50	8.100	2116	2118	2125	rBV2	549	520	0.01%	0.002%
51	8.174	2128	2141	2167	rBV	171773	306460	6.77%	1.406%
52	8.267	2167	2170	2173	rVB4	627	405	0.01%	0.002%
53	8.460	2228	2230	2236	rVB3	583	439	0.01%	0.002%
54	8.547	2242	2257	2274	rBV	2652783	4526818	100.00%	20.762%
55	8.637	2274	2285	2325	rVB3	414908	1051486	23.23%	4.823%
56	8.872	2356	2358	2362	rBV3	827	518	0.01%	0.002%
57	9.000	2395	2398	2407	rVB4	941	1078	0.02%	0.005%
58	9.174	2450	2452	2455	rVV3	625	325	0.01%	0.001%
59	9.293	2487	2489	2492	rVB	967	486	0.01%	0.002%
60	9.415	2513	2527	2549	rBV	889314	1500783	33.15%	6.883%
61	9.640	2595	2597	2602	rVB6	562	392	0.01%	0.002%
62	9.695	2608	2614	2623	rVB5	916	1592	0.04%	0.007%
63	9.772	2634	2638	2640	rBV2	556	376	0.01%	0.002%
64	9.788	2640	2643	2650	rVV3	435	498	0.01%	0.002%
65	9.820	2650	2653	2660	rVB2	556	488	0.01%	0.002%
66	9.991	2704	2706	2717	rVB3	830	927	0.02%	0.004%
67	10.100	2736	2740	2742	rBV2	383	329	0.01%	0.002%
68	10.139	2749	2752	2756	rVB3	516	381	0.01%	0.002%
69	10.354	2816	2819	2822	rBV2	522	338	0.01%	0.002%
70	10.598	2888	2895	2898	rBV3	476	639	0.01%	0.003%
71	10.753	2929	2943	2963	rBV	735698	1200731	26.52%	5.507%
72	11.004	3018	3021	3026	rBV2	832	558	0.01%	0.003%
73	11.061	3033	3039	3043	rBV4	723	834	0.02%	0.004%
74	11.209	3082	3085	3089	rBV2	391	354	0.01%	0.002%
75	11.258	3097	3100	3105	rVB2	527	442	0.01%	0.002%
76	11.335	3122	3124	3129	rVB2	545	333	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055836.D
 Acq On : 20 Oct 2023 16:39
 Operator : MD/SY
 Sample : 04947-12 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.377	3134	3137	3140	rVV	569	500	0.01%	0.002%
78	11.412	3142	3148	3158	rVB7	4513	5771	0.13%	0.026%
79	11.602	3202	3207	3210	rBV5	544	478	0.01%	0.002%
80	11.631	3212	3216	3217	rBV2	752	507	0.01%	0.002%
81	11.743	3246	3251	3257	rBV4	586	738	0.02%	0.003%
82	11.811	3257	3272	3295	rBV	915456	1492776	32.98%	6.847%
83	12.036	3340	3342	3350	rVB5	769	576	0.01%	0.003%
84	12.074	3350	3354	3356	rBV3	523	465	0.01%	0.002%
85	12.190	3377	3390	3414	rBV	910211	1529253	33.78%	7.014%
86	12.373	3444	3447	3448	rBV	727	426	0.01%	0.002%
87	12.447	3468	3470	3475	rBV5	578	391	0.01%	0.002%
88	12.582	3505	3512	3517	rBV4	1494	1906	0.04%	0.009%
89	12.669	3532	3539	3544	rBV6	1113	1783	0.04%	0.008%
90	12.991	3637	3639	3642	rBV2	591	355	0.01%	0.002%
91	13.007	3642	3644	3646	rBV	1244	344	0.01%	0.002%
92	13.254	3718	3721	3729	rVB5	944	1155	0.03%	0.005%
93	13.592	3822	3826	3830	rBV2	917	748	0.02%	0.003%
94	13.627	3834	3837	3840	rVB3	777	549	0.01%	0.003%
95	13.650	3841	3844	3846	rBV2	583	471	0.01%	0.002%
96	13.695	3855	3858	3860	rBV3	727	355	0.01%	0.002%
97	14.560	4125	4127	4132	rBV5	915	934	0.02%	0.004%
98	14.714	4172	4175	4177	rBV2	831	567	0.01%	0.003%
99	14.769	4190	4192	4195	rBV2	737	421	0.01%	0.002%
100	15.077	4285	4288	4291	rBV3	852	712	0.02%	0.003%




Sum of corrected areas: 21803048

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055836.D
Acq On : 20 Oct 2023 16:39
Operator : MD/SY
Sample : 04947-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

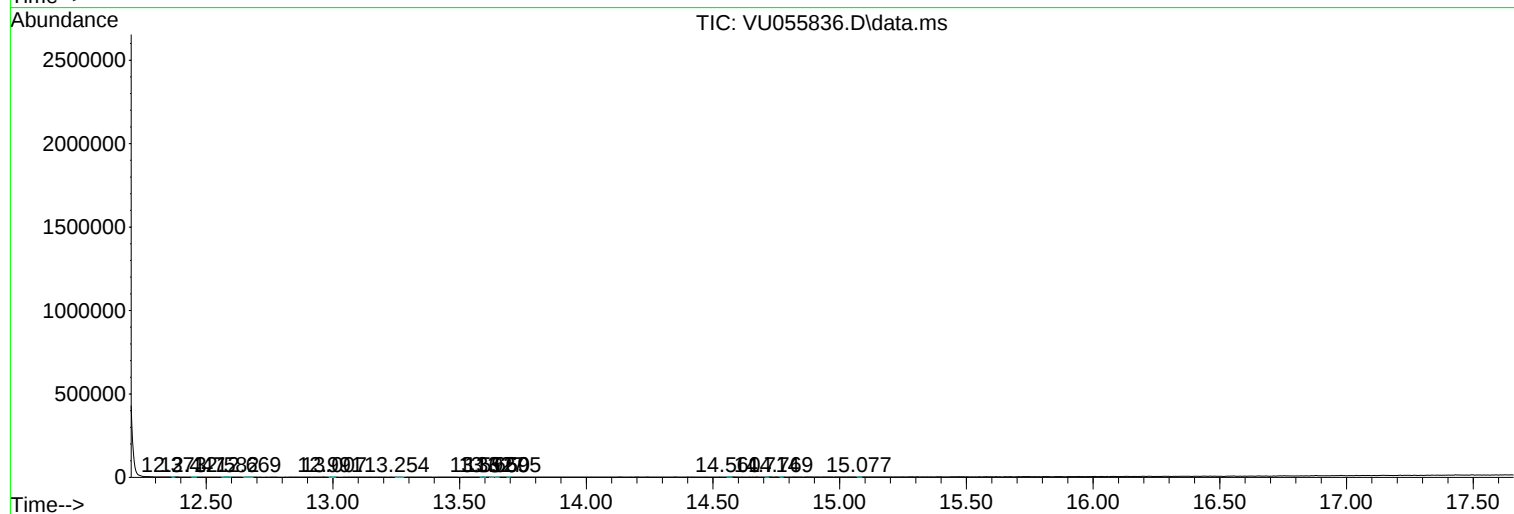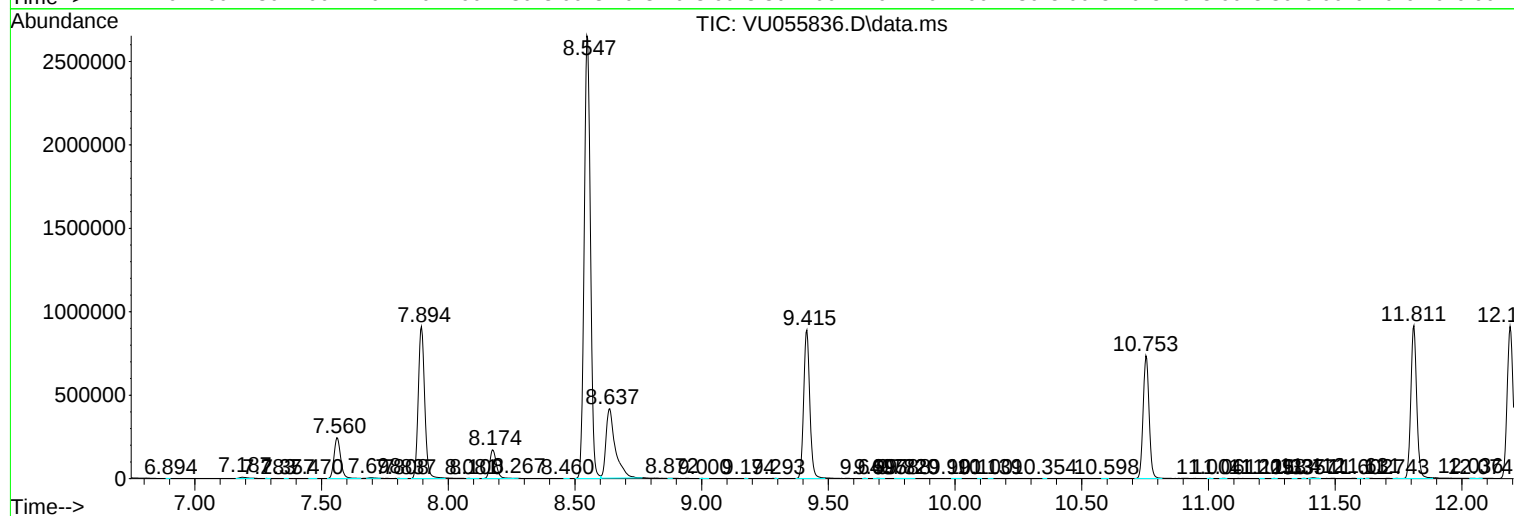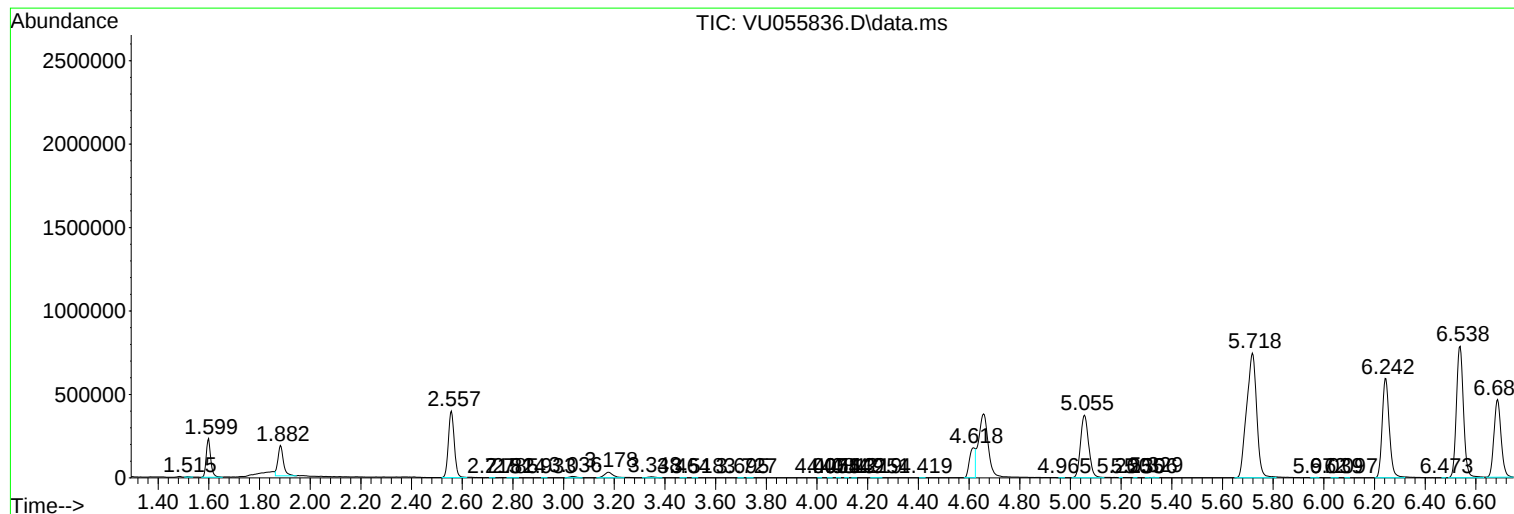

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055836.D
Acq On : 20 Oct 2023 16:39
Operator : MD/SY
Sample : 04947-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055836.D
Acq On : 20 Oct 2023 16:39
Operator : MD/SY
Sample : 04947-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------