

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055840.D
 Acq On : 20 Oct 2023 18:16
 Operator : MD/SY
 Sample : 04947-05DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	111	rBV	213273	267245	12.83%	1.456%
2	1.882	178	184	201	rVB	179182	268790	12.91%	1.465%
3	2.557	381	394	412	rBV	396782	652779	31.35%	3.557%
4	2.692	434	436	438	rBV3	631	357	0.02%	0.002%
5	2.750	452	454	456	rBV	583	324	0.02%	0.002%
6	2.869	487	491	494	rBV4	890	536	0.03%	0.003%
7	2.939	510	513	520	rVB4	566	627	0.03%	0.003%
8	3.036	533	543	554	rBV4	6261	11248	0.54%	0.061%
9	3.177	571	587	602	rBV	42157	99648	4.78%	0.543%
10	3.351	628	641	651	rVV7	5169	9650	0.46%	0.053%
11	3.431	659	666	668	rBV	560	461	0.02%	0.003%
12	3.464	672	676	679	rVV2	313	308	0.01%	0.002%
13	3.775	771	773	778	rVB2	434	311	0.01%	0.002%
14	3.846	786	795	798	rBV3	728	865	0.04%	0.005%
15	3.865	798	801	804	rVB2	988	605	0.03%	0.003%
16	4.071	862	865	869	rBV2	388	325	0.02%	0.002%
17	4.615	1022	1034	1040	rBV	177951	369669	17.75%	2.014%
18	4.904	1121	1124	1127	rBV2	819	540	0.03%	0.003%
19	4.965	1137	1143	1144	rBV4	806	620	0.03%	0.003%
20	5.055	1154	1171	1196	rBV	379294	843004	40.48%	4.594%
21	5.309	1245	1250	1252	rBV4	1223	1127	0.05%	0.006%
22	5.373	1265	1270	1283	rVB9	2099	4154	0.20%	0.023%
23	5.518	1306	1315	1320	rBV3	1448	1859	0.09%	0.010%
24	5.717	1355	1377	1416	rBV2	758118	2082537	100.00%	11.348%
25	5.978	1452	1458	1464	rVB5	1294	1679	0.08%	0.009%
26	6.087	1488	1492	1496	rBV4	348	330	0.02%	0.002%
27	6.123	1496	1503	1505	rBV3	506	482	0.02%	0.003%
28	6.242	1527	1540	1568	rBV	603220	1163926	55.89%	6.343%
29	6.537	1616	1632	1656	rBV3	346412	689388	33.10%	3.757%
30	6.685	1664	1678	1698	rBV	471580	924710	44.40%	5.039%
31	7.074	1794	1799	1802	rVB	442	309	0.01%	0.002%
32	7.097	1802	1806	1807	rBV	579	419	0.02%	0.002%
33	7.110	1807	1810	1815	rVB4	601	543	0.03%	0.003%
34	7.187	1825	1834	1848	rBV3	7801	17571	0.84%	0.096%
35	7.560	1937	1950	1981	rBV	243451	449503	21.58%	2.449%
36	7.695	1986	1992	2001	rBV3	4239	6398	0.31%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055840.D
 Acq On : 20 Oct 2023 18:16
 Operator : MD/SY
 Sample : 04947-05DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.894	2040	2054	2075	rBV	902309	1601775	76.91%	8.729%
38	8.129	2122	2127	2129	rVB4	595	576	0.03%	0.003%
39	8.177	2129	2142	2163	rBV	172177	303576	14.58%	1.654%
40	8.357	2196	2198	2205	rVB2	450	422	0.02%	0.002%
41	8.402	2205	2212	2220	rVB5	1366	2021	0.10%	0.011%
42	8.444	2220	2225	2228	rBV2	470	436	0.02%	0.002%
43	8.483	2233	2237	2241	rBV2	640	563	0.03%	0.003%
44	8.547	2244	2257	2274	rBV	1033661	1766056	84.80%	9.624%
45	8.637	2274	2285	2323	rVB3	411338	1034905	49.69%	5.640%
46	8.917	2366	2372	2375	rBV4	966	1216	0.06%	0.007%
47	9.139	2438	2441	2444	rVB	717	416	0.02%	0.002%
48	9.164	2444	2449	2453	rBV3	890	900	0.04%	0.005%
49	9.277	2478	2484	2485	rBV4	574	478	0.02%	0.003%
50	9.325	2496	2499	2504	rVB4	486	305	0.01%	0.002%
51	9.351	2504	2507	2510	rBV2	446	299	0.01%	0.002%
52	9.415	2514	2527	2548	rBV	886332	1504060	72.22%	8.196%
53	9.659	2597	2603	2604	rBV3	530	500	0.02%	0.003%
54	9.698	2610	2615	2617	rBV4	2129	1770	0.08%	0.010%
55	9.772	2636	2638	2646	rVB2	374	311	0.01%	0.002%
56	9.804	2646	2648	2653	rBV3	423	301	0.01%	0.002%
57	10.100	2733	2740	2744	rBV5	2082	2853	0.14%	0.016%
58	10.241	2777	2784	2790	rBV2	474	545	0.03%	0.003%
59	10.296	2798	2801	2808	rVB3	929	803	0.04%	0.004%
60	10.483	2851	2859	2863	rBV6	2015	2565	0.12%	0.014%
61	10.624	2901	2903	2909	rVB3	408	301	0.01%	0.002%
62	10.753	2931	2943	2962	rBV	728472	1203127	57.77%	6.556%
63	10.852	2972	2974	2979	rVB3	481	448	0.02%	0.002%
64	10.901	2987	2989	2992	rVB3	932	494	0.02%	0.003%
65	10.991	3015	3017	3022	rVB2	515	425	0.02%	0.002%
66	11.068	3037	3041	3042	rBV	520	357	0.02%	0.002%
67	11.097	3044	3050	3054	rVV4	1495	1841	0.09%	0.010%
68	11.222	3083	3089	3094	rBV2	514	421	0.02%	0.002%
69	11.380	3134	3138	3141	rVB3	677	570	0.03%	0.003%
70	11.409	3141	3147	3148	rBV5	1951	1434	0.07%	0.008%
71	11.466	3160	3165	3166	rBV2	1341	1086	0.05%	0.006%
72	11.589	3200	3203	3205	rBV	486	303	0.01%	0.002%
73	11.643	3215	3220	3222	rBV3	677	547	0.03%	0.003%
74	11.746	3246	3252	3259	rVB6	1558	2403	0.12%	0.013%
75	11.810	3259	3272	3294	rBV	904070	1477223	70.93%	8.050%
76	11.981	3323	3325	3328	rBV3	704	490	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055840.D
 Acq On : 20 Oct 2023 18:16
 Operator : MD/SY
 Sample : 04947-05DL 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	12.042	3340	3344	3350	rBV4	567	554	0.03%	0.003%
78	12.074	3350	3354	3357	rVB2	637	438	0.02%	0.002%
79	12.190	3377	3390	3417	rBV	916840	1537000	73.80%	8.376%
80	12.408	3455	3458	3461	rBV3	649	435	0.02%	0.002%
81	12.482	3477	3481	3482	rBV2	507	322	0.02%	0.002%
82	12.659	3533	3536	3539	rBV4	785	517	0.02%	0.003%
83	12.772	3564	3571	3576	rBV4	875	1173	0.06%	0.006%
84	12.833	3587	3590	3596	rVV3	669	677	0.03%	0.004%
85	12.875	3600	3603	3608	rBV5	542	507	0.02%	0.003%
86	12.942	3621	3624	3630	rBV4	636	444	0.02%	0.002%
87	13.003	3639	3643	3646	rBV2	646	504	0.02%	0.003%
88	13.437	3770	3778	3789	rBV6	2771	5469	0.26%	0.030%
89	13.582	3819	3823	3825	rBV2	1873	1669	0.08%	0.009%
90	13.756	3874	3877	3879	rBV3	666	386	0.02%	0.002%
91	13.839	3900	3903	3904	rBV	535	296	0.01%	0.002%
92	13.865	3908	3911	3912	rBV3	826	457	0.02%	0.002%
93	13.923	3925	3929	3933	rBV	957	839	0.04%	0.005%
94	14.035	3962	3964	3969	rVB2	718	499	0.02%	0.003%
95	14.170	4003	4006	4010	rBV4	834	677	0.03%	0.004%
96	14.190	4010	4012	4018	rVB4	1328	1082	0.05%	0.006%
97	14.302	4045	4047	4052	rBV2	578	577	0.03%	0.003%
98	14.453	4088	4094	4096	rBV4	1882	2096	0.10%	0.011%
99	14.569	4124	4130	4131	rBV3	1775	1910	0.09%	0.010%
100	15.055	4279	4281	4283	rBV	897	416	0.02%	0.002%

Sum of corrected areas: 18350913




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055840.D
Acq On : 20 Oct 2023 18:16
Operator : MD/SY
Sample : 04947-05DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

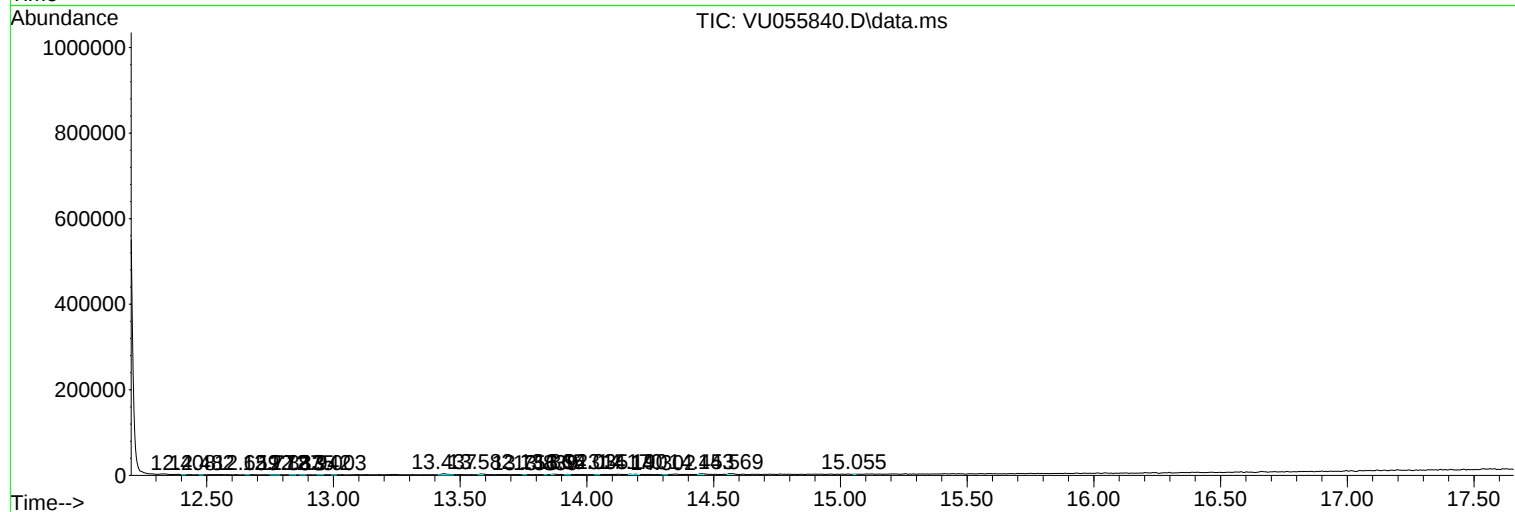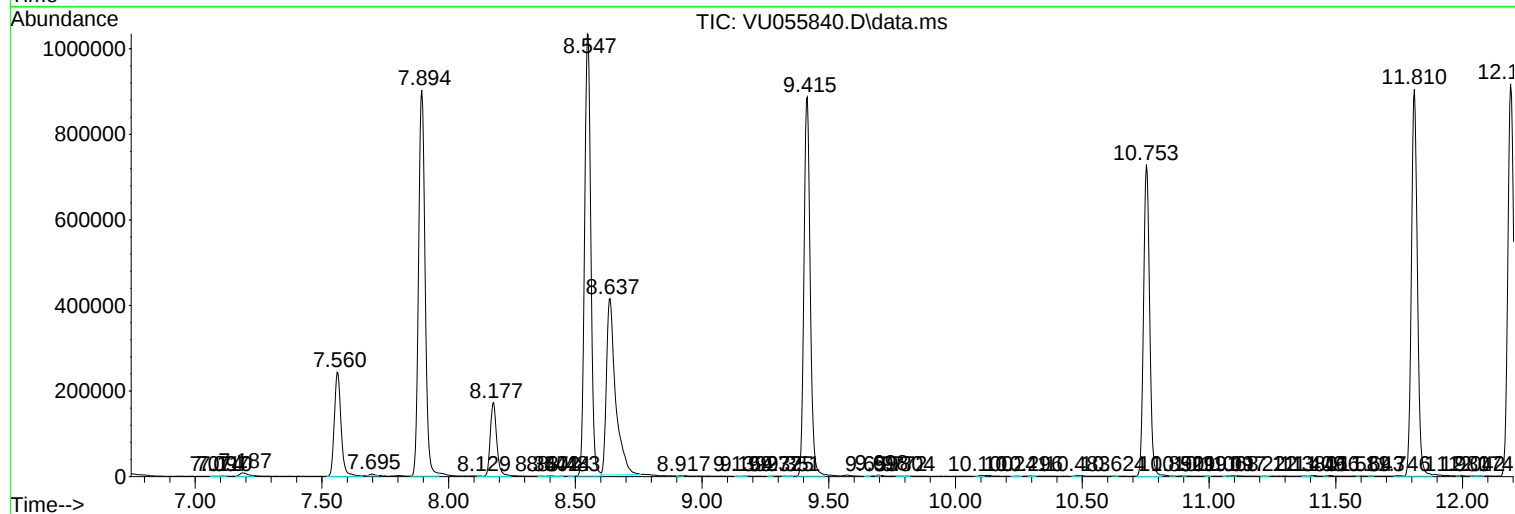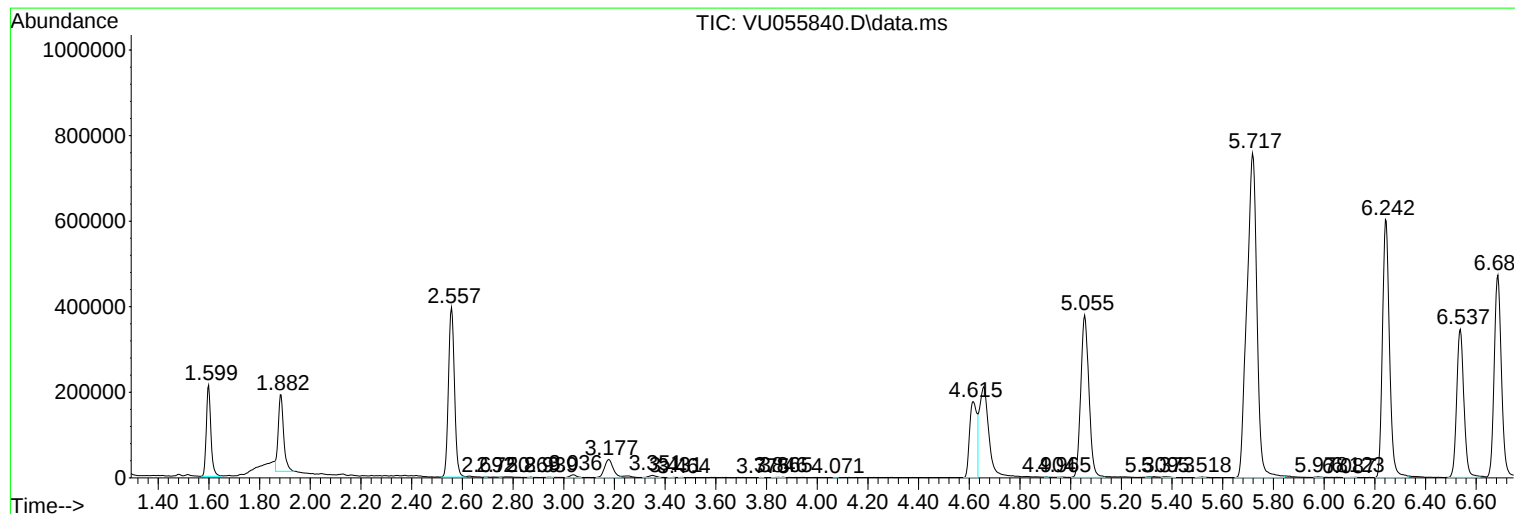

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055840.D
Acq On : 20 Oct 2023 18:16
Operator : MD/SY
Sample : 04947-05DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055840.D
Acq On : 20 Oct 2023 18:16
Operator : MD/SY
Sample : 04947-05DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------