

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055841.D
 Acq On : 20 Oct 2023 18:40
 Operator : MD/SY
 Sample : 04947-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	110	rBV	202940	249935	12.34%	1.588%
2	1.882	178	184	206	rVB	182241	272172	13.44%	1.730%
3	2.557	381	394	411	rBV	390523	627214	30.97%	3.986%
4	2.676	428	431	433	rVB4	866	488	0.02%	0.003%
5	2.840	480	482	488	rVB3	758	569	0.03%	0.004%
6	2.869	488	491	495	rVB3	476	410	0.02%	0.003%
7	2.895	495	499	504	rBV2	591	652	0.03%	0.004%
8	2.920	504	507	510	rVB2	568	360	0.02%	0.002%
9	2.940	510	513	515	rBV2	480	338	0.02%	0.002%
10	3.033	533	542	556	rVB2	6753	12773	0.63%	0.081%
11	3.116	566	568	572	rBV	597	289	0.01%	0.002%
12	3.174	572	586	605	rBV	36472	87810	4.34%	0.558%
13	3.348	637	640	642	rBV2	462	337	0.02%	0.002%
14	3.403	654	657	659	rVB2	537	273	0.01%	0.002%
15	3.422	659	663	668	rVB2	292	278	0.01%	0.002%
16	3.473	676	679	684	rVB2	453	335	0.02%	0.002%
17	3.673	738	741	744	rVB3	638	330	0.02%	0.002%
18	3.740	758	762	764	rBV	379	316	0.02%	0.002%
19	3.872	799	803	808	rBV2	483	433	0.02%	0.003%
20	3.901	808	812	814	rBV2	406	286	0.01%	0.002%
21	3.997	838	842	846	rBV2	435	405	0.02%	0.003%
22	4.126	877	882	885	rVB	273	275	0.01%	0.002%
23	4.161	885	893	896	rBV	572	595	0.03%	0.004%
24	4.364	953	956	960	rVB2	432	308	0.02%	0.002%
25	4.499	994	998	1001	rBV2	409	382	0.02%	0.002%
26	4.615	1022	1034	1075	rBV	168048	489379	24.16%	3.110%
27	4.962	1140	1142	1145	rBV3	468	311	0.02%	0.002%
28	5.055	1154	1171	1194	rBV	368378	819849	40.48%	5.210%
29	5.300	1243	1247	1248	rBV2	680	444	0.02%	0.003%
30	5.425	1282	1286	1288	rBV2	371	278	0.01%	0.002%
31	5.718	1355	1377	1402	rBV2	736471	2025212	100.00%	12.870%
32	5.972	1453	1456	1459	rVB2	970	652	0.03%	0.004%
33	6.110	1495	1499	1501	rBV3	503	359	0.02%	0.002%
34	6.126	1501	1504	1509	rBV2	371	307	0.02%	0.002%
35	6.152	1509	1512	1520	rVB3	763	720	0.04%	0.005%
36	6.242	1520	1540	1571	rBV	597942	1168994	57.72%	7.429%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055841.D
 Acq On : 20 Oct 2023 18:40
 Operator : MD/SY
 Sample : 04947-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.415	1591	1594	1598	rVB3	1083	760	0.04%	0.005%
38	6.441	1598	1602	1604	rBV2	432	343	0.02%	0.002%
39	6.531	1618	1630	1643	rBV5	23951	50704	2.50%	0.322%
40	6.615	1654	1656	1662	rVB4	882	846	0.04%	0.005%
41	6.685	1662	1678	1703	rBV	467374	927355	45.79%	5.893%
42	6.836	1723	1725	1730	rVB4	1423	1160	0.06%	0.007%
43	6.862	1730	1733	1737	rBV3	628	610	0.03%	0.004%
44	7.090	1801	1804	1809	rVB	597	422	0.02%	0.003%
45	7.132	1809	1817	1819	rBV2	328	364	0.02%	0.002%
46	7.187	1822	1834	1848	rBV5	7898	18167	0.90%	0.115%
47	7.386	1893	1896	1898	rBV2	417	312	0.02%	0.002%
48	7.431	1909	1910	1917	rVB2	532	364	0.02%	0.002%
49	7.473	1919	1923	1924	rBV	466	276	0.01%	0.002%
50	7.560	1938	1950	1978	rVV	241460	438140	21.63%	2.784%
51	7.695	1985	1992	2000	rBV5	3621	6363	0.31%	0.040%
52	7.785	2016	2020	2024	rVB3	587	459	0.02%	0.003%
53	7.894	2040	2054	2084	rBV	889423	1555325	76.80%	9.884%
54	8.174	2130	2141	2172	rVV	166725	294920	14.56%	1.874%
55	8.550	2249	2258	2269	rVB3	13883	23623	1.17%	0.150%
56	8.634	2269	2284	2326	rBV2	404978	1038354	51.27%	6.599%
57	8.878	2357	2360	2362	rBV3	710	413	0.02%	0.003%
58	8.894	2362	2365	2371	rVB4	773	625	0.03%	0.004%
59	8.939	2374	2379	2380	rBV3	424	342	0.02%	0.002%
60	8.978	2388	2391	2393	rBV2	673	388	0.02%	0.002%
61	9.045	2409	2412	2414	rBV2	644	334	0.02%	0.002%
62	9.094	2420	2427	2434	rBV4	554	751	0.04%	0.005%
63	9.126	2434	2437	2442	rVB3	622	544	0.03%	0.003%
64	9.177	2450	2453	2458	rVB3	539	429	0.02%	0.003%
65	9.200	2458	2460	2463	rBV2	460	306	0.02%	0.002%
66	9.415	2512	2527	2548	rBV	883367	1492649	73.70%	9.485%
67	9.573	2574	2576	2581	rVB3	826	423	0.02%	0.003%
68	9.698	2612	2615	2625	rVB6	1126	1535	0.08%	0.010%
69	9.823	2651	2654	2658	rBV2	425	293	0.01%	0.002%
70	9.949	2690	2693	2699	rBV	637	486	0.02%	0.003%
71	10.065	2724	2729	2730	rBV	531	320	0.02%	0.002%
72	10.225	2773	2779	2782	rVB	420	407	0.02%	0.003%
73	10.335	2810	2813	2816	rBV2	427	333	0.02%	0.002%
74	10.415	2834	2838	2842	rBV2	311	306	0.02%	0.002%
75	10.753	2930	2943	2968	rBV	727481	1201139	59.31%	7.633%
76	10.840	2968	2970	2975	rVB3	828	505	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
 Data File : VU055841.D
 Acq On : 20 Oct 2023 18:40
 Operator : MD/SY
 Sample : 04947-09 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	10.891	2981	2986	2988	rBV3	548	585	0.03%	0.004%
78	11.010	3020	3023	3026	rVV2	470	379	0.02%	0.002%
79	11.039	3029	3032	3037	rVB3	487	408	0.02%	0.003%
80	11.415	3143	3149	3155	rBV6	1627	2305	0.11%	0.015%
81	11.566	3193	3196	3200	rVV3	432	329	0.02%	0.002%
82	11.669	3225	3228	3231	rBV	445	318	0.02%	0.002%
83	11.811	3259	3272	3292	rBV	861522	1432135	70.72%	9.101%
84	12.042	3341	3344	3348	rVB3	999	735	0.04%	0.005%
85	12.190	3377	3390	3419	rVV	886228	1464698	72.32%	9.308%
86	12.331	3432	3434	3438	rVB3	649	339	0.02%	0.002%
87	12.534	3493	3497	3502	rBV5	755	717	0.04%	0.005%
88	12.585	3510	3513	3519	rBV3	778	909	0.04%	0.006%
89	12.984	3634	3637	3639	rBV	611	484	0.02%	0.003%
90	13.036	3650	3653	3655	rBV2	487	319	0.02%	0.002%
91	13.052	3655	3658	3660	rVV3	479	274	0.01%	0.002%
92	13.155	3686	3690	3692	rBV	561	376	0.02%	0.002%
93	13.431	3774	3776	3778	rBV2	587	306	0.02%	0.002%
94	13.589	3819	3825	3827	rBV2	921	1109	0.05%	0.007%
95	13.749	3872	3875	3878	rBV2	625	424	0.02%	0.003%
96	14.187	4007	4011	4014	rBV3	889	979	0.05%	0.006%
97	14.521	4112	4115	4117	rBV2	630	317	0.02%	0.002%
98	14.852	4216	4218	4220	rBV2	839	392	0.02%	0.002%
99	14.968	4250	4254	4259	rBV6	1070	1214	0.06%	0.008%
100	15.309	4357	4360	4362	rBV2	1053	606	0.03%	0.004%




Sum of corrected areas: 15736120

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055841.D
Acq On : 20 Oct 2023 18:40
Operator : MD/SY
Sample : 04947-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

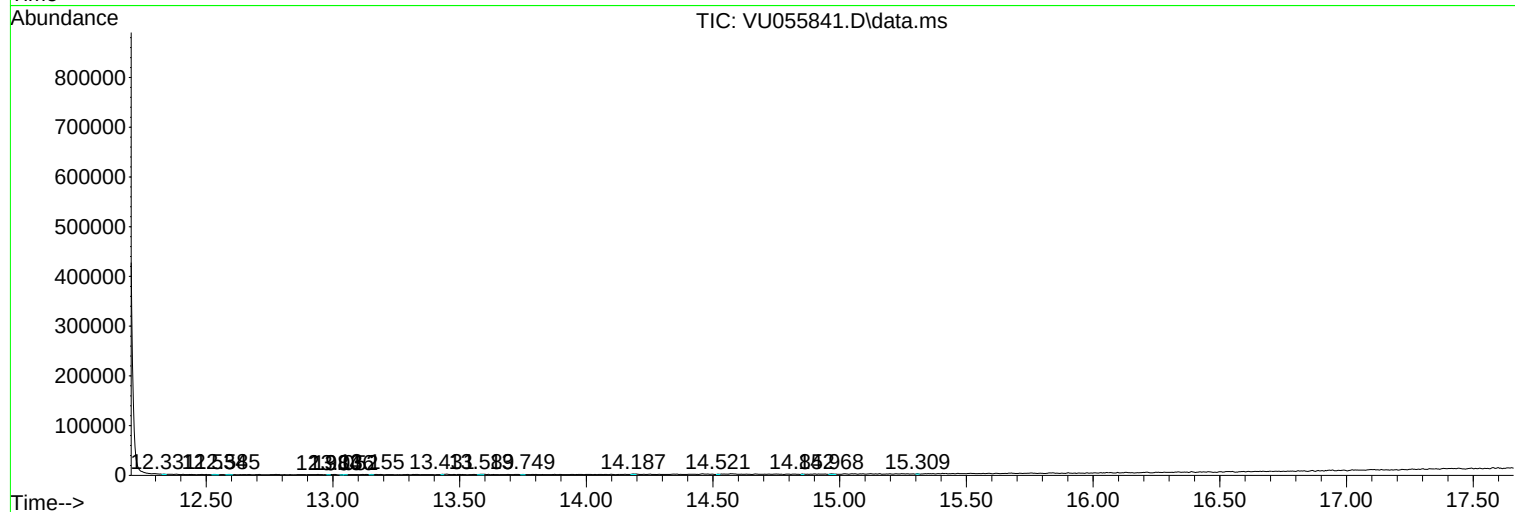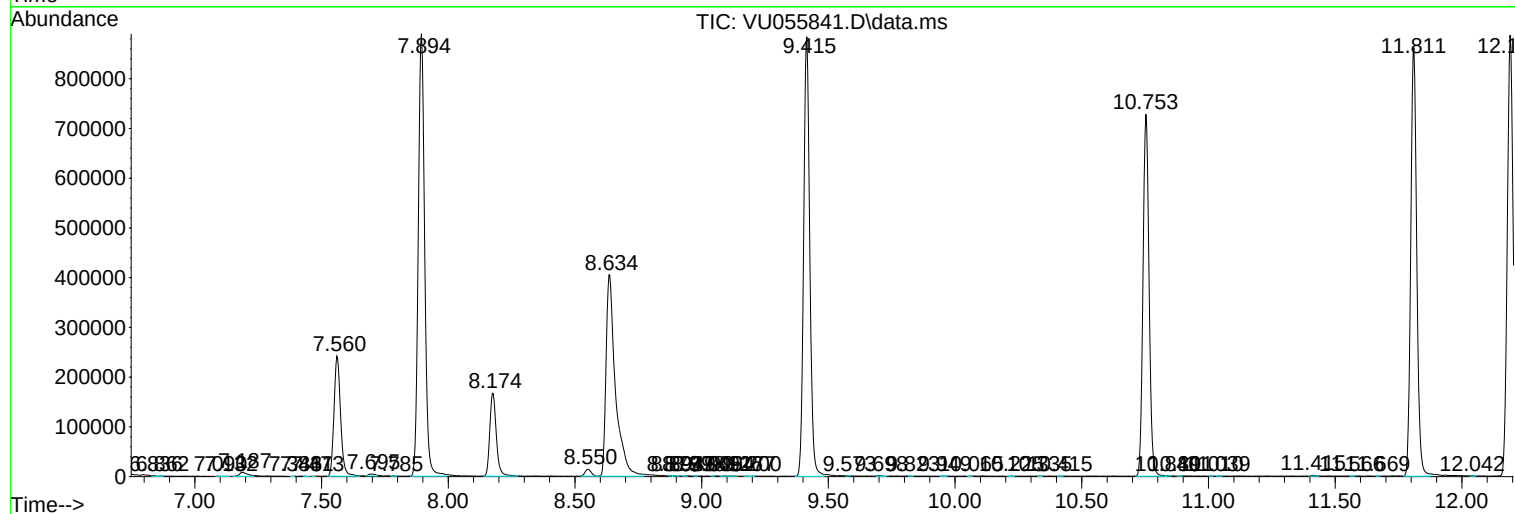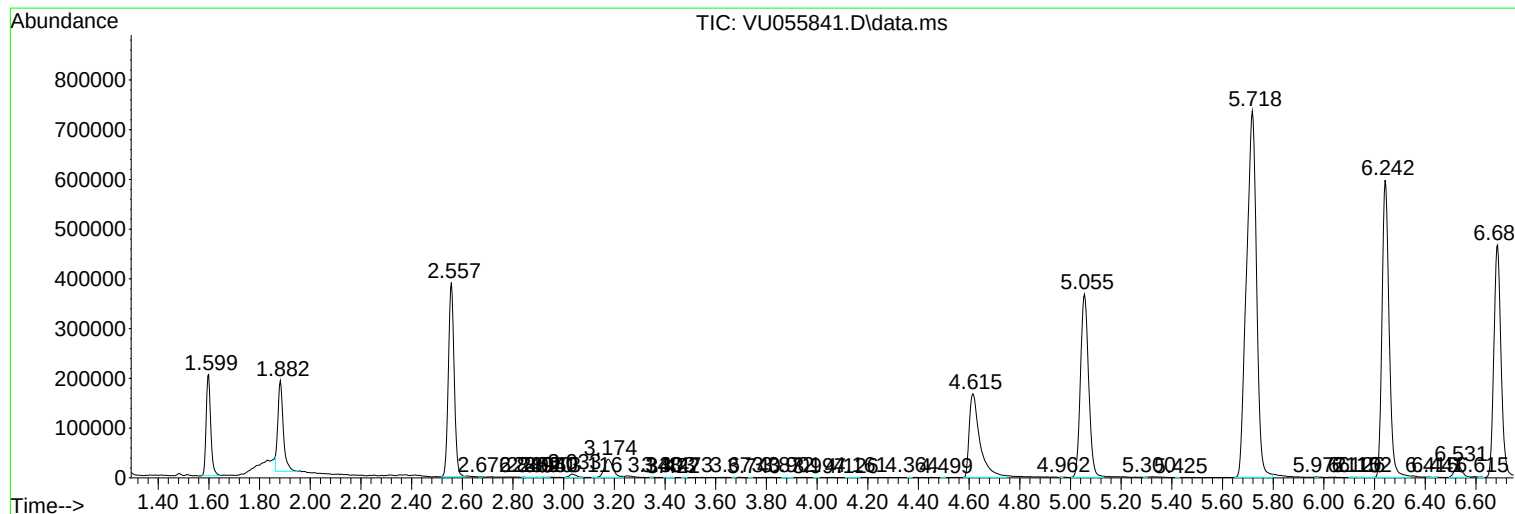

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055841.D
Acq On : 20 Oct 2023 18:40
Operator : MD/SY
Sample : 04947-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055841.D
Acq On : 20 Oct 2023 18:40
Operator : MD/SY
Sample : 04947-09 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------