


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102023\
Data File : VU055818.D
Acq On : 20 Oct 2023 08:34
Operator : MD/SY
Sample : BFB025
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB025

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Title : VOC Analysis
Last Update : Thu Oct 26 01:50:39 2023

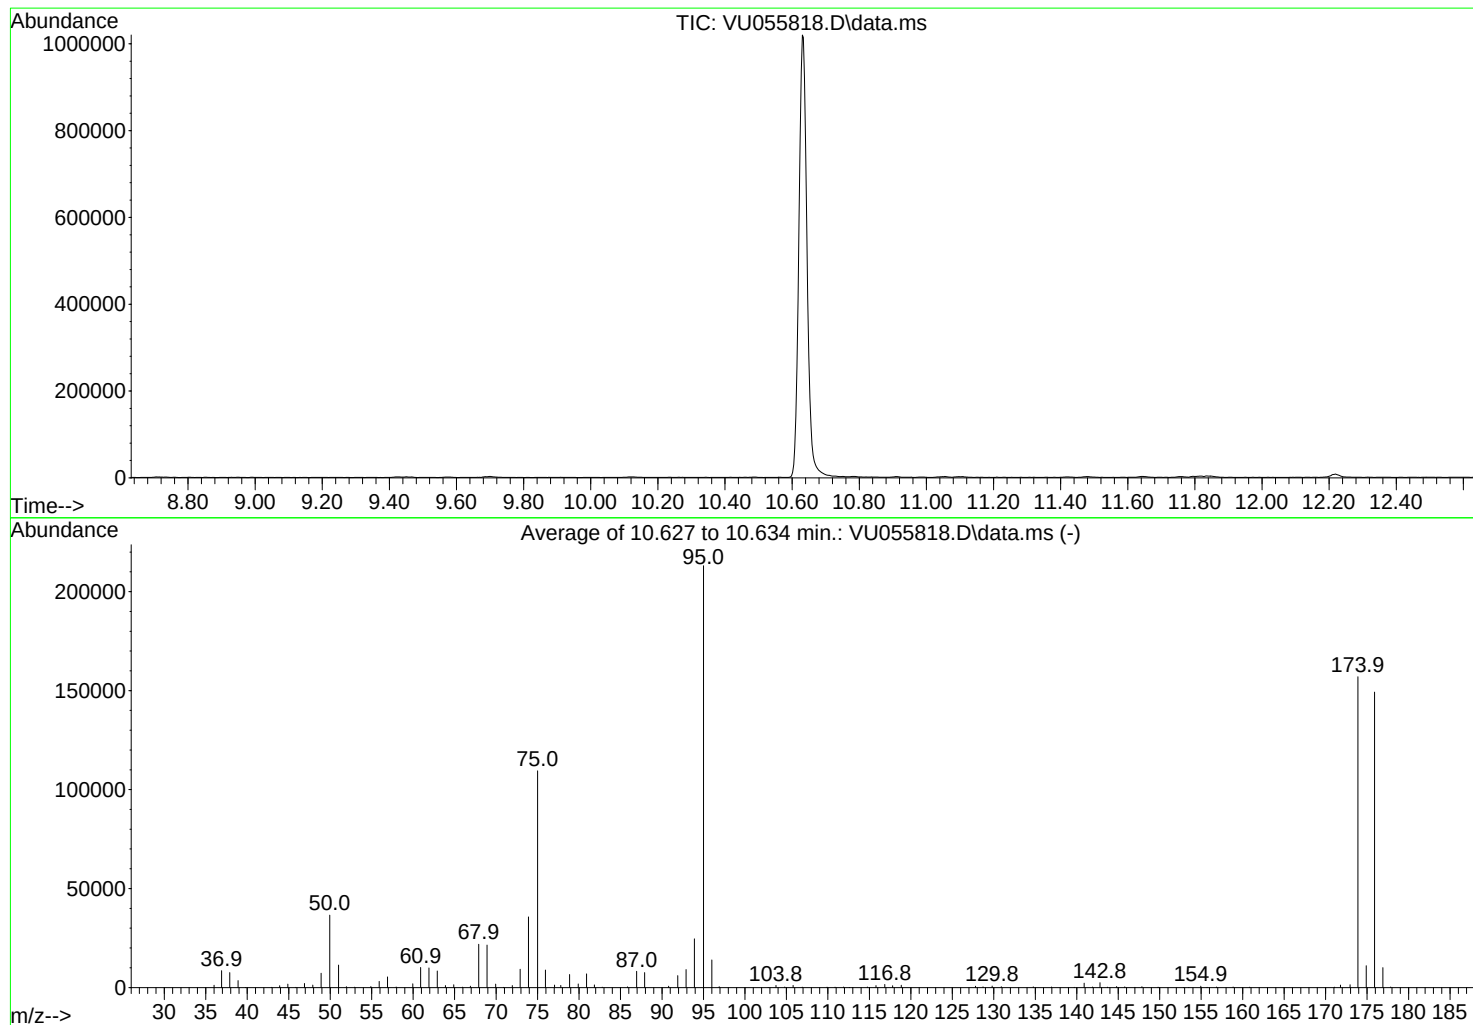

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	36597	PASS
75	95	30	80	51.4	109453	PASS
95	95	100	100	100.0	213077	PASS
96	95	5	9	6.6	13960	PASS
173	174	0.00	2	0.9	1391	PASS
174	95	50	120	73.7	157035	PASS
175	174	5	9	7.0	11023	PASS
176	174	95	101	95.0	149227	PASS
177	176	5	9	6.7	10072	PASS

m/z	Abundance
39.80	299.0
43.90	777.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
36.00	1183.0
36.90	8051.0
37.90	7495.0
38.90	3347.0
39.80	310.0
42.90	131.0
43.90	1663.0
44.90	1625.0
45.80	159.0
46.90	1886.0
47.90	1129.0
48.90	7203.0
49.90	35296.0
51.00	11408.0
51.90	454.0
53.00	158.0
54.90	537.0
55.90	2994.0
56.90	5338.0
57.90	257.0
59.90	1982.0
60.90	9512.0
61.90	9160.0
62.90	8122.0
63.90	948.0
64.90	1324.0
66.00	143.0
66.90	727.0
67.90	20296.0
68.90	20632.0
70.00	1706.0
70.90	113.0
71.90	827.0
72.90	8877.0
73.90	34264.0
75.00	103736.0
75.90	8504.0
77.10	1206.0
77.80	1053.0
78.90	6359.0
79.90	1778.0
80.90	6762.0
81.80	1355.0
82.80	209.0
85.90	282.0
87.00	7475.0
87.90	7100.0
90.80	659.0
91.90	5499.0
92.90	8796.0
93.90	23608.0
95.00	203648.0
96.00	13572.0
96.90	359.0
102.80	109.0
103.80	989.0
104.80	262.0
105.80	972.0
106.90	177.0
109.90	169.0
110.90	137.0
111.80	334.0
112.60	161.0
113.10	101.0
114.80	236.0
115.80	869.0
116.90	1555.0
117.80	923.0
118.90	1098.0
127.80	533.0
128.70	328.0
129.80	674.0
130.90	515.0
134.80	349.0
136.90	319.0
139.60	110.0
140.90	2323.0
142.00	319.0
142.80	2393.0
143.70	203.0
144.80	467.0
145.80	283.0
147.00	145.0
147.80	433.0
149.80	244.0
154.90	644.0
155.70	130.0
156.80	280.0
158.80	250.0
160.80	220.0
171.00	186.0
171.80	1128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

173.00	1353.0
173.90	145408.0
174.90	10363.0
175.90	137408.0
176.90	9607.0
177.80	206.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
36.00	1233.0
36.90	8650.0
37.90	7900.0
38.90	3724.0
39.80	407.0
42.90	145.0
43.90	1783.0
44.90	1752.0
45.80	127.0
46.90	2179.0
47.90	1304.0
48.90	7429.0
49.90	37760.0
51.00	11717.0
51.90	477.0
53.00	190.0
54.90	592.0
55.90	3303.0
56.90	5622.0
57.90	314.0
60.00	2016.0
60.90	10490.0
61.90	10195.0
62.90	8659.0
63.90	998.0
64.90	1497.0
66.00	209.0
66.90	709.0
67.90	22640.0
68.90	22248.0
70.00	1778.0
70.90	147.0
72.00	1027.0
72.90	9534.0
73.90	36880.0
75.00	113120.0
76.00	8997.0
77.00	1317.0
77.80	1169.0
78.80	6782.0
79.90	1847.0
80.90	7174.0
81.80	1311.0
82.80	236.0
85.90	399.0
86.90	8400.0
87.90	7669.0
90.80	703.0
91.90	6201.0
92.90	9329.0
93.90	25392.0
95.00	219072.0
96.00	14272.0
96.90	435.0
103.70	1110.0
104.80	307.0
105.80	1092.0
106.90	186.0
109.90	178.0
110.80	202.0
111.90	325.0
114.70	260.0
115.80	1063.0
116.80	1717.0
117.80	968.0
118.80	1105.0
127.80	716.0
128.70	349.0
129.80	769.0
130.90	426.0
134.80	357.0
136.90	313.0
139.70	116.0
140.90	2310.0
141.90	293.0
142.80	2602.0
143.70	190.0
144.80	511.0
145.80	349.0
147.00	172.0
147.80	480.0
149.80	190.0
152.80	125.0
154.90	735.0
155.70	171.0
156.90	299.0
158.90	293.0
160.80	221.0
171.10	216.0
171.80	1244.0
173.00	1422.0
173.90	162048.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

174.90	11209.0
175.90	153664.0
176.90	10341.0
177.90	275.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
36.00	1214.0
36.90	8836.0
37.90	7388.0
38.90	3534.0
39.80	427.0
42.90	121.0
43.90	1780.0
44.90	1749.0
45.90	136.0
46.90	2157.0
47.90	1273.0
48.90	7170.0
50.00	36736.0
51.00	11046.0
52.00	455.0
52.90	190.0
54.90	569.0
55.90	3166.0
56.90	5235.0
58.00	317.0
60.00	1773.0
60.90	10417.0
61.90	10328.0
62.90	8276.0
63.90	1115.0
64.90	1545.0
65.90	217.0
66.90	648.0
67.90	22632.0
68.90	21592.0
69.90	1739.0
70.90	135.0
72.00	1130.0
72.90	9289.0
73.90	35808.0
75.00	111504.0
76.00	9041.0
77.00	1261.0
77.80	1075.0
78.80	6614.0
79.90	1764.0
80.90	6940.0
81.90	1264.0
82.80	249.0
85.80	404.0
86.90	8789.0
87.90	7837.0
90.80	728.0
91.90	6294.0
92.90	9117.0
93.90	24744.0
95.00	216512.0
96.00	14035.0
96.90	437.0
103.80	1108.0
104.80	348.0
105.80	1105.0
106.90	232.0
109.90	161.0
110.80	243.0
112.00	250.0
112.90	151.0
114.70	286.0
115.80	1008.0
116.80	1566.0
117.80	836.0
118.80	1226.0
127.80	900.0
128.70	343.0
129.80	869.0
130.80	298.0
134.70	346.0
137.00	310.0
139.80	140.0
140.90	1988.0
141.80	292.0
142.80	2531.0
143.70	144.0
144.80	564.0
145.80	353.0
147.00	180.0
147.90	481.0
149.80	132.0
152.90	121.0
153.50	113.0
155.00	684.0
155.70	139.0
156.90	260.0
158.90	318.0
160.90	207.0
171.10	151.0
171.80	1363.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

172.90	1398.0
173.90	163648.0
174.90	11496.0
175.90	156608.0
176.90	10269.0
177.90	353.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025