


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102119\
Data File : VU035319.D
Acq On : 21 Oct 2019 08:36
Operator : JC/SP
Sample : BFB45
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB45

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM101919WMA.M
Title : VOC Analysis
Last Update : Tue Oct 22 16:41:37 2019

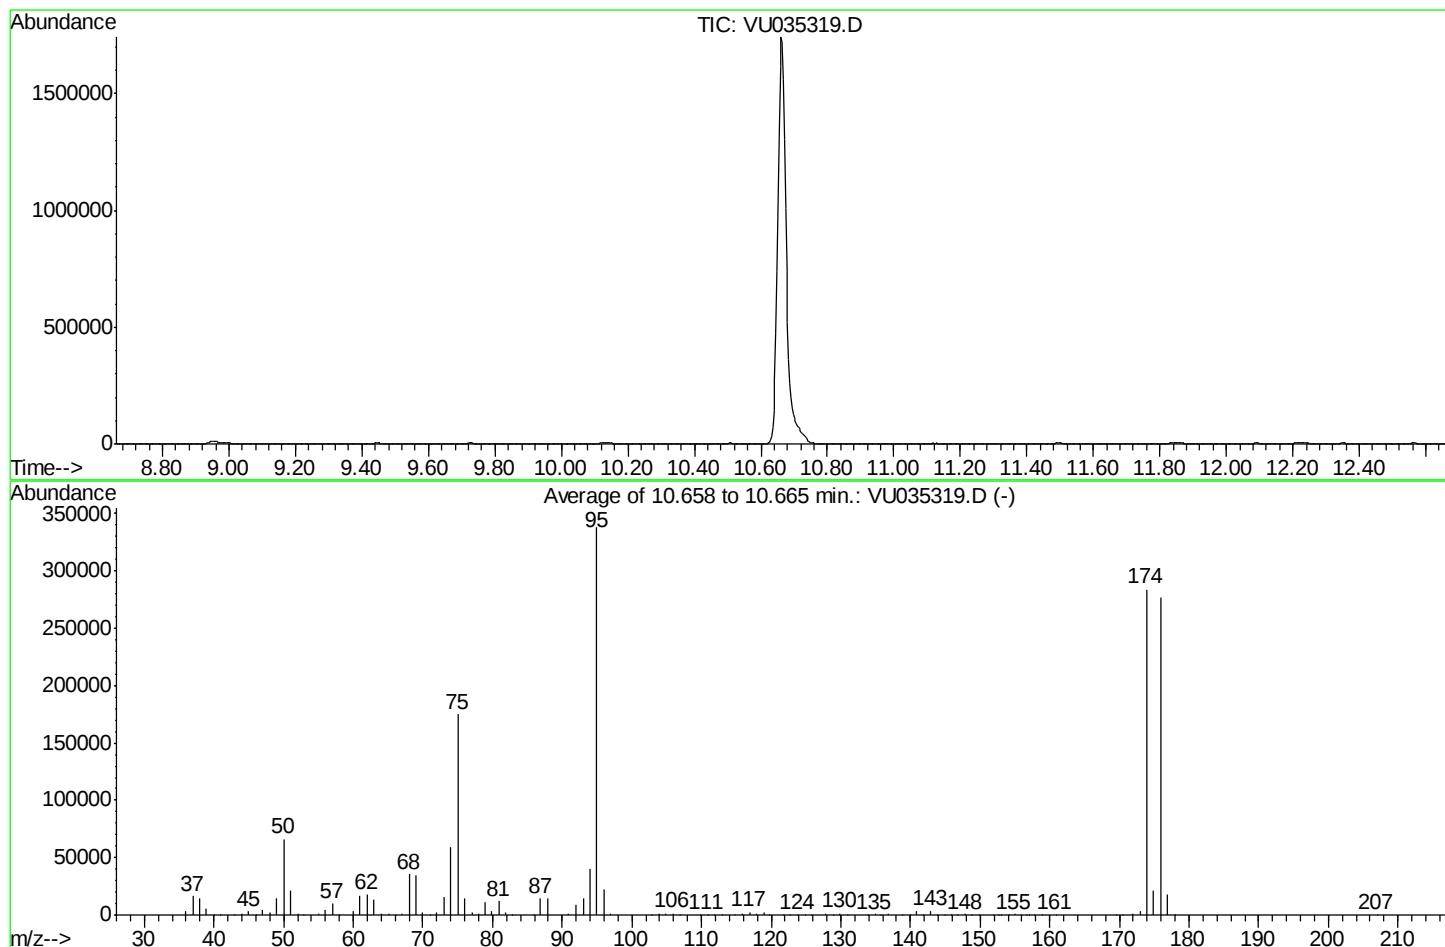

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	66360	PASS
75	95	30	80	51.8	175189	PASS
95	95	100	100	100.0	338048	PASS
96	95	5	9	6.7	22770	PASS
173	174	0.00	2	1.0	2925	PASS
174	95	50	120	83.9	283690	PASS
175	174	5	9	7.3	20792	PASS
176	174	95	101	97.4	276394	PASS
177	176	5	9	6.5	18048	PASS

m/z	Abundance
36.00	3423.0
37.00	15983.0
38.00	14478.0
39.00	5471.0
40.00	321.0
40.90	161.0
42.90	311.0
44.00	2757.0
45.00	2831.0
46.00	300.0
47.00	3825.0
48.00	2384.0
49.00	14228.0
50.00	64344.0
51.00	20632.0
52.00	884.0
52.90	215.0
55.00	970.0
56.00	4895.0
57.00	9312.0
58.00	459.0
60.00	2915.0
61.00	17000.0
62.00	17320.0
63.00	12720.0
64.00	1284.0
65.00	991.0
66.00	166.0
67.00	867.0
68.00	34680.0
69.00	33744.0
70.00	2793.0
71.00	140.0
72.00	1830.0
73.00	15098.0
74.00	56504.0
75.00	167872.0
76.00	14001.0
77.00	2048.0
77.90	1521.0
78.90	10910.0
79.90	3423.0
80.90	11549.0
81.90	2580.0
82.90	192.0
86.00	516.0
86.90	13762.0
87.90	13341.0
90.90	1352.0
92.00	9200.0
93.00	13641.0
94.00	39184.0
95.00	324928.0
96.00	21848.0
97.00	650.0
102.80	213.0
103.90	1344.0
104.80	662.0
105.90	1537.0
106.80	333.0
109.70	137.0
110.80	335.0
111.80	234.0
112.90	259.0
114.80	377.0
115.90	1307.0
116.90	2271.0
117.90	1373.0
118.90	1835.0
119.80	125.0
121.80	108.0
123.80	152.0
125.70	191.0
127.90	1073.0
128.80	501.0
129.90	1194.0
130.80	422.0
134.90	641.0
135.80	190.0
136.90	607.0
138.80	135.0
139.80	219.0
140.90	3385.0
141.80	339.0
142.90	3347.0
143.80	204.0
144.90	310.0
145.80	444.0
146.70	201.0
147.80	712.0
148.90	256.0
149.90	303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

151.80	147.0
152.70	154.0
153.00	140.0
154.00	130.0
154.90	646.0
155.80	217.0
156.70	454.0
157.10	352.0
157.80	110.0
158.90	430.0
160.90	351.0
170.60	131.0
171.90	1656.0
173.00	2604.0
173.90	265600.0
174.90	20216.0
175.90	259008.0
176.90	17520.0
177.90	505.0
207.00	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	3553.0
37.00	17320.0
38.00	15087.0
39.00	6116.0
40.00	327.0
40.90	180.0
43.00	266.0
44.00	2748.0
45.00	2948.0
46.00	317.0
47.00	4318.0
48.00	2377.0
49.00	15089.0
50.00	68232.0
51.00	21464.0
52.00	961.0
52.90	178.0
55.00	1023.0
56.00	5173.0
57.00	10256.0
58.10	452.0
60.00	3245.0
61.00	17544.0
62.00	18528.0
63.00	13663.0
64.00	1375.0
65.00	1007.0
66.00	146.0
67.00	940.0
68.00	36616.0
69.00	35544.0
70.00	2755.0
72.00	1904.0
73.00	16364.0
74.00	60904.0
75.00	180672.0
76.00	14862.0
77.00	2083.0
78.00	1578.0
78.90	11951.0
79.90	3486.0
80.90	12447.0
81.90	2701.0
82.80	255.0
85.90	548.0
86.90	14722.0
87.90	14425.0
90.90	1465.0
92.00	9580.0
93.00	14856.0
94.00	42088.0
95.00	348224.0
96.00	23360.0
97.00	630.0
102.80	244.0
103.90	1434.0
104.80	651.0
105.90	1536.0
106.90	354.0
109.80	172.0
110.90	397.0
111.90	220.0
112.80	279.0
114.80	445.0
115.90	1211.0
116.90	2392.0
117.90	1491.0
118.90	1954.0
123.90	157.0
125.80	225.0
127.90	1146.0
128.90	574.0
129.90	1183.0
130.90	459.0
134.90	682.0
135.80	226.0
136.90	664.0
138.80	198.0
139.90	238.0
140.90	3626.0
141.80	367.0
142.90	3728.0
143.80	195.0
144.80	317.0
145.80	454.0
146.70	198.0
147.90	779.0
148.90	286.0
149.90	373.0
151.80	143.0
152.70	170.0
154.00	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

155.00	697.0
155.80	246.0
156.70	516.0
157.10	393.0
157.90	101.0
158.90	530.0
160.90	392.0
170.50	168.0
171.90	1658.0
173.00	2989.0
173.90	291968.0
174.90	21344.0
175.90	284288.0
176.90	18568.0
177.90	462.0
207.00	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	3393.0
37.00	16880.0
38.00	14629.0
39.00	6262.0
40.00	302.0
40.90	198.0
43.00	267.0
44.00	2755.0
45.00	2892.0
46.00	282.0
47.00	4314.0
48.00	2115.0
49.00	14617.0
50.00	66504.0
51.00	20376.0
52.00	899.0
52.80	140.0
55.00	1071.0
56.00	5045.0
57.00	10117.0
58.10	359.0
60.00	3288.0
61.00	16784.0
62.00	17680.0
63.00	13494.0
64.00	1421.0
65.10	878.0
66.00	102.0
67.00	911.0
68.00	35384.0
69.00	34928.0
70.00	2565.0
72.00	1781.0
73.00	16356.0
74.00	60528.0
75.00	177024.0
76.00	14551.0
77.00	1937.0
78.00	1519.0
78.90	11802.0
79.90	3521.0
80.90	12113.0
81.90	2626.0
82.80	287.0
85.90	482.0
86.90	14294.0
87.90	14599.0
90.90	1419.0
92.00	9466.0
93.00	14741.0
94.00	41032.0
95.00	340992.0
96.00	23104.0
97.00	612.0
102.90	247.0
103.90	1475.0
104.80	528.0
105.90	1442.0
106.90	368.0
109.80	185.0
110.90	368.0
112.00	224.0
112.80	263.0
114.80	479.0
115.90	1142.0
116.90	2344.0
117.90	1450.0
118.90	1937.0
122.70	100.0
123.90	162.0
124.90	119.0
125.80	223.0
127.90	1077.0
128.90	633.0
129.90	1198.0
130.90	499.0
133.90	104.0
134.90	587.0
135.80	184.0
136.90	636.0
138.80	202.0
140.00	232.0
140.90	3520.0
141.80	363.0
142.90	3888.0
143.80	166.0
144.80	303.0
145.80	460.0
146.70	176.0
148.00	926.0
148.80	271.0
149.90	396.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

151.80	112.0
152.70	188.0
154.00	107.0
154.90	741.0
155.90	238.0
156.80	498.0
158.80	526.0
160.80	389.0
169.60	103.0
170.40	207.0
171.90	1405.0
173.00	3182.0
173.90	293504.0
174.90	20816.0
175.90	285888.0
176.90	18056.0
177.90	403.0
206.90	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

Scan 2885 (10.616 min): VU035319.D
BFB45

m/z	Abundance
36.00	563.0
37.80	215.0
38.90	102.0
39.90	219.0
40.90	114.0
44.00	1062.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45