


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102120\
 Data File : VU040864.D
 Acq On : 21 Oct 2020 10:53
 Operator : SY/MD
 Sample : BFB61
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB61

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Oct 22 01:39:14 2020

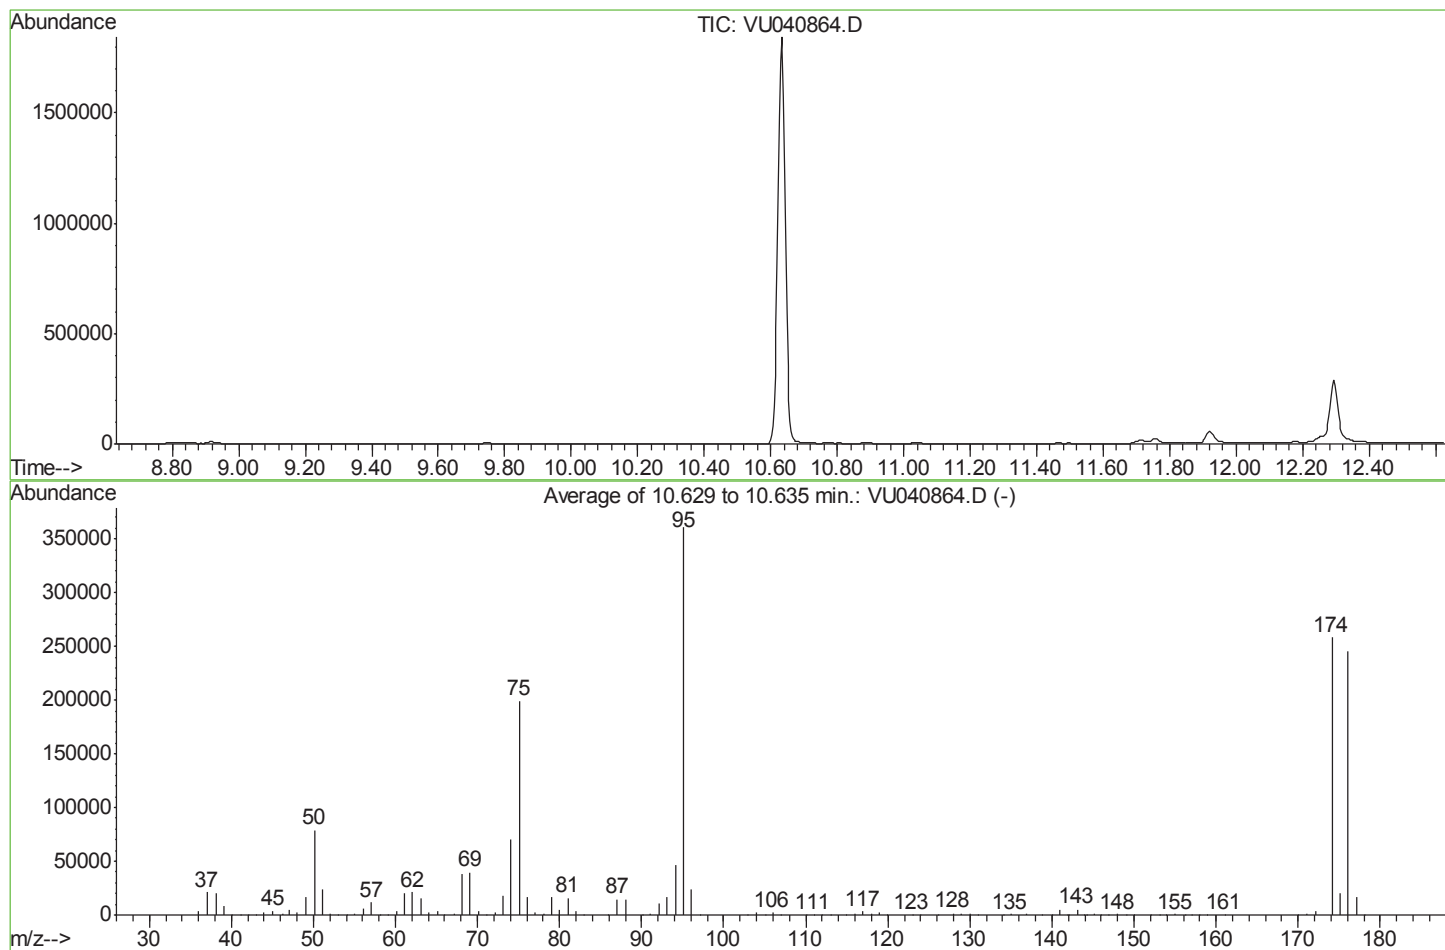

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2874

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.8	78752	PASS
75	95	30	80	55.2	199210	PASS
95	95	100	100	100.0	360704	PASS
96	95	5	9	6.7	24085	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.6	258261	PASS
175	174	5	9	7.8	20256	PASS
176	174	95	101	95.0	245440	PASS
177	176	5	9	6.6	16309	PASS

m/z	Abundance
36.00	3659.0
37.00	20928.0
38.10	19384.0
39.10	8136.0
40.10	666.0
41.10	235.0
43.00	454.0
44.00	3303.0
45.00	3514.0
46.20	687.0
47.10	4769.0
48.00	2380.0
49.10	16784.0
50.10	78408.0
51.10	24384.0
52.10	1175.0
53.00	430.0
54.00	231.0
55.00	1323.0
56.10	5841.0
57.10	11635.0
58.10	571.0
59.00	197.0
60.10	3538.0
61.10	19728.0
62.10	20448.0
63.10	15659.0
64.10	2655.0
65.10	3729.0
66.00	403.0
67.10	878.0
68.10	37488.0
69.10	38192.0
70.10	3437.0
71.10	231.0
72.10	2354.0
73.10	17888.0
74.10	68888.0
75.10	193472.0
76.10	17264.0
77.00	2312.0
78.10	1375.0
79.00	16888.0
80.00	4722.0
81.00	15749.0
82.00	4017.0
82.90	398.0
86.00	575.0
87.00	13678.0
88.10	13811.0
90.10	193.0
91.00	1479.0
92.10	10329.0
93.10	16904.0
94.10	45128.0
95.10	350848.0
96.10	23832.0
97.10	640.0
102.90	331.0
104.00	1761.0
105.10	393.0
105.90	1921.0
107.00	395.0
110.00	386.0
111.00	596.0
112.00	397.0
112.90	431.0
114.90	543.0
116.00	1485.0
117.00	2840.0
118.00	1619.0
119.00	2658.0
123.00	199.0
123.90	258.0
128.00	1604.0
129.00	788.0
130.00	1222.0
131.00	514.0
134.10	112.0
135.00	951.0
136.90	717.0
138.80	198.0
140.00	361.0
141.00	4197.0
141.90	438.0
143.10	5138.0
143.90	344.0
145.10	1225.0
146.00	532.0
146.90	305.0
148.00	814.0
149.10	265.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61

150.10	339.0
153.10	296.0
153.80	264.0
155.00	1113.0
156.20	166.0
157.00	521.0
157.90	149.0
158.80	346.0
161.00	436.0
171.00	863.0
172.10	4180.0
174.10	244224.0
175.10	19576.0
176.10	231744.0
177.10	15599.0
178.00	489.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61

m/z	Abundance
36.00	3951.0
37.00	21792.0
38.10	20608.0
39.10	8386.0
40.10	721.0
41.10	212.0
42.10	111.0
43.00	463.0
44.00	3528.0
45.00	3746.0
46.20	690.0
47.10	5324.0
48.10	2681.0
49.10	17440.0
50.10	81376.0
51.10	24968.0
52.10	1239.0
53.00	418.0
54.10	274.0
55.10	1361.0
56.00	6321.0
57.10	11957.0
58.00	498.0
59.10	200.0
60.10	3726.0
61.10	20368.0
62.10	21648.0
63.10	16358.0
64.10	2473.0
65.10	3588.0
66.00	314.0
67.10	856.0
68.10	39848.0
69.10	40776.0
70.10	3416.0
71.10	187.0
72.10	2675.0
73.10	19248.0
74.10	71992.0
75.10	205952.0
76.10	17848.0
77.00	2379.0
78.10	1427.0
79.00	17480.0
80.00	4582.0
81.00	16160.0
82.00	4152.0
83.00	449.0
86.00	514.0
87.10	15045.0
88.10	14756.0
90.20	152.0
91.00	1760.0
92.10	10515.0
93.10	17648.0
94.10	47464.0
95.10	372608.0
96.10	24648.0
97.00	636.0
102.90	284.0
104.00	2004.0
105.00	519.0
105.90	2065.0
107.00	407.0
110.00	311.0
111.00	447.0
112.00	447.0
113.00	574.0
114.90	481.0
116.00	1688.0
117.00	3149.0
118.00	1782.0
119.00	2781.0
119.90	101.0
123.00	147.0
124.00	183.0
126.10	144.0
128.00	1702.0
129.00	827.0
130.00	1595.0
131.00	704.0
135.00	937.0
136.90	754.0
138.80	201.0
139.90	351.0
141.00	4417.0
142.10	527.0
143.10	5057.0
144.10	325.0
145.10	1195.0
146.00	501.0
146.90	305.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61

148.00	860.0
149.10	399.0
150.10	381.0
152.00	108.0
153.00	281.0
153.80	251.0
155.00	1038.0
156.20	149.0
157.00	559.0
157.90	168.0
158.90	363.0
161.00	389.0
171.10	798.0
172.10	4281.0
174.10	265536.0
175.10	20688.0
176.10	252480.0
177.10	16720.0
178.00	486.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61

m/z	Abundance
36.00	3827.0
37.00	20440.0
38.10	19512.0
39.10	7880.0
40.10	691.0
41.20	149.0
42.10	157.0
43.00	423.0
44.00	3549.0
45.10	3537.0
46.20	569.0
47.10	5281.0
48.10	2688.0
49.10	16270.0
50.10	76472.0
51.10	22952.0
52.10	1195.0
53.10	449.0
54.10	263.0
55.10	1319.0
56.00	6137.0
57.10	11199.0
58.00	452.0
60.10	3674.0
61.10	19048.0
62.10	20896.0
63.10	15666.0
64.10	2062.0
65.10	3124.0
66.00	236.0
67.10	937.0
68.10	38776.0
69.10	39576.0
70.10	2906.0
70.90	173.0
72.10	2586.0
73.10	18392.0
74.10	68888.0
75.10	198208.0
76.10	16568.0
77.00	2104.0
78.10	1543.0
79.00	16648.0
80.00	4485.0
81.00	15198.0
82.00	3893.0
83.00	506.0
85.90	433.0
87.10	15050.0
88.10	14714.0
91.00	1854.0
92.10	10058.0
93.10	16648.0
94.10	45432.0
95.10	358656.0
96.10	23776.0
97.00	549.0
102.90	233.0
103.90	2007.0
105.00	646.0
106.00	2123.0
106.90	365.0
110.00	254.0
111.00	352.0
112.00	418.0
113.00	615.0
114.90	368.0
116.00	1620.0
117.00	3191.0
118.00	1729.0
119.00	2573.0
124.00	155.0
126.10	131.0
128.00	1596.0
129.00	776.0
130.00	1685.0
131.00	680.0
134.00	104.0
135.00	778.0
136.90	729.0
138.70	146.0
139.90	337.0
141.00	4199.0
142.10	610.0
143.00	4718.0
144.20	369.0
145.10	1008.0
145.90	456.0
146.90	287.0
148.00	824.0
149.10	376.0
150.00	361.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61

152.00	130.0
153.00	252.0
153.90	217.0
155.00	798.0
156.20	107.0
157.00	610.0
157.90	169.0
158.90	317.0
161.00	320.0
170.00	118.0
171.10	634.0
172.10	3816.0
174.10	265024.0
175.10	20504.0
176.10	252096.0
177.10	16608.0
178.10	425.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61

Scan 2874 (10.581 min): VU040864.D
BFB61

m/z	Abundance
40.00	307.0
41.10	130.0
43.00	204.0
44.00	831.0

Instrument :
MSVOA_U
ClientSampleId :
BFB61