


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102120\
 Data File : VU040898.D
 Acq On : 22 Oct 2020 09:45
 Operator : SY/MD
 Sample : BFB26
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB26

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Oct 22 23:17:57 2020

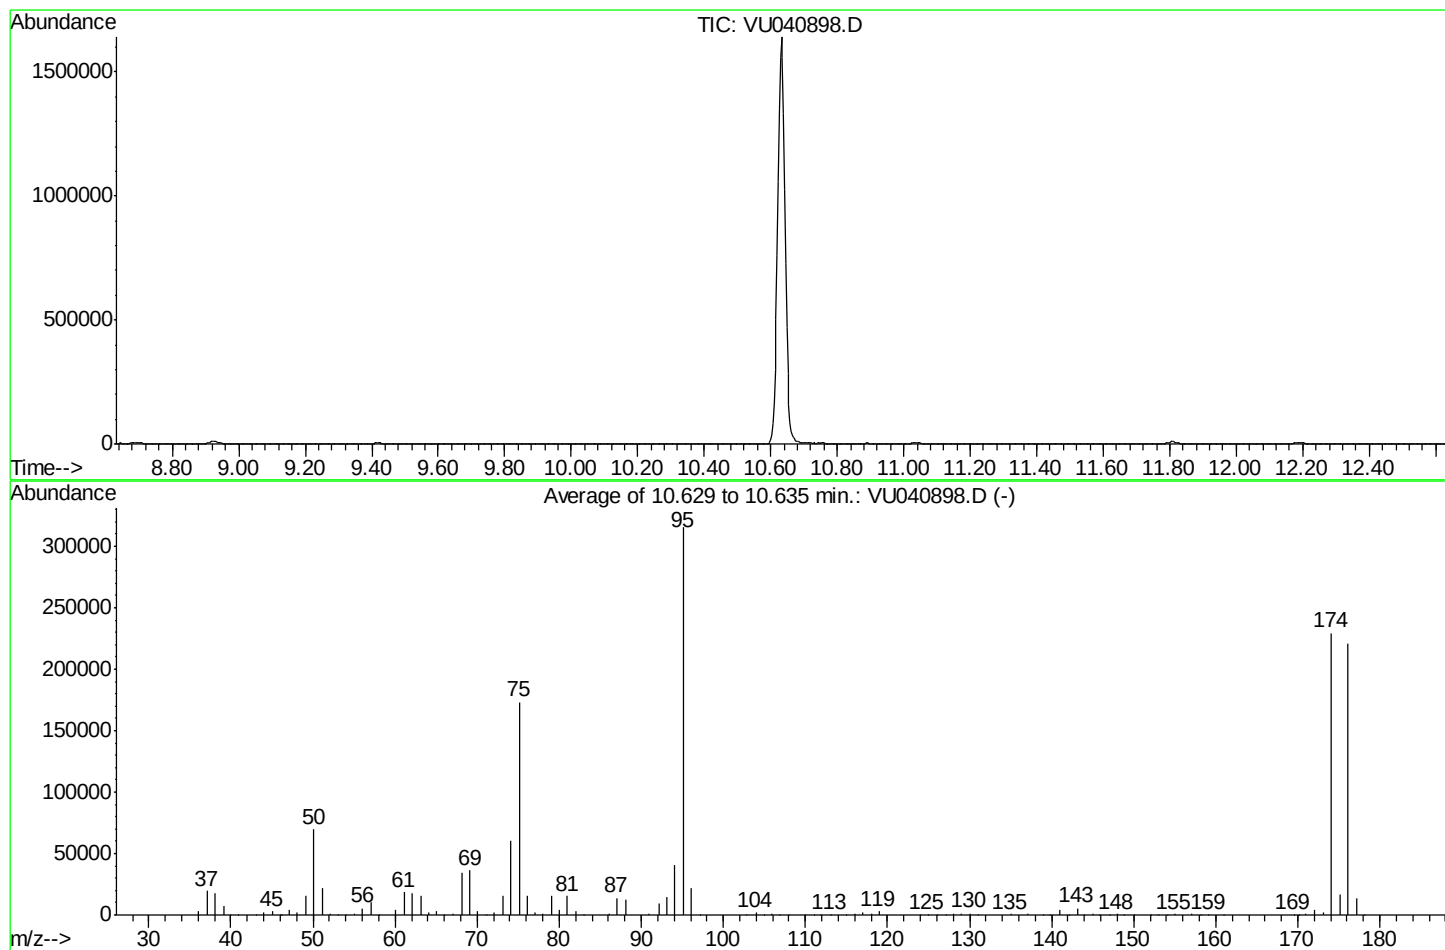

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	69413	PASS
75	95	30	80	54.8	172928	PASS
95	95	100	100	100.0	315434	PASS
96	95	5	9	6.9	21629	PASS
173	174	0.00	2	1.0	2307	PASS
174	95	50	120	72.7	229312	PASS
175	174	5	9	7.2	16546	PASS
176	174	95	101	96.4	220949	PASS
177	176	5	9	6.2	13771	PASS

m/z	Abundance
36.00	3724.0
37.10	19792.0
38.10	17352.0
39.10	7863.0
39.90	643.0
40.90	235.0
43.00	226.0
44.10	3085.0
45.00	3122.0
46.00	506.0
47.00	4166.0
48.00	2017.0
49.10	15595.0
50.10	70616.0
51.10	21400.0
52.00	786.0
53.00	345.0
53.90	215.0
55.00	1138.0
56.10	5787.0
57.10	10130.0
58.00	417.0
60.10	3814.0
61.10	18352.0
62.10	17584.0
63.10	15037.0
64.00	2224.0
65.10	3034.0
66.00	335.0
67.10	1265.0
68.10	34632.0
69.10	35600.0
70.00	2628.0
71.10	267.0
72.00	1683.0
73.10	15081.0
74.10	60472.0
75.10	172608.0
76.10	15463.0
77.10	2213.0
78.00	1288.0
79.00	15597.0
80.00	4418.0
81.00	15959.0
82.00	3186.0
83.10	329.0
86.20	637.0
87.00	13511.0
88.00	12308.0
91.00	1502.0
92.10	9702.0
93.10	14661.0
94.10	40560.0
95.10	310592.0
96.10	22120.0
97.10	572.0
102.90	236.0
104.00	1774.0
105.00	410.0
105.90	1489.0
106.90	313.0
108.00	245.0
109.90	114.0
111.10	444.0
111.90	267.0
113.00	512.0
114.90	498.0
116.00	1368.0
117.00	2336.0
118.00	1432.0
119.00	2871.0
124.90	181.0
126.00	112.0
127.10	133.0
128.00	955.0
129.00	684.0
130.00	1103.0
131.00	427.0
135.10	544.0
137.10	575.0
141.00	3455.0
142.00	375.0
143.10	5336.0
144.10	338.0
145.10	1610.0
145.90	445.0
147.00	305.0
148.00	593.0
148.80	301.0
150.00	212.0
152.00	118.0
153.00	245.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

155.00	718.0
157.00	752.0
159.10	469.0
161.00	251.0
169.50	121.0
170.10	216.0
171.00	571.0
172.10	3717.0
174.10	220736.0
175.10	15799.0
176.10	212096.0
177.10	13568.0
178.10	397.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.10	3702.0
37.10	20216.0
38.10	18080.0
39.10	7998.0
39.90	700.0
40.90	204.0
43.00	230.0
44.10	3207.0
45.10	2965.0
45.90	491.0
46.20	475.0
47.10	4042.0
48.00	2006.0
49.10	15953.0
50.10	71712.0
51.10	22520.0
52.00	653.0
52.90	320.0
53.90	136.0
55.00	1186.0
56.00	5815.0
57.00	11033.0
58.00	443.0
60.10	3997.0
61.10	19008.0
62.10	18120.0
63.10	15650.0
64.10	2015.0
65.10	3014.0
66.00	315.0
67.00	1201.0
68.10	35968.0
69.10	37856.0
70.10	2753.0
71.20	279.0
72.00	1710.0
73.10	15637.0
74.10	62480.0
75.10	178240.0
76.10	15851.0
77.00	2213.0
78.00	1160.0
79.00	15843.0
80.00	4634.0
81.00	15941.0
82.00	3110.0
83.00	336.0
86.10	633.0
87.00	14398.0
88.00	12546.0
91.00	1566.0
92.10	10034.0
93.10	15427.0
94.10	42616.0
95.10	326528.0
96.10	22320.0
97.10	570.0
102.80	212.0
104.00	1866.0
104.90	463.0
106.00	1612.0
106.90	364.0
108.00	220.0
110.00	143.0
111.00	486.0
111.90	308.0
113.00	560.0
114.90	564.0
116.00	1469.0
117.00	2751.0
118.00	1503.0
119.00	3058.0
124.00	102.0
124.90	170.0
125.90	165.0
127.00	102.0
128.00	1026.0
129.00	588.0
130.00	1152.0
131.00	469.0
135.00	566.0
137.10	628.0
139.70	101.0
141.00	3931.0
142.10	369.0
143.10	5599.0
144.00	354.0
145.10	1607.0
145.80	492.0
147.00	341.0
148.00	636.0
148.90	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

150.00	295.0
152.00	121.0
153.00	318.0
154.20	146.0
155.00	828.0
157.00	729.0
158.10	111.0
159.10	550.0
161.00	284.0
170.10	286.0
170.90	590.0
172.10	4057.0
173.10	3468.0
174.10	237056.0
175.10	16896.0
176.10	228544.0
177.10	14027.0
178.10	408.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.10	3279.0
37.10	18592.0
38.10	16808.0
39.10	7245.0
39.90	609.0
40.90	130.0
43.00	253.0
44.00	3067.0
45.10	2629.0
45.90	421.0
46.20	432.0
47.10	3729.0
48.00	1920.0
49.10	14426.0
50.10	65912.0
51.10	21688.0
52.10	581.0
52.90	258.0
55.00	1254.0
56.00	5287.0
57.00	10598.0
58.00	454.0
60.00	3506.0
61.10	17536.0
62.10	16688.0
63.10	14828.0
64.10	1895.0
65.10	2707.0
66.00	343.0
67.00	1007.0
68.10	34112.0
69.10	35896.0
70.10	2623.0
71.20	233.0
72.00	1678.0
73.10	15100.0
74.10	58304.0
75.10	167936.0
76.10	14773.0
77.00	2244.0
78.00	1032.0
79.00	14304.0
80.00	4199.0
81.00	14650.0
82.00	2950.0
83.00	313.0
86.10	495.0
87.00	13259.0
88.10	12039.0
91.00	1410.0
92.10	9666.0
93.10	14414.0
94.10	39600.0
95.10	309184.0
96.10	20448.0
97.20	512.0
102.80	151.0
104.00	1798.0
105.00	479.0
106.00	1620.0
106.90	368.0
108.00	123.0
110.00	161.0
111.00	458.0
111.90	299.0
113.00	491.0
114.90	455.0
116.00	1374.0
117.00	2748.0
118.00	1427.0
119.00	2773.0
124.00	138.0
124.90	129.0
125.90	203.0
128.00	1131.0
129.10	487.0
130.00	1105.0
131.00	411.0
134.90	679.0
137.00	576.0
139.00	105.0
139.70	116.0
141.00	4066.0
142.00	424.0
143.10	5125.0
143.90	377.0
145.10	1411.0
145.80	427.0
147.00	241.0
148.00	572.0
148.90	171.0
150.00	349.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

152.00	139.0
153.00	293.0
154.10	246.0
155.00	796.0
157.10	555.0
158.10	135.0
159.10	574.0
161.00	299.0
170.10	252.0
170.90	550.0
172.10	3836.0
173.10	3454.0
174.10	230144.0
175.10	16944.0
176.10	222208.0
177.10	13718.0
178.10	393.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

Scan 2874 (10.581 min): VU040898.D
BFB26

m/z	Abundance
40.00	374.0
43.10	100.0
44.00	868.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26