

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102122\
 Data File : VU051480.D
 Acq On : 21 Oct 2022 11:47
 Operator : JC/MD
 Sample : VU1021WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK004

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M

Title : VOC Analysis

Signal : TIC: VU051480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	242437	277726	14.61%	1.975%
2	1.899	165	174	197	rVB	185413	271438	14.28%	1.930%
3	2.507	359	363	368	rBV3	576	667	0.04%	0.005%
4	2.562	368	380	400	rBV	366559	606635	31.90%	4.314%
5	2.780	445	448	450	rBV2	1312	835	0.04%	0.006%
6	2.835	462	465	467	rBV2	512	295	0.02%	0.002%
7	2.938	493	497	498	rBV2	564	375	0.02%	0.003%
8	2.973	506	508	512	rVB2	523	330	0.02%	0.002%
9	3.041	521	529	542	rBV2	4973	9375	0.49%	0.067%
10	3.140	556	560	563	rBV	407	298	0.02%	0.002%
11	3.186	563	574	583	rVB4	2004	3968	0.21%	0.028%
12	3.227	583	587	593	rBV2	276	286	0.02%	0.002%
13	3.259	593	597	601	rBV2	418	466	0.02%	0.003%
14	3.478	662	665	671	rVB2	321	289	0.02%	0.002%
15	3.510	671	675	679	rVB2	260	271	0.01%	0.002%
16	3.658	715	721	727	rVB3	288	324	0.02%	0.002%
17	3.777	755	758	762	rBV	364	342	0.02%	0.002%
18	3.964	809	816	817	rBV2	289	321	0.02%	0.002%
19	4.083	848	853	856	rBV2	412	393	0.02%	0.003%
20	4.182	880	884	886	rBV	555	451	0.02%	0.003%
21	4.275	910	913	916	rBV2	342	276	0.01%	0.002%
22	4.382	941	946	950	rBV2	229	272	0.01%	0.002%
23	4.536	990	994	997	rBV2	413	284	0.01%	0.002%
24	4.616	1005	1019	1051	rBV	186235	463549	24.38%	3.296%
25	4.983	1128	1133	1136	rBV3	446	458	0.02%	0.003%
26	5.060	1140	1157	1180	rBV	346538	761101	40.03%	5.412%
27	5.282	1220	1226	1238	rBV5	1364	2546	0.13%	0.018%
28	5.362	1249	1251	1254	rBV3	542	289	0.02%	0.002%
29	5.478	1281	1287	1292	rBV	472	537	0.03%	0.004%
30	5.539	1300	1306	1310	rBV2	255	304	0.02%	0.002%
31	5.623	1328	1332	1336	rBV2	375	301	0.02%	0.002%
32	5.722	1341	1363	1393	rBV2	698277	1901426	100.00%	13.521%
33	6.086	1473	1476	1479	rBV2	388	344	0.02%	0.002%
34	6.105	1479	1482	1485	rVV2	400	273	0.01%	0.002%
35	6.163	1496	1500	1501	rBV	491	301	0.02%	0.002%
36	6.246	1508	1526	1552	rBV	577454	1097288	57.71%	7.803%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102122\
 Data File : VU051480.D
 Acq On : 21 Oct 2022 11:47
 Operator : JC/MD
 Sample : VU1021WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK004

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

37	6.462	1589	1593	1595	rBV3	425	299	0.02%	0.002%
38	6.523	1605	1612	1625	rVB7	3359	6327	0.33%	0.045%
39	6.587	1629	1632	1638	rBV3	523	473	0.02%	0.003%
40	6.687	1648	1663	1691	rBV	444368	875797	46.06%	6.228%
41	7.108	1786	1794	1798	rBV3	559	571	0.03%	0.004%
42	7.185	1810	1818	1831	rVB7	2064	4304	0.23%	0.031%
43	7.417	1885	1890	1893	rBV2	333	312	0.02%	0.002%
44	7.459	1900	1903	1908	rVB	356	297	0.02%	0.002%
45	7.565	1923	1936	1956	rBV	211744	380670	20.02%	2.707%
46	7.799	2000	2009	2016	rBV5	1126	1563	0.08%	0.011%
47	7.896	2025	2039	2057	rBV	806236	1392311	73.22%	9.900%
48	8.121	2106	2109	2112	rVB3	627	394	0.02%	0.003%
49	8.176	2113	2126	2145	rBV	151834	263093	13.84%	1.871%
50	8.327	2171	2173	2179	rVB3	469	354	0.02%	0.003%
51	8.401	2190	2196	2200	rBV4	788	820	0.04%	0.006%
52	8.423	2200	2203	2206	rBV3	383	318	0.02%	0.002%
53	8.471	2211	2218	2220	rVV2	341	481	0.03%	0.003%
54	8.536	2233	2238	2239	rBV3	375	349	0.02%	0.002%
55	8.632	2251	2268	2301	rBV2	548779	1040779	54.74%	7.401%
56	8.857	2336	2338	2344	rVB4	726	578	0.03%	0.004%
57	8.928	2357	2360	2364	rBV2	494	347	0.02%	0.002%
58	8.976	2370	2375	2379	rBV2	550	486	0.03%	0.003%
59	9.111	2414	2417	2422	rVB2	456	442	0.02%	0.003%
60	9.205	2440	2446	2448	rVV	463	450	0.02%	0.003%
61	9.285	2467	2471	2476	rVB3	372	343	0.02%	0.002%
62	9.333	2481	2486	2488	rBV2	447	400	0.02%	0.003%
63	9.414	2498	2511	2545	rBV	821048	1371609	72.14%	9.753%
64	9.603	2567	2570	2573	rVB3	715	460	0.02%	0.003%
65	9.693	2594	2598	2606	rVB5	1337	1743	0.09%	0.012%
66	9.758	2610	2618	2623	rBV3	502	819	0.04%	0.006%
67	9.822	2635	2638	2643	rBV	392	366	0.02%	0.003%
68	10.114	2726	2729	2730	rBV3	596	355	0.02%	0.003%
69	10.150	2737	2740	2749	rVB2	492	495	0.03%	0.004%
70	10.446	2829	2832	2835	rBV2	409	275	0.01%	0.002%
71	10.481	2838	2843	2848	rVV3	671	747	0.04%	0.005%
72	10.632	2884	2890	2900	rVB5	2092	3438	0.18%	0.024%
73	10.674	2900	2903	2908	rBV2	291	319	0.02%	0.002%
74	10.754	2914	2928	2953	rBV	678066	1089858	57.32%	7.750%
75	10.889	2967	2970	2973	rBV4	491	363	0.02%	0.003%
76	10.918	2977	2979	2990	rVB3	615	826	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102122\
 Data File : VU051480.D
 Acq On : 21 Oct 2022 11:47
 Operator : JC/MD
 Sample : VU1021WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK004

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis

77	10.989	2998	3001	3005	rVB2	406	283	0.01%	0.002%
78	11.082	3026	3030	3032	rBV2	463	340	0.02%	0.002%
79	11.246	3076	3081	3086	rVB2	382	478	0.03%	0.003%
80	11.468	3147	3150	3156	rVB	960	966	0.05%	0.007%
81	11.532	3166	3170	3173	rBV2	490	483	0.03%	0.003%
82	11.745	3229	3236	3244	rVB5	1750	2326	0.12%	0.017%
83	11.809	3244	3256	3273	rBV	636678	1020032	53.65%	7.253%
84	12.012	3317	3319	3328	rVB4	696	964	0.05%	0.007%
85	12.050	3328	3331	3335	rBV2	399	317	0.02%	0.002%
86	12.192	3362	3375	3405	rBV	707902	1157907	60.90%	8.234%
87	12.687	3526	3529	3534	rBV2	493	454	0.02%	0.003%
88	12.770	3551	3555	3557	rBV2	625	479	0.03%	0.003%
89	12.915	3597	3600	3603	rBV3	410	295	0.02%	0.002%
90	12.999	3619	3626	3632	rBV6	811	936	0.05%	0.007%
91	13.227	3689	3697	3705	rBV5	1900	2799	0.15%	0.020%
92	13.362	3735	3739	3742	rVB3	543	408	0.02%	0.003%
93	13.391	3742	3748	3754	rBV4	619	943	0.05%	0.007%
94	13.635	3819	3824	3826	rBV2	457	496	0.03%	0.004%
95	13.841	3881	3888	3897	rBV7	3824	6031	0.32%	0.043%
96	14.092	3960	3966	3978	rVB3	6166	9933	0.52%	0.071%
97	14.333	4034	4041	4054	rVB7	3576	6420	0.34%	0.046%
98	14.417	4065	4067	4070	rVB2	611	376	0.02%	0.003%
99	14.761	4172	4174	4176	rBV2	426	282	0.01%	0.002%
100	15.571	4424	4426	4428	rBV2	692	334	0.02%	0.002%




Sum of corrected areas: 14063147

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102122\
Data File : VU051480.D
Acq On : 21 Oct 2022 11:47
Operator : JC/MD
Sample : VU1021WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK004

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

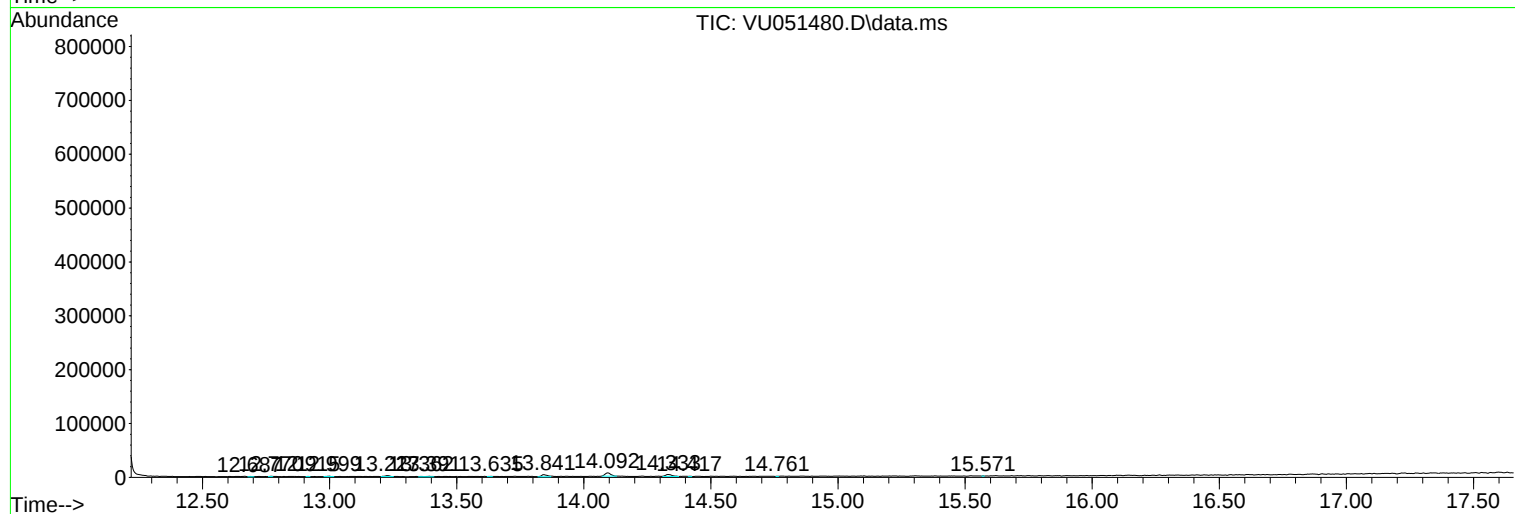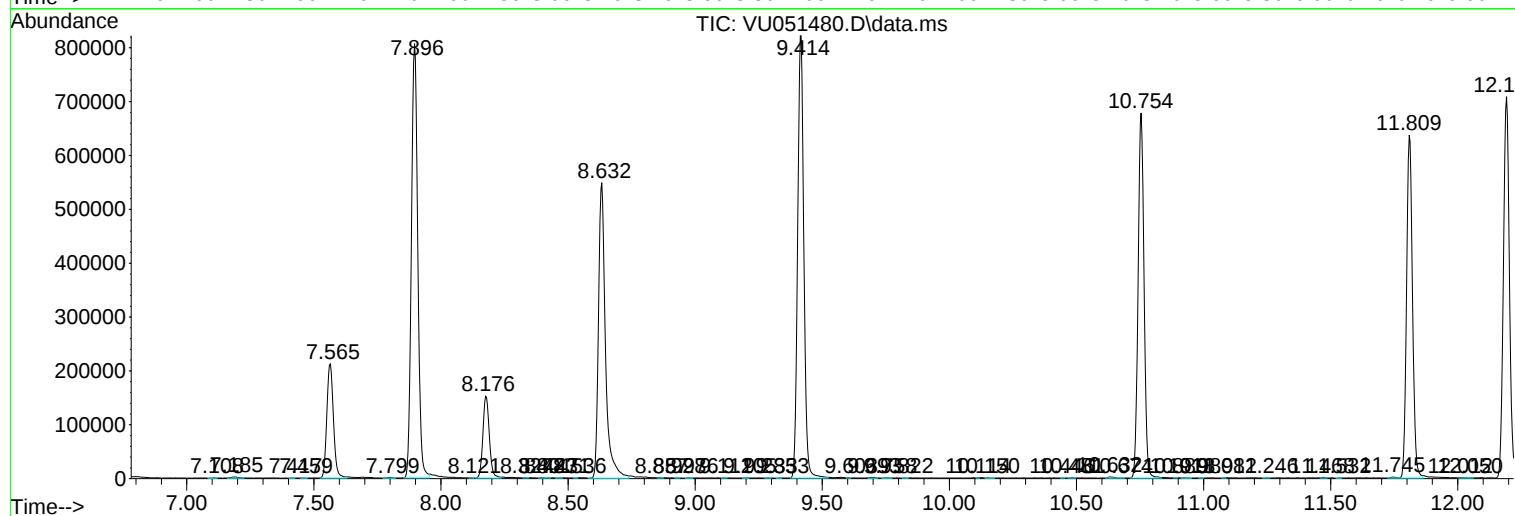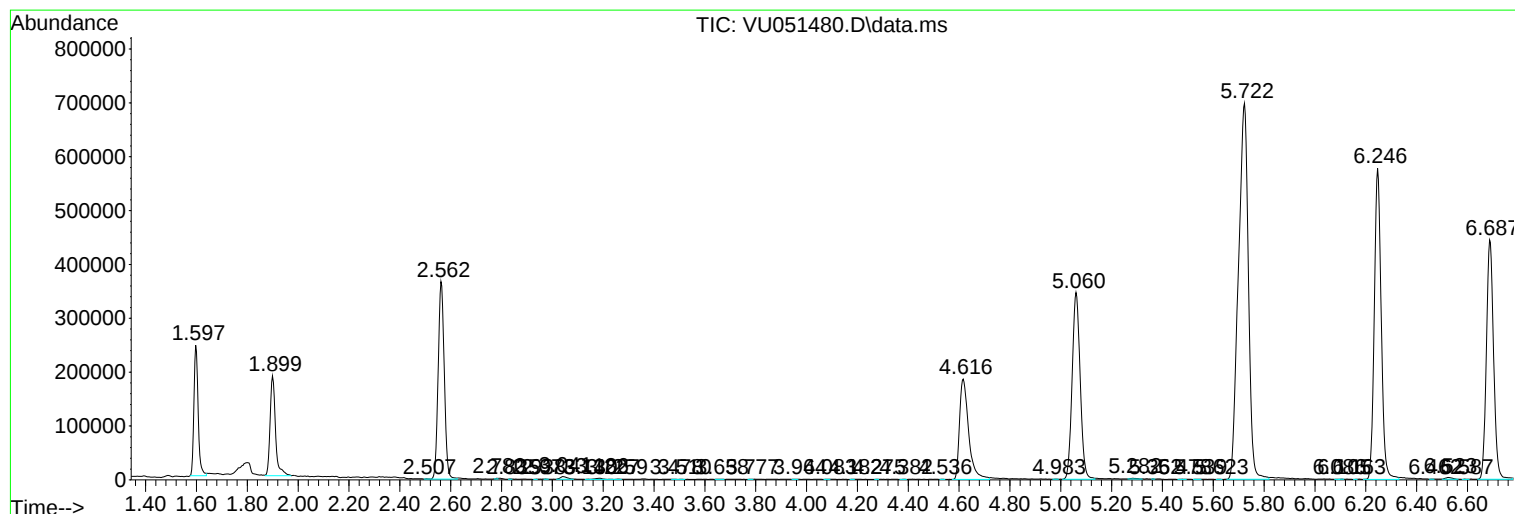

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102122\
Data File : VU051480.D
Acq On : 21 Oct 2022 11:47
Operator : JC/MD
Sample : VU1021WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK004

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102122\
Data File : VU051480.D
Acq On : 21 Oct 2022 11:47
Operator : JC/MD
Sample : VU1021WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK004

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc