
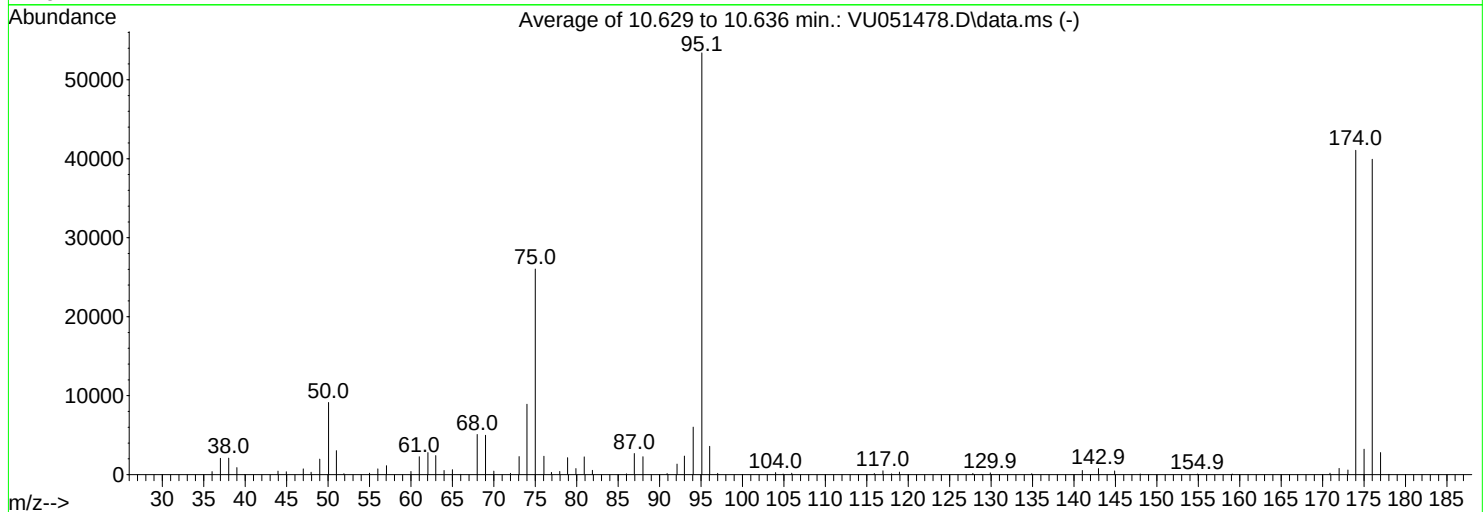


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102122\
 Data File : VU051478.D
 Acq On : 21 Oct 2022 10:08
 Operator : JC/MD
 Sample : BFB139
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB139

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102022WMA.M
 Title : VOC Analysis
 Last Update : Thu Oct 20 21:53:25 2022

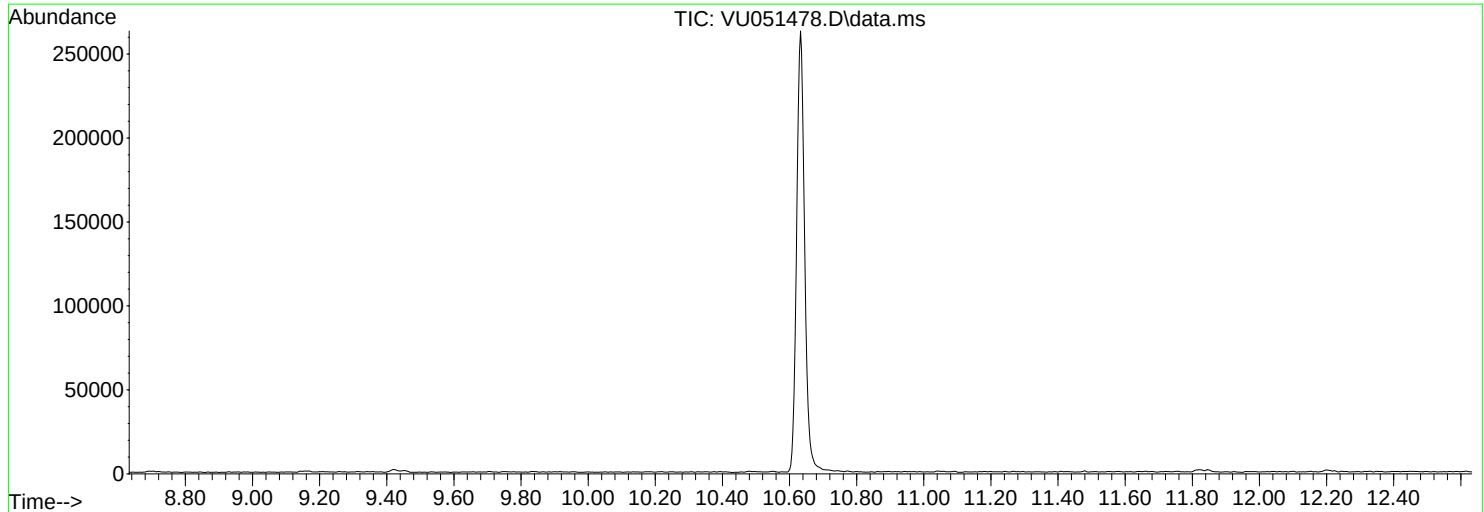

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	9140	PASS
75	95	30	80	48.7	26032	PASS
95	95	100	100	100.0	53408	PASS
96	95	5	9	6.7	3595	PASS
173	174	0.00	2	1.4	587	PASS
174	95	50	120	76.9	41069	PASS
175	174	5	9	7.9	3231	PASS
176	174	95	101	97.2	39939	PASS
177	176	5	9	7.0	2792	PASS

m/z	Abundance
39.90	675.0
43.90	433.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
36.00	415.0
37.00	2026.0
38.00	2127.0
39.00	1002.0
39.90	678.0
44.00	862.0
45.00	349.0
47.00	692.0
48.00	299.0
49.00	1914.0
50.10	9160.0
51.00	2940.0
52.00	113.0
55.00	164.0
56.00	747.0
57.00	1103.0
60.00	360.0
61.00	2331.0
62.10	2721.0
63.00	2440.0
64.00	517.0
65.00	576.0
66.00	102.0
68.00	5222.0
69.00	4910.0
70.00	467.0
72.10	130.0
73.00	2185.0
74.00	8694.0
75.00	26128.0
76.10	2667.0
77.00	306.0
78.00	394.0
78.90	2121.0
79.90	741.0
80.90	2315.0
81.90	587.0
87.00	2509.0
88.00	2292.0
90.90	145.0
92.10	1492.0
93.00	2365.0
94.00	6016.0
95.10	51872.0
96.00	3564.0
97.00	145.0
104.00	234.0
106.00	190.0
115.90	197.0
117.00	449.0
118.00	102.0
119.00	362.0
127.80	192.0
129.90	243.0
134.90	104.0
141.00	482.0
142.90	742.0
144.90	378.0
159.10	114.0
170.90	127.0
172.00	713.0
173.00	581.0
174.00	39960.0
175.00	3292.0
176.00	38184.0
177.00	2786.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
36.00	385.0
37.00	2140.0
38.00	2182.0
39.00	907.0
39.90	703.0
44.00	906.0
44.90	368.0
47.00	772.0
48.00	329.0
49.00	2000.0
50.10	9423.0
51.00	3082.0
51.90	118.0
55.00	202.0
56.00	770.0
57.00	1122.0
60.00	416.0
61.00	2289.0
62.10	2880.0
63.00	2491.0
64.00	560.0
65.00	638.0
68.00	5170.0
69.00	5169.0
70.00	482.0
72.00	166.0
73.10	2339.0
74.00	9164.0
75.00	26968.0
76.00	2391.0
76.90	277.0
78.00	405.0
78.90	2201.0
79.90	807.0
80.90	2304.0
81.90	555.0
86.00	129.0
87.00	2753.0
88.00	2389.0
90.90	165.0
92.10	1338.0
93.00	2424.0
94.00	6270.0
95.10	55248.0
96.10	3763.0
97.00	182.0
104.00	305.0
104.90	131.0
105.90	191.0
115.90	145.0
117.00	514.0
118.00	100.0
118.90	334.0
127.80	166.0
129.90	221.0
134.90	127.0
141.00	558.0
142.90	773.0
144.90	473.0
148.00	101.0
154.90	130.0
159.10	102.0
170.90	187.0
172.00	829.0
173.00	565.0
174.00	42488.0
175.00	3350.0
176.00	41128.0
177.00	2897.0
178.00	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
36.00	336.0
37.00	2042.0
38.00	1964.0
39.00	767.0
39.90	733.0
44.00	850.0
45.00	381.0
47.00	745.0
47.90	279.0
49.00	1970.0
50.00	8836.0
51.00	3088.0
51.80	134.0
55.00	190.0
56.00	652.0
57.10	1185.0
60.00	414.0
61.00	2187.0
62.00	2766.0
63.00	2321.0
64.00	499.0
65.00	685.0
68.00	4879.0
69.00	4893.0
70.00	373.0
71.90	205.0
73.10	2333.0
74.00	8910.0
75.00	25000.0
76.00	1965.0
76.90	278.0
77.90	394.0
78.90	2096.0
79.90	753.0
80.90	2103.0
81.90	523.0
86.00	156.0
86.90	2777.0
88.00	2116.0
90.90	138.0
92.10	1162.0
93.00	2286.0
94.10	5777.0
95.10	53104.0
96.10	3458.0
97.00	186.0
104.00	268.0
104.90	119.0
105.90	182.0
115.80	114.0
116.90	505.0
118.00	104.0
118.90	307.0
127.80	119.0
128.80	130.0
129.90	180.0
134.90	121.0
141.00	516.0
143.00	800.0
144.90	525.0
148.00	116.0
154.90	135.0
170.90	237.0
172.00	827.0
173.10	615.0
174.00	40760.0
175.00	3050.0
176.00	40504.0
177.00	2692.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139