

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102218\
 Data File : VU027741.D
 Acq On : 22 Oct 2018 14:31
 Operator : MD/SY
 Sample : J5589-08DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0T29DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	64	70	79	rBV	65852	64874	14.15%	1.743%
2	1.681	151	158	173	rVB	45190	59557	12.99%	1.601%
3	2.273	333	342	355	rVB	97548	145326	31.70%	3.906%
4	2.402	380	382	383	rBV	191	69	0.02%	0.002%
5	2.447	390	396	407	rVB2	2223	3497	0.76%	0.094%
6	2.800	503	506	508	rBV	93	60	0.01%	0.002%
7	2.839	516	518	526	rBV2	292	262	0.06%	0.007%
8	3.244	642	644	646	rBV	132	55	0.01%	0.001%
9	3.321	666	668	671	rBV	60	36	0.01%	0.001%
10	3.398	689	692	694	rBV	56	30	0.01%	0.001%
11	3.427	698	701	702	rBV	64	36	0.01%	0.001%
12	3.530	729	733	736	rBV	143	97	0.02%	0.003%
13	3.582	742	749	752	rBV	82	91	0.02%	0.002%
14	3.604	752	756	760	rBV	118	108	0.02%	0.003%
15	3.627	760	763	766	rVV	89	47	0.01%	0.001%
16	3.662	771	774	775	rBV	55	30	0.01%	0.001%
17	3.800	814	817	822	rBV	115	126	0.03%	0.003%
18	3.874	836	840	848	rVB	201	237	0.05%	0.006%
19	3.913	848	852	855	rBV	84	78	0.02%	0.002%
20	4.006	877	881	890	rBV	100	163	0.04%	0.004%
21	4.096	906	909	910	rBV	48	28	0.01%	0.001%
22	4.180	921	935	959	rBV	45951	121961	26.60%	3.278%
23	4.402	1001	1004	1008	rBV2	264	226	0.05%	0.006%
24	4.482	1026	1029	1032	rBV	73	55	0.01%	0.001%
25	4.498	1032	1034	1041	rVB	187	113	0.02%	0.003%
26	4.559	1047	1053	1056	rBV	78	84	0.02%	0.002%
27	4.649	1064	1081	1106	rBV	77005	177105	38.63%	4.760%
28	5.016	1193	1195	1197	rBV	146	100	0.02%	0.003%
29	5.083	1214	1216	1219	rVB2	122	73	0.02%	0.002%
30	5.106	1219	1223	1227	rBV2	145	111	0.02%	0.003%
31	5.141	1232	1234	1239	rVB	70	37	0.01%	0.001%
32	5.167	1239	1242	1244	rBV	65	39	0.01%	0.001%
33	5.186	1245	1248	1250	rBV	121	56	0.01%	0.002%
34	5.344	1272	1297	1318	rBV2	154892	458440	100.00%	12.321%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102218\
 Data File : VU027741.D
 Acq On : 22 Oct 2018 14:31
 Operator : MD/SY
 Sample : J5589-08DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0T29DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
 Title : VOC Analysis

35	5.566	1362	1366	1371	rBV	107	120	0.03%	0.003%
36	5.694	1402	1406	1408	rBV	43	34	0.01%	0.001%
37	5.713	1409	1412	1417	rVB	83	68	0.01%	0.002%
38	5.736	1417	1419	1423	rVB	60	37	0.01%	0.001%
39	5.778	1426	1432	1434	rBV	94	79	0.02%	0.002%
40	5.836	1447	1450	1452	rBV	90	63	0.01%	0.002%
41	5.887	1452	1466	1493	rVV	138710	272853	59.52%	7.333%
42	6.045	1512	1515	1520	rVB2	250	208	0.05%	0.006%
43	6.189	1546	1560	1580	rBV	91113	174423	38.05%	4.688%
44	6.334	1591	1605	1624	rBV	106809	213256	46.52%	5.731%
45	6.450	1638	1641	1643	rBV	50	30	0.01%	0.001%
46	6.463	1643	1645	1649	rVB	124	56	0.01%	0.002%
47	6.578	1676	1681	1690	rBV	116	178	0.04%	0.005%
48	6.617	1690	1693	1695	rBV	91	59	0.01%	0.002%
49	6.668	1706	1709	1710	rBV	66	42	0.01%	0.001%
50	6.803	1749	1751	1753	rBV	60	29	0.01%	0.001%
51	6.858	1764	1768	1769	rBV	1007	591	0.13%	0.016%
52	6.910	1781	1784	1788	rVB	82	57	0.01%	0.002%
53	6.974	1801	1804	1810	rBV	105	83	0.02%	0.002%
54	7.000	1810	1812	1815	rBV	45	29	0.01%	0.001%
55	7.038	1821	1824	1827	rBV	57	42	0.01%	0.001%
56	7.077	1833	1836	1839	rBV	59	38	0.01%	0.001%
57	7.122	1847	1850	1853	rBV	73	68	0.01%	0.002%
58	7.228	1872	1883	1911	rVB	65804	116617	25.44%	3.134%
59	7.334	1911	1916	1920	rVB	97	87	0.02%	0.002%
60	7.363	1920	1925	1929	rBV	120	125	0.03%	0.003%
61	7.382	1929	1931	1938	rVB	139	79	0.02%	0.002%
62	7.498	1965	1967	1969	rBV	210	141	0.03%	0.004%
63	7.565	1976	1988	2009	rBV	206256	357667	78.02%	9.612%
64	7.723	2036	2037	2041	rVB	166	94	0.02%	0.003%
65	7.742	2041	2043	2046	rBV	138	63	0.01%	0.002%
66	7.848	2066	2076	2100	rBV	45381	77845	16.98%	2.092%
67	8.051	2138	2139	2143	rVB	130	87	0.02%	0.002%
68	8.070	2143	2145	2147	rBV	145	59	0.01%	0.002%
69	8.093	2151	2152	2155	rVB	130	49	0.01%	0.001%
70	8.122	2158	2161	2162	rBV	56	37	0.01%	0.001%
71	8.183	2168	2180	2186	rBV2	13830	26545	5.79%	0.713%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102218\
Data File : VU027741.D
Acq On : 22 Oct 2018 14:31
Operator : MD/SY
Sample : J5589-08DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0T29DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Title : VOC Analysis

72	8.311	2211	2220	2253	rVB	157297	272467	59.43%	7.323%
73	8.491	2273	2276	2281	rVB2	219	178	0.04%	0.005%
74	8.517	2281	2284	2288	rBV	130	93	0.02%	0.002%
75	8.681	2332	2335	2340	rBV	72	76	0.02%	0.002%
76	8.720	2344	2347	2351	rVB	115	84	0.02%	0.002%
77	8.823	2375	2379	2380	rBV	83	58	0.01%	0.002%
78	8.852	2384	2388	2399	rVB	163	256	0.06%	0.007%
79	8.903	2399	2404	2408	rBV	137	118	0.03%	0.003%
80	8.929	2408	2412	2413	rBV	62	50	0.01%	0.001%
81	9.090	2450	2462	2481	rBV	199178	331798	72.38%	8.917%
82	9.299	2526	2527	2528	rBV	122	32	0.01%	0.001%
83	9.389	2553	2555	2557	rVB	157	61	0.01%	0.002%
84	9.617	2623	2626	2631	rBV	125	138	0.03%	0.004%
85	9.678	2642	2645	2646	rBV	80	51	0.01%	0.001%
86	9.845	2694	2697	2699	rBV	73	55	0.01%	0.001%
87	9.903	2711	2715	2720	rBV	135	147	0.03%	0.004%
88	10.012	2746	2749	2751	rBV	121	76	0.02%	0.002%
89	10.086	2769	2772	2774	rBV	129	91	0.02%	0.002%
90	10.434	2868	2880	2899	rVB	132613	211982	46.24%	5.697%
91	10.559	2912	2919	2924	rBV	132	200	0.04%	0.005%
92	10.614	2925	2936	2952	rVV2	7874	16133	3.52%	0.434%
93	10.877	3011	3018	3027	rVB2	677	959	0.21%	0.026%
94	11.485	3195	3207	3223	rBV	187739	294335	64.20%	7.910%
95	11.861	3312	3324	3339	rBV	187779	297825	64.96%	8.004%
96	12.208	3430	3432	3437	rVB	183	107	0.02%	0.003%
97	12.234	3437	3440	3442	rBV	147	94	0.02%	0.003%
98	12.478	3506	3516	3527	rBV2	3653	6118	1.33%	0.164%
99	14.067	4008	4010	4012	rBV	250	57	0.01%	0.002%
100	14.279	4066	4076	4087	rVB	7364	12136	2.65%	0.326%


Sum of corrected areas: 3720920

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102218\
Data File : VU027741.D
Acq On : 22 Oct 2018 14:31
Operator : MD/SY
Sample : J5589-08DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0T29DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

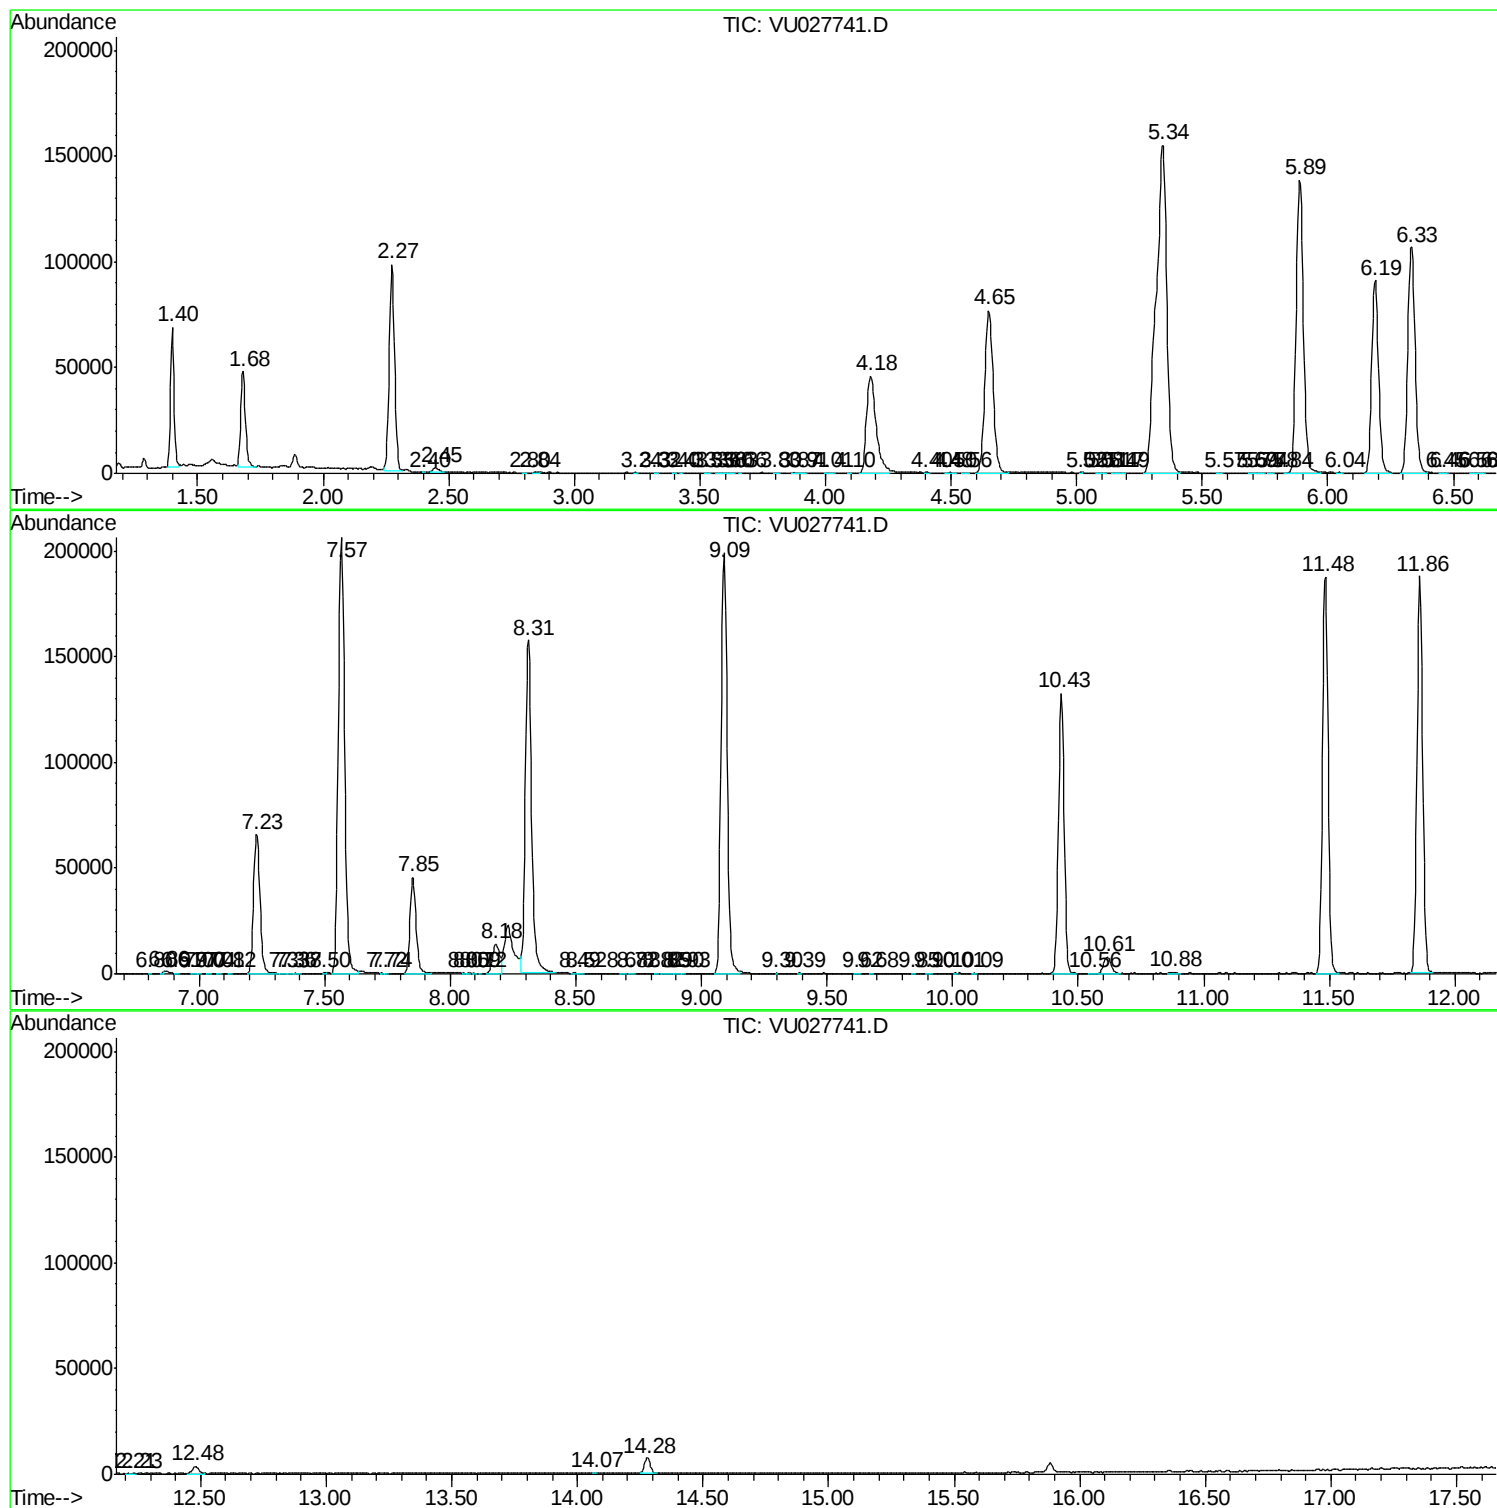

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU102218\
Data File : VU027741.D
Acq On : 22 Oct 2018 14:31
Operator : MD/SY
Sample : J5589-08DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0T29DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU102218\
Data File : VU027741.D
Acq On : 22 Oct 2018 14:31
Operator : MD/SY
Sample : J5589-08DL 5X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0T29DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM102218WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc