


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102218\
Data File : VU027727.D
Acq On : 22 Oct 2018 08:09
Operator : MD/SY
Sample : BFB46
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB46

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM102218WMA.M
Title : VOC Analysis
Last Update : Tue Oct 23 08:01:28 2018

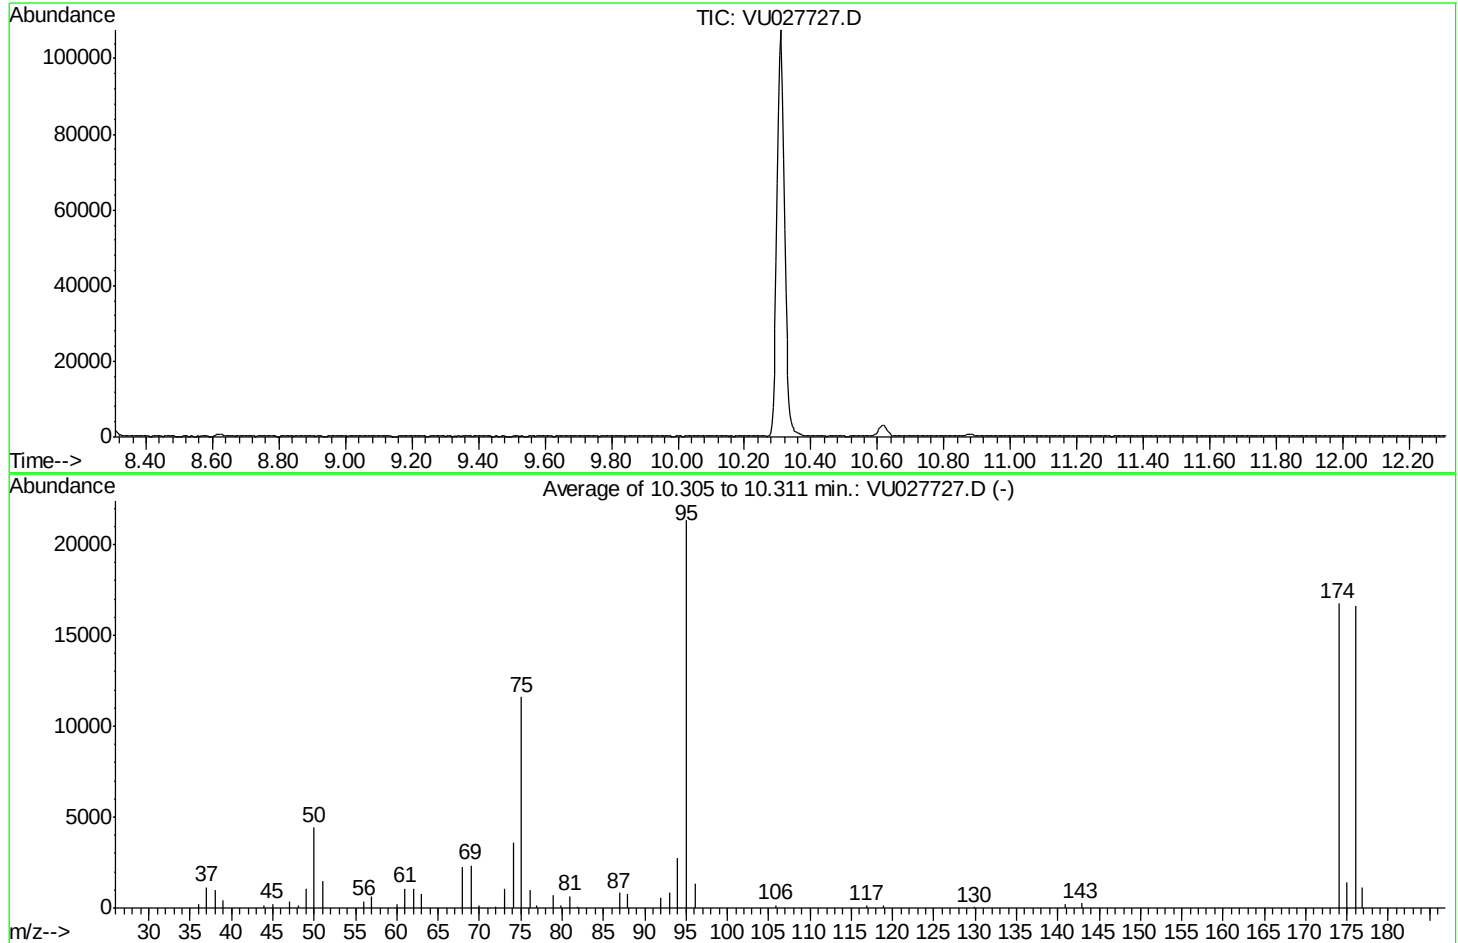

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	4423	PASS
75	95	30	80	54.4	11603	PASS
95	95	100	100	100.0	21333	PASS
96	95	5	9	6.3	1349	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.5	16740	PASS
175	174	5	9	8.5	1421	PASS
176	174	95	101	99.3	16626	PASS
177	176	5	9	6.7	1116	PASS

m/z	Abundance
43.90	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	215.0
37.00	1168.0
38.00	1027.0
39.00	477.0
44.00	368.0
45.00	232.0
47.00	361.0
48.10	143.0
49.00	1126.0
50.00	4536.0
51.10	1528.0
56.10	406.0
57.00	606.0
60.10	205.0
61.00	1130.0
62.00	1064.0
63.00	831.0
68.00	2383.0
69.00	2388.0
70.00	141.0
71.90	102.0
73.00	1073.0
74.10	3687.0
75.10	12025.0
76.10	1038.0
76.90	160.0
79.00	708.0
79.90	180.0
80.90	684.0
81.80	123.0
87.00	865.0
87.90	744.0
92.00	581.0
93.10	881.0
94.00	2874.0
95.10	22008.0
96.10	1395.0
105.90	150.0
116.90	146.0
118.90	132.0
129.90	103.0
140.80	246.0
142.90	283.0
174.00	17320.0
175.00	1481.0
176.00	17088.0
176.90	1154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
35.90	216.0
37.00	1164.0
38.00	983.0
39.00	432.0
43.90	345.0
45.00	219.0
47.00	377.0
48.10	140.0
49.00	1103.0
50.00	4175.0
51.10	1414.0
56.10	394.0
57.00	600.0
60.10	174.0
61.00	1016.0
62.00	940.0
63.00	843.0
68.00	2119.0
69.00	2378.0
70.00	143.0
71.90	100.0
73.00	1059.0
74.00	3543.0
75.10	11494.0
76.10	957.0
76.90	119.0
79.00	662.0
79.90	197.0
80.90	674.0
81.80	137.0
86.90	740.0
87.90	765.0
92.00	535.0
93.00	855.0
94.00	2691.0
95.10	21144.0
96.10	1411.0
105.90	146.0
117.00	151.0
118.90	117.0
129.90	109.0
140.80	242.0
142.80	281.0
174.00	17088.0
175.00	1449.0
176.00	17048.0
176.90	1153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	214.0
37.00	1103.0
38.00	950.0
39.00	437.0
44.00	357.0
45.00	216.0
47.00	327.0
48.10	128.0
49.00	963.0
50.00	4558.0
51.10	1466.0
56.00	347.0
57.00	597.0
60.10	210.0
61.00	1129.0
62.00	1081.0
63.00	758.0
68.00	2328.0
69.00	2250.0
70.00	150.0
73.00	986.0
74.10	3465.0
75.10	11290.0
76.10	1070.0
77.00	145.0
79.00	679.0
79.90	151.0
81.00	642.0
87.00	890.0
88.00	717.0
92.00	618.0
93.10	808.0
94.00	2762.0
95.10	20848.0
96.10	1243.0
105.90	134.0
116.90	119.0
118.90	130.0
140.90	245.0
142.90	264.0
174.00	15814.0
175.00	1334.0
176.00	15744.0
176.90	1042.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46