


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102219\
Data File : VU035326.D
Acq On : 21 Oct 2019 15:36
Operator : JC/SP
Sample : BFB23
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB23

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Oct 24 14:19:48 2019

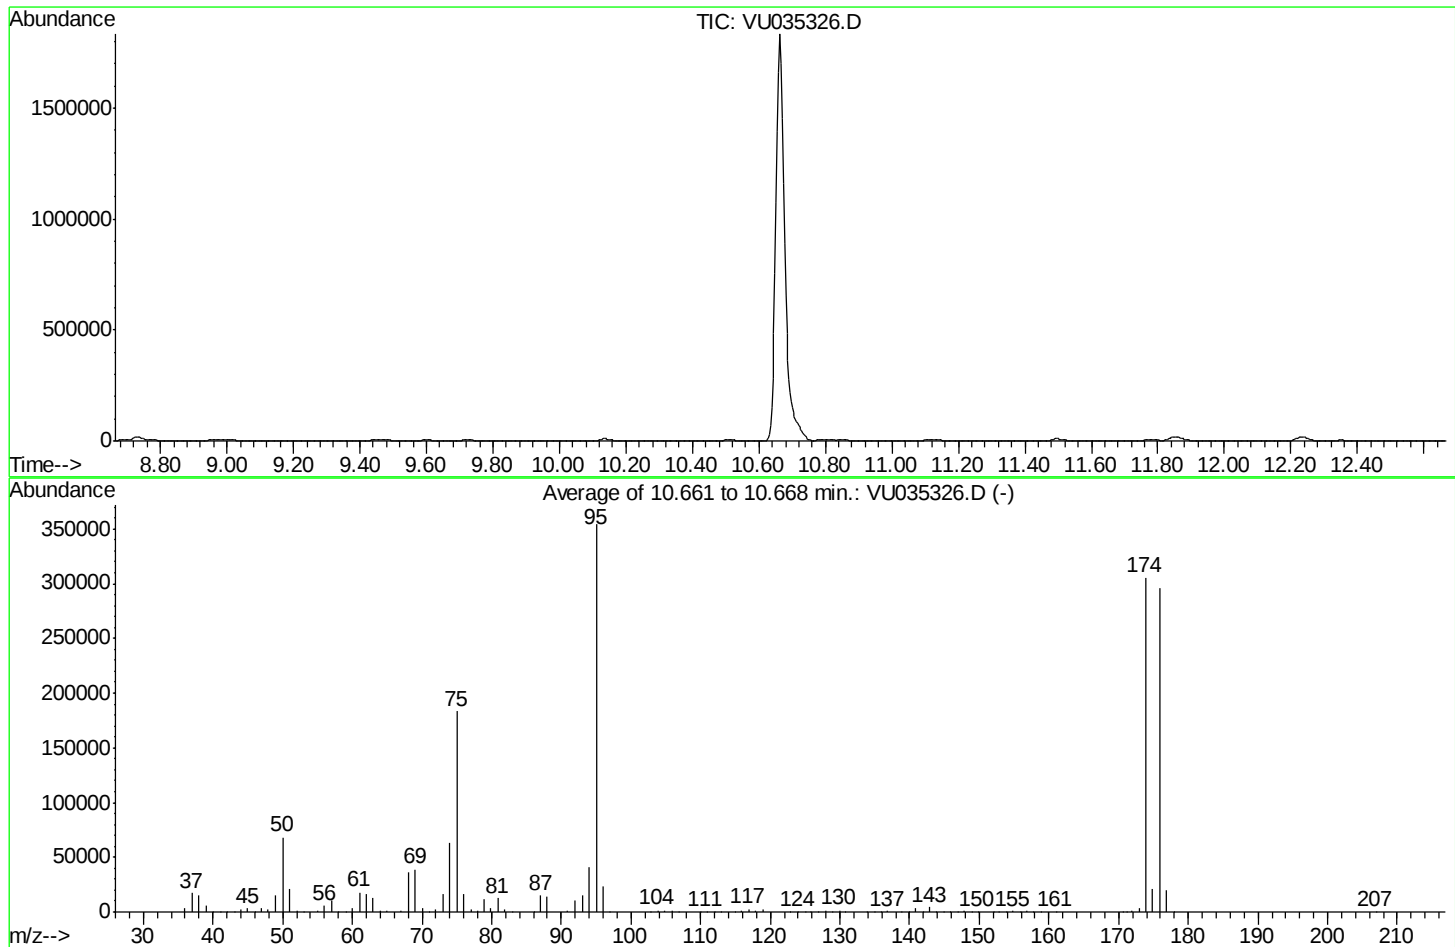

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	68410	PASS
75	95	30	80	51.7	183168	PASS
95	95	100	100	100.0	354218	PASS
96	95	5	9	6.7	23634	PASS
173	174	0.00	2	1.0	3019	PASS
174	95	50	120	86.3	305813	PASS
175	174	5	9	7.0	21506	PASS
176	174	95	101	96.7	295637	PASS
177	176	5	9	6.6	19624	PASS

m/z	Abundance
36.00	3251.0
37.00	18280.0
38.00	16584.0
39.00	6709.0
40.00	381.0
41.00	110.0
41.90	107.0
43.10	188.0
44.00	3190.0
45.00	3155.0
45.90	295.0
47.00	4115.0
47.90	2251.0
49.00	15786.0
50.00	70664.0
51.00	22040.0
52.00	959.0
53.00	108.0
55.00	1037.0
56.00	5795.0
57.00	10596.0
58.00	404.0
59.00	125.0
60.00	3319.0
61.00	18352.0
62.00	17352.0
63.00	14125.0
64.00	1533.0
65.00	667.0
66.90	1032.0
68.00	37128.0
69.00	39656.0
70.00	3149.0
71.00	125.0
72.00	2085.0
73.00	17072.0
74.00	64888.0
75.00	187840.0
76.00	16648.0
77.00	2543.0
78.00	1500.0
78.90	12160.0
79.90	3614.0
80.90	12750.0
81.90	2860.0
83.00	278.0
86.10	334.0
87.00	15084.0
87.90	14526.0
90.90	1463.0
92.00	10450.0
93.00	15469.0
94.00	42800.0
95.00	363456.0
96.00	24528.0
96.90	716.0
102.80	197.0
103.90	1760.0
104.90	697.0
105.90	1625.0
106.80	417.0
109.90	266.0
110.90	342.0
111.90	203.0
112.80	273.0
115.00	390.0
115.90	1490.0
116.90	2434.0
117.80	1263.0
118.90	1855.0
122.90	113.0
123.90	199.0
125.00	113.0
125.80	250.0
126.80	102.0
127.90	1325.0
128.80	582.0
129.90	1459.0
130.80	626.0
133.90	127.0
134.90	691.0
136.80	640.0
138.70	129.0
139.90	182.0
140.90	3729.0
141.90	488.0
142.90	4370.0
143.80	238.0
144.90	282.0
145.80	542.0
146.70	213.0
147.80	839.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

149.00	150.0
149.80	474.0
152.00	154.0
152.80	256.0
153.90	236.0
154.90	786.0
155.90	170.0
156.90	630.0
157.80	227.0
158.90	383.0
160.90	318.0
170.60	182.0
171.10	190.0
172.00	1010.0
173.00	3079.0
173.90	307520.0
174.90	21848.0
175.90	295168.0
176.90	20080.0
177.90	506.0
206.90	213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	3180.0
37.00	17944.0
38.00	16152.0
39.00	6412.0
40.00	317.0
43.10	218.0
44.00	3254.0
45.00	3083.0
46.00	363.0
47.00	4115.0
47.90	2223.0
49.00	15560.0
50.00	70240.0
51.00	21624.0
52.00	960.0
55.00	1053.0
56.00	5882.0
57.00	10352.0
58.00	410.0
59.00	160.0
60.00	3159.0
61.00	18536.0
62.00	17448.0
63.00	13877.0
64.00	1450.0
65.00	634.0
66.90	994.0
68.00	37288.0
69.00	40032.0
70.00	3078.0
71.00	143.0
72.00	2031.0
73.00	17040.0
74.00	64408.0
75.00	188032.0
76.00	16322.0
77.00	2528.0
78.00	1685.0
78.90	12319.0
79.90	3585.0
80.90	12629.0
81.90	2837.0
82.90	290.0
86.00	301.0
87.00	15220.0
87.90	14649.0
90.90	1454.0
92.00	10400.0
93.00	15545.0
94.00	42712.0
95.00	364096.0
96.00	24256.0
96.90	595.0
102.80	218.0
103.80	1784.0
104.90	736.0
105.90	1749.0
106.80	367.0
109.90	252.0
110.90	377.0
111.90	206.0
112.90	237.0
115.00	388.0
115.90	1442.0
116.90	2558.0
117.90	1473.0
118.90	1924.0
124.00	218.0
125.80	235.0
127.90	1312.0
128.80	552.0
129.90	1507.0
130.80	577.0
134.90	639.0
135.90	116.0
136.80	657.0
138.70	146.0
139.90	256.0
140.90	3691.0
142.00	449.0
142.90	4448.0
143.80	283.0
144.90	310.0
145.90	462.0
146.80	222.0
147.80	918.0
148.80	142.0
149.80	514.0
152.00	121.0
152.80	258.0
153.80	211.0
154.90	803.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

155.90	180.0
156.80	690.0
157.80	219.0
158.90	359.0
160.90	265.0
170.60	161.0
171.90	1019.0
173.00	3086.0
173.90	314624.0
174.90	22008.0
175.90	303872.0
176.90	20224.0
177.90	427.0
206.90	191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

m/z	Abundance
36.00	2872.0
37.00	16025.0
38.00	14431.0
39.00	5695.0
40.00	286.0
43.10	282.0
44.00	3122.0
45.00	2763.0
46.00	367.0
47.00	3727.0
48.00	1999.0
49.00	13974.0
50.00	64328.0
51.00	20016.0
52.00	916.0
55.00	1062.0
56.00	5456.0
57.00	9216.0
58.00	371.0
59.00	164.0
60.00	2890.0
61.00	16944.0
62.00	15842.0
63.00	12426.0
64.00	1235.0
65.00	594.0
66.90	917.0
68.00	34456.0
69.00	36552.0
70.00	2795.0
71.00	124.0
71.90	1819.0
73.00	15824.0
74.00	58656.0
75.00	173632.0
76.00	14741.0
77.00	2283.0
78.00	1563.0
78.90	11363.0
79.90	3116.0
80.90	11624.0
81.90	2691.0
83.00	273.0
85.90	321.0
87.00	14232.0
87.90	13682.0
90.90	1257.0
92.00	9658.0
93.00	14498.0
94.00	39120.0
95.00	335104.0
96.00	22120.0
97.00	454.0
102.90	224.0
103.90	1690.0
104.90	662.0
105.90	1630.0
106.70	311.0
109.90	213.0
110.80	333.0
111.90	208.0
112.90	220.0
114.90	336.0
115.90	1244.0
116.90	2306.0
117.90	1541.0
118.90	1795.0
124.10	242.0
125.80	199.0
127.90	1181.0
128.90	532.0
129.90	1319.0
130.70	543.0
134.90	533.0
135.90	123.0
136.90	583.0
138.80	159.0
139.90	305.0
140.90	3456.0
141.90	351.0
142.90	4111.0
143.80	291.0
144.90	369.0
145.90	392.0
146.90	221.0
147.80	873.0
148.80	169.0
149.80	473.0
152.80	214.0
153.70	224.0
154.80	810.0
155.90	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

156.80	663.0
157.80	221.0
158.90	304.0
161.00	263.0
170.60	122.0
171.90	959.0
173.00	2893.0
173.90	295296.0
174.90	20664.0
175.90	287872.0
176.90	18568.0
177.90	358.0
206.90	133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23

Scan 2884 (10.613 min): VU035326.D
BFB23

m/z	Abundance
39.90	289.0
44.00	1064.0

Instrument :
MSVOA_U
ClientSampleId :
BFB23