


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102219\
 Data File : VU035349.D
 Acq On : 22 Oct 2019 08:24
 Operator : JC/SP
 Sample : BFB24
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB24

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Oct 24 14:19:48 2019

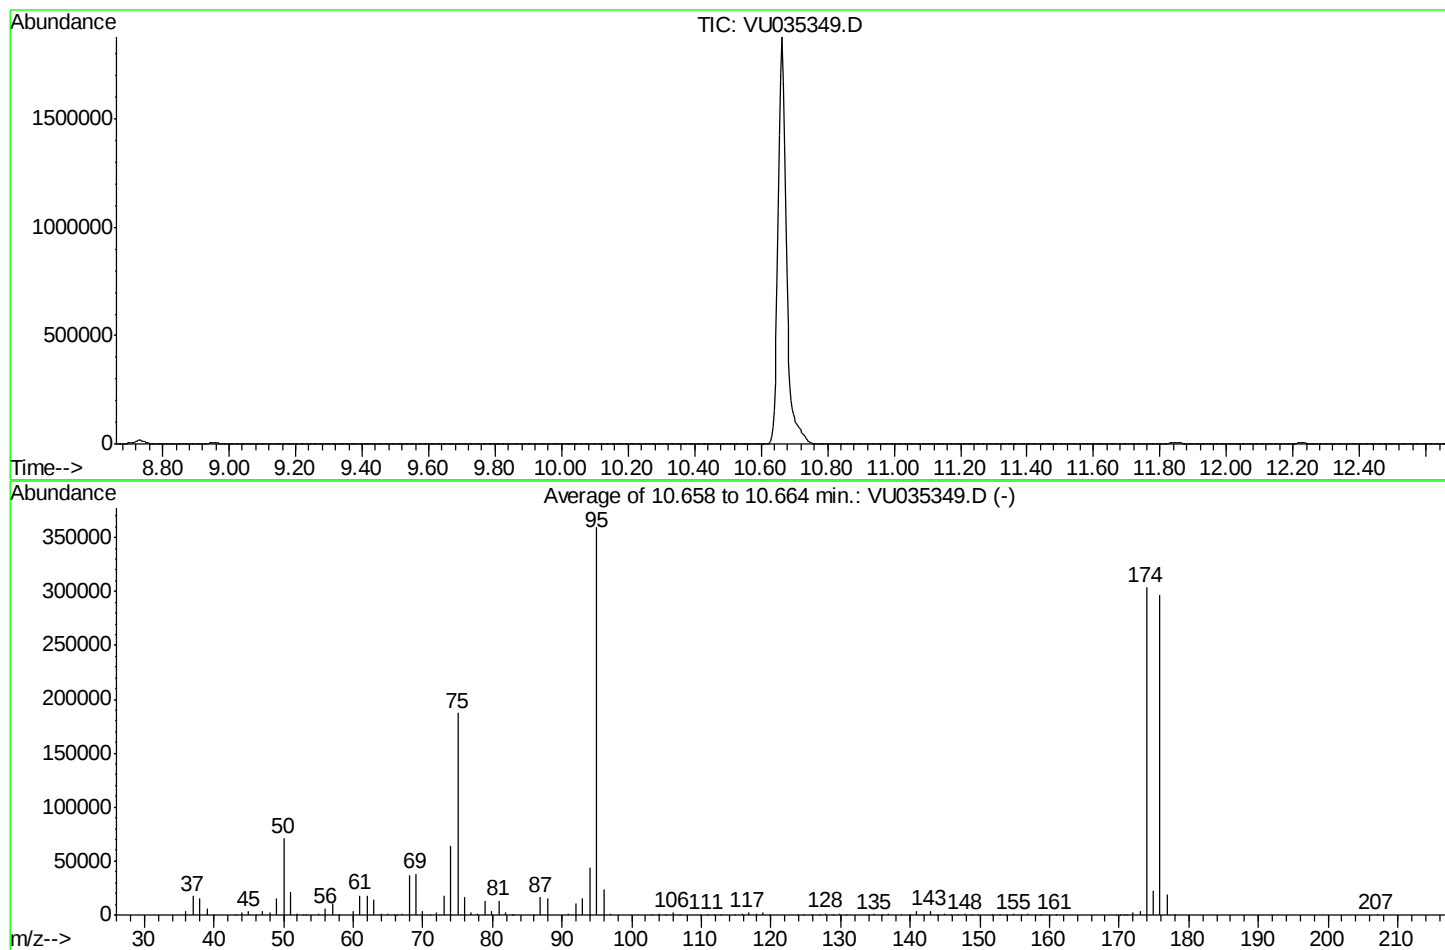

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	70845	PASS
75	95	30	80	52.1	187349	PASS
95	95	100	100	100.0	359466	PASS
96	95	5	9	6.7	23933	PASS
173	174	0.00	2	1.2	3575	PASS
174	95	50	120	84.5	303786	PASS
175	174	5	9	7.4	22597	PASS
176	174	95	101	97.6	296554	PASS
177	176	5	9	6.4	19090	PASS

m/z	Abundance
36.00	3208.0
37.00	17136.0
38.00	15254.0
39.00	6236.0
40.00	439.0
43.00	174.0
44.00	3038.0
45.00	3365.0
46.00	411.0
47.00	3851.0
48.00	2494.0
49.00	15198.0
50.00	67440.0
51.00	21000.0
51.90	767.0
53.10	139.0
55.00	1067.0
56.00	5360.0
57.00	9955.0
58.10	378.0
60.00	3431.0
61.00	17472.0
62.00	17040.0
63.00	14368.0
64.00	1507.0
65.10	1716.0
66.20	189.0
67.00	977.0
68.00	35640.0
69.00	37504.0
70.00	3272.0
71.00	148.0
72.00	2105.0
73.00	16792.0
74.00	61328.0
75.00	178304.0
76.00	15639.0
77.00	2382.0
77.80	1241.0
78.90	12321.0
79.90	3482.0
80.90	12768.0
81.90	2809.0
82.80	355.0
85.90	571.0
86.90	15233.0
87.90	14274.0
90.90	1534.0
92.00	10077.0
93.00	14929.0
94.00	41560.0
95.00	340480.0
96.00	23264.0
97.00	667.0
102.90	143.0
103.80	1777.0
104.90	525.0
105.90	1864.0
106.90	406.0
109.80	236.0
110.90	415.0
111.80	261.0
112.80	324.0
114.80	464.0
115.90	1230.0
116.80	2039.0
117.90	1237.0
118.90	1742.0
123.80	254.0
124.60	108.0
125.80	117.0
127.80	1244.0
128.90	602.0
129.80	1035.0
130.80	567.0
134.80	629.0
135.80	132.0
136.80	592.0
138.70	182.0
139.90	249.0
140.90	3383.0
141.90	466.0
142.90	3965.0
143.90	204.0
144.90	749.0
145.90	500.0
146.80	293.0
147.90	742.0
148.80	229.0
149.80	324.0
151.80	142.0
152.80	219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

153.70	150.0
154.90	915.0
156.00	256.0
156.90	653.0
157.90	168.0
158.80	526.0
160.90	345.0
169.50	135.0
170.10	134.0
170.70	222.0
171.10	214.0
171.90	2234.0
173.00	3445.0
173.90	280640.0
174.90	21096.0
175.90	273344.0
176.90	17568.0
177.90	436.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	3498.0
37.00	18360.0
38.00	16424.0
39.00	6740.0
40.00	460.0
43.00	177.0
44.00	3285.0
45.00	3559.0
46.10	401.0
47.00	4190.0
48.00	2554.0
49.00	16152.0
50.00	73144.0
51.00	22480.0
52.00	878.0
53.20	127.0
55.00	1105.0
56.00	5640.0
57.00	10965.0
58.00	427.0
60.00	3640.0
61.00	19096.0
62.00	18608.0
63.00	15162.0
64.00	1459.0
65.00	1563.0
65.80	117.0
66.20	162.0
67.00	1070.0
68.00	38400.0
69.00	39816.0
70.00	3368.0
71.00	176.0
72.00	2226.0
73.00	17968.0
74.00	66592.0
75.00	193344.0
76.00	16656.0
76.90	2498.0
77.80	1638.0
78.90	13140.0
79.90	3857.0
80.90	13695.0
81.90	3015.0
82.80	359.0
85.90	616.0
86.90	16864.0
87.90	15488.0
90.90	1564.0
92.00	11226.0
93.00	16144.0
94.00	45128.0
95.00	371840.0
96.00	24744.0
97.00	807.0
102.90	195.0
103.80	1852.0
104.90	577.0
105.90	1956.0
106.90	417.0
109.80	261.0
110.90	408.0
111.90	274.0
112.80	340.0
114.90	506.0
115.90	1382.0
116.80	2247.0
117.90	1328.0
118.90	2028.0
119.80	109.0
123.70	246.0
124.70	110.0
125.80	126.0
127.00	100.0
127.90	1374.0
128.90	649.0
129.80	1153.0
130.90	599.0
134.90	752.0
135.90	138.0
136.80	717.0
138.70	245.0
139.90	260.0
140.90	3768.0
141.80	510.0
142.90	4198.0
143.90	223.0
144.90	797.0
145.90	461.0
146.80	292.0
147.90	902.0
148.80	176.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

149.80	326.0
151.80	186.0
152.90	255.0
153.70	193.0
154.90	921.0
156.00	286.0
156.90	766.0
157.90	191.0
158.80	596.0
160.80	372.0
169.50	151.0
170.10	125.0
170.70	267.0
171.10	225.0
171.90	2288.0
173.00	3736.0
173.90	313600.0
174.90	23352.0
175.90	306624.0
176.90	19744.0
177.90	407.0
207.00	137.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
36.00	3400.0
37.00	17528.0
38.00	16028.0
39.00	6538.0
39.90	479.0
43.00	192.0
44.00	3240.0
45.00	3333.0
46.10	351.0
47.00	4237.0
48.00	2433.0
49.00	15603.0
50.00	71952.0
51.00	22064.0
52.00	899.0
52.80	103.0
53.20	112.0
54.90	1001.0
56.00	5708.0
57.00	10712.0
57.90	450.0
60.00	3460.0
61.00	18368.0
62.00	18440.0
63.00	14586.0
64.00	1361.0
65.00	1305.0
65.80	137.0
67.00	1034.0
68.00	37584.0
69.00	38456.0
70.00	3285.0
71.00	172.0
71.90	2029.0
73.00	17736.0
74.00	65264.0
75.00	190400.0
76.00	16220.0
77.00	2321.0
77.90	1711.0
78.90	12635.0
79.90	3965.0
80.90	13449.0
81.90	2878.0
83.00	319.0
85.90	595.0
86.90	16373.0
87.90	15053.0
90.90	1454.0
92.00	11125.0
93.00	15699.0
94.00	44528.0
95.00	366080.0
96.00	23792.0
97.00	774.0
102.80	252.0
103.90	1687.0
104.90	573.0
105.90	1933.0
106.90	370.0
109.90	314.0
110.90	337.0
111.90	294.0
112.80	306.0
114.90	468.0
115.90	1354.0
116.80	2310.0
117.80	1370.0
118.90	2095.0
119.80	102.0
123.70	220.0
125.80	129.0
127.00	133.0
127.90	1305.0
128.90	568.0
129.90	1144.0
130.90	529.0
133.90	114.0
134.90	770.0
135.90	123.0
136.80	703.0
138.70	224.0
139.90	249.0
140.90	3835.0
141.80	516.0
142.90	4006.0
143.90	228.0
144.90	762.0
145.90	455.0
146.80	269.0
147.90	974.0
148.80	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

149.80	322.0
151.70	222.0
152.90	294.0
153.80	190.0
154.90	873.0
155.90	284.0
156.90	886.0
157.90	207.0
158.80	559.0
160.80	399.0
169.60	100.0
170.70	328.0
171.90	2141.0
173.00	3545.0
173.90	317120.0
174.90	23344.0
175.90	309696.0
176.90	19960.0
178.00	386.0
207.00	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

Scan 2884 (10.613 min): VU035349.D
BFB24

m/z	Abundance
39.90	172.0
44.00	961.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24