



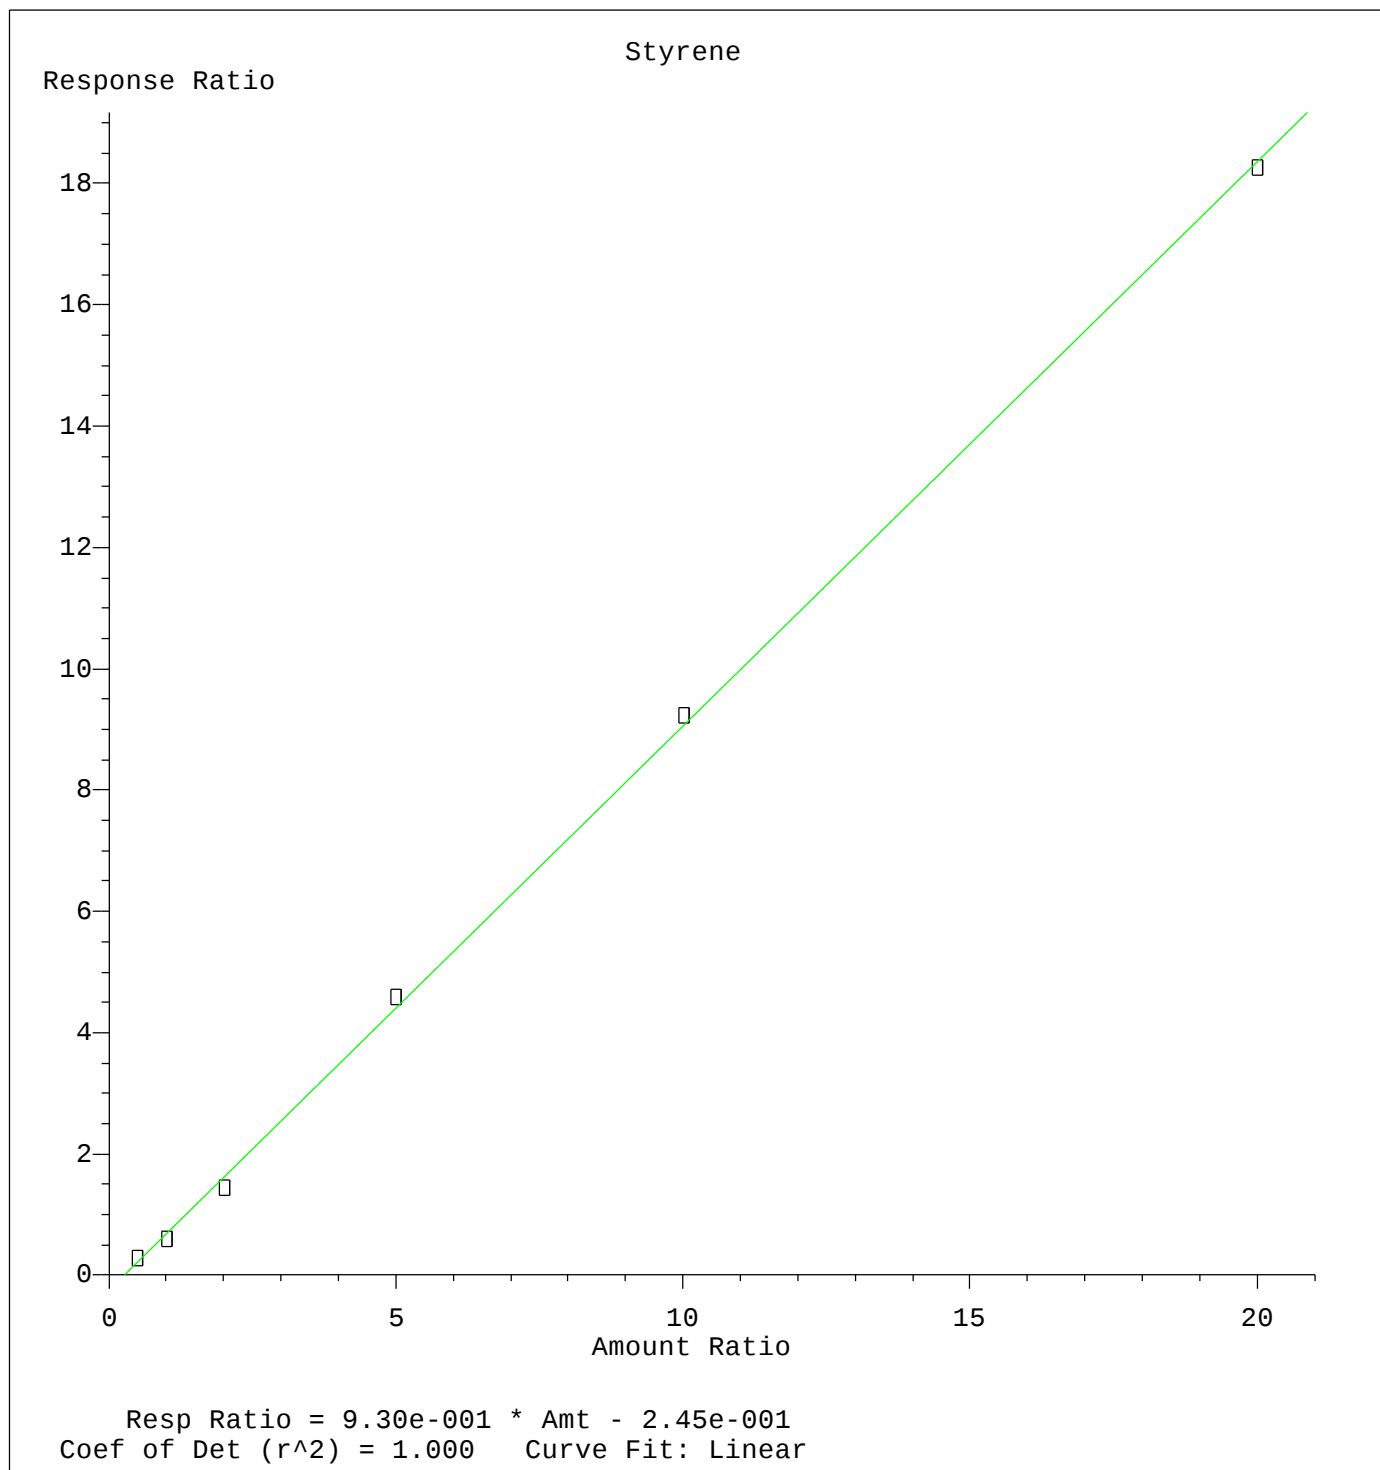


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
Calibration Table Last Updated: Fri Oct 23 07:07:33 2020

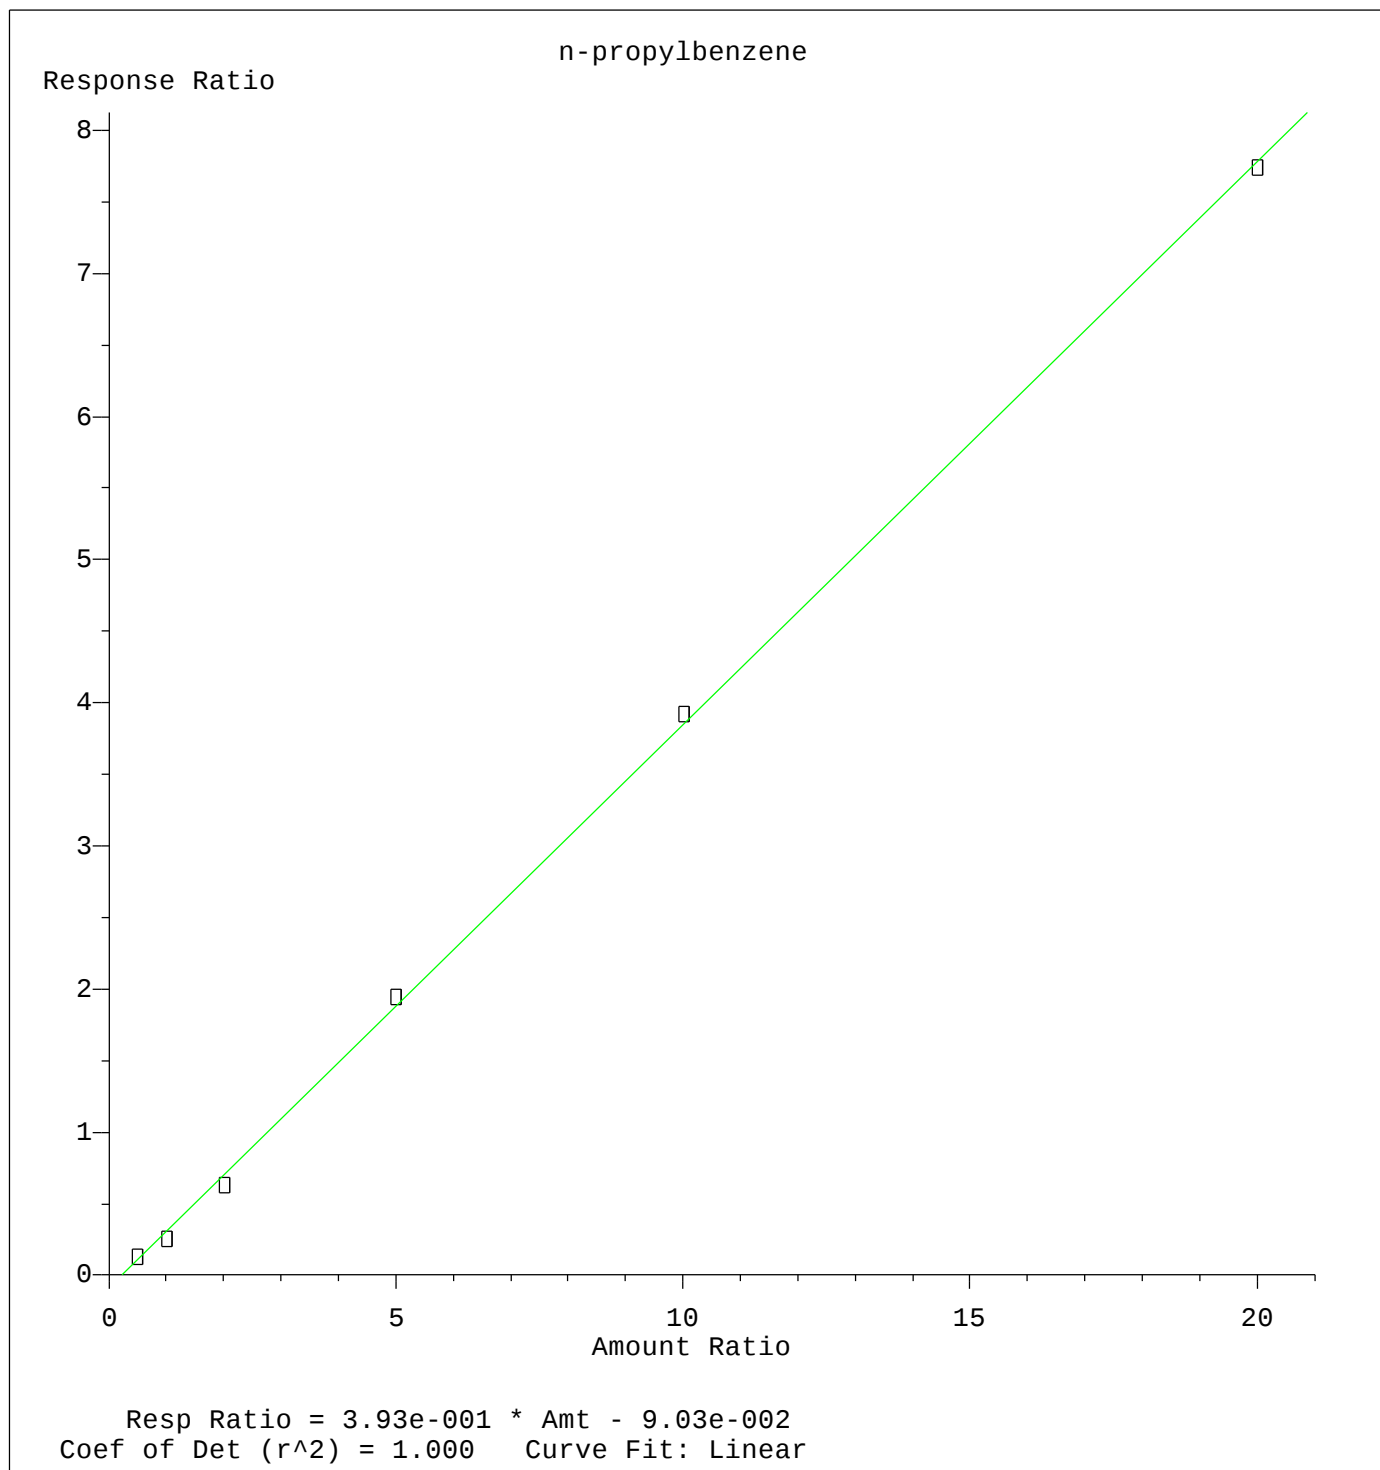

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
Calibration Table Last Updated: Fri Oct 23 07:07:33 2020

1,3,5-Trimethylbenzene

Response Ratio

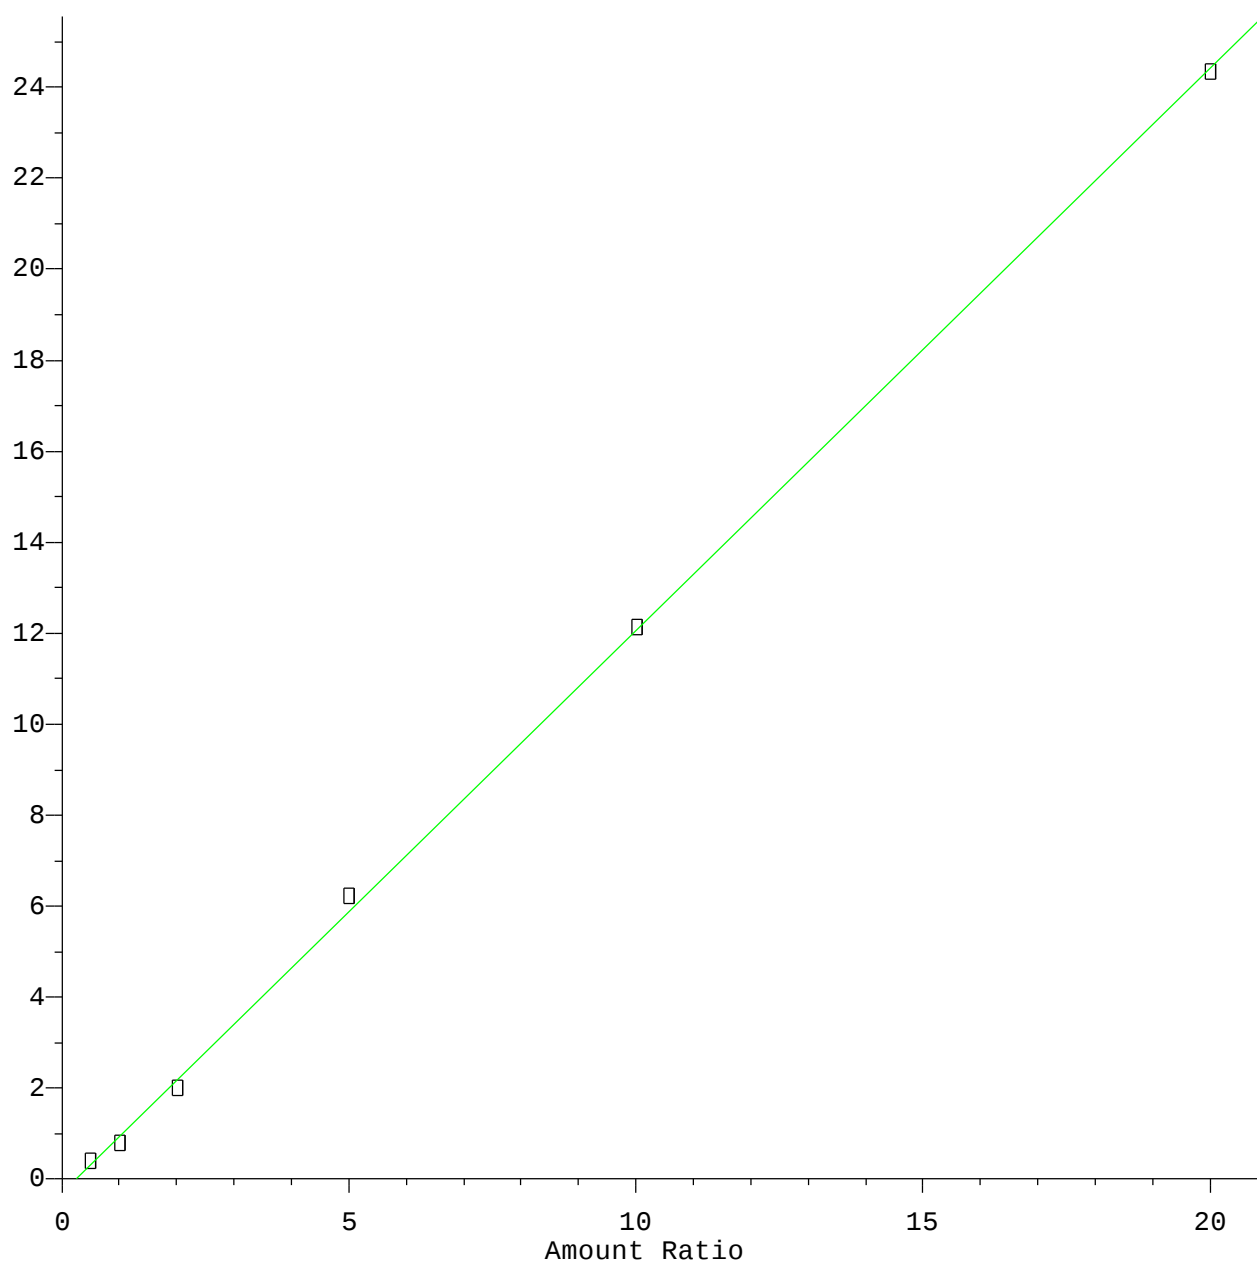


Resp Ratio = 1.24×10^0 * Amt - 2.92×10^{-1}
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
Calibration Table Last Updated: Fri Oct 23 07:07:33 2020

1,2,4-Trimethylbenzene

Response Ratio

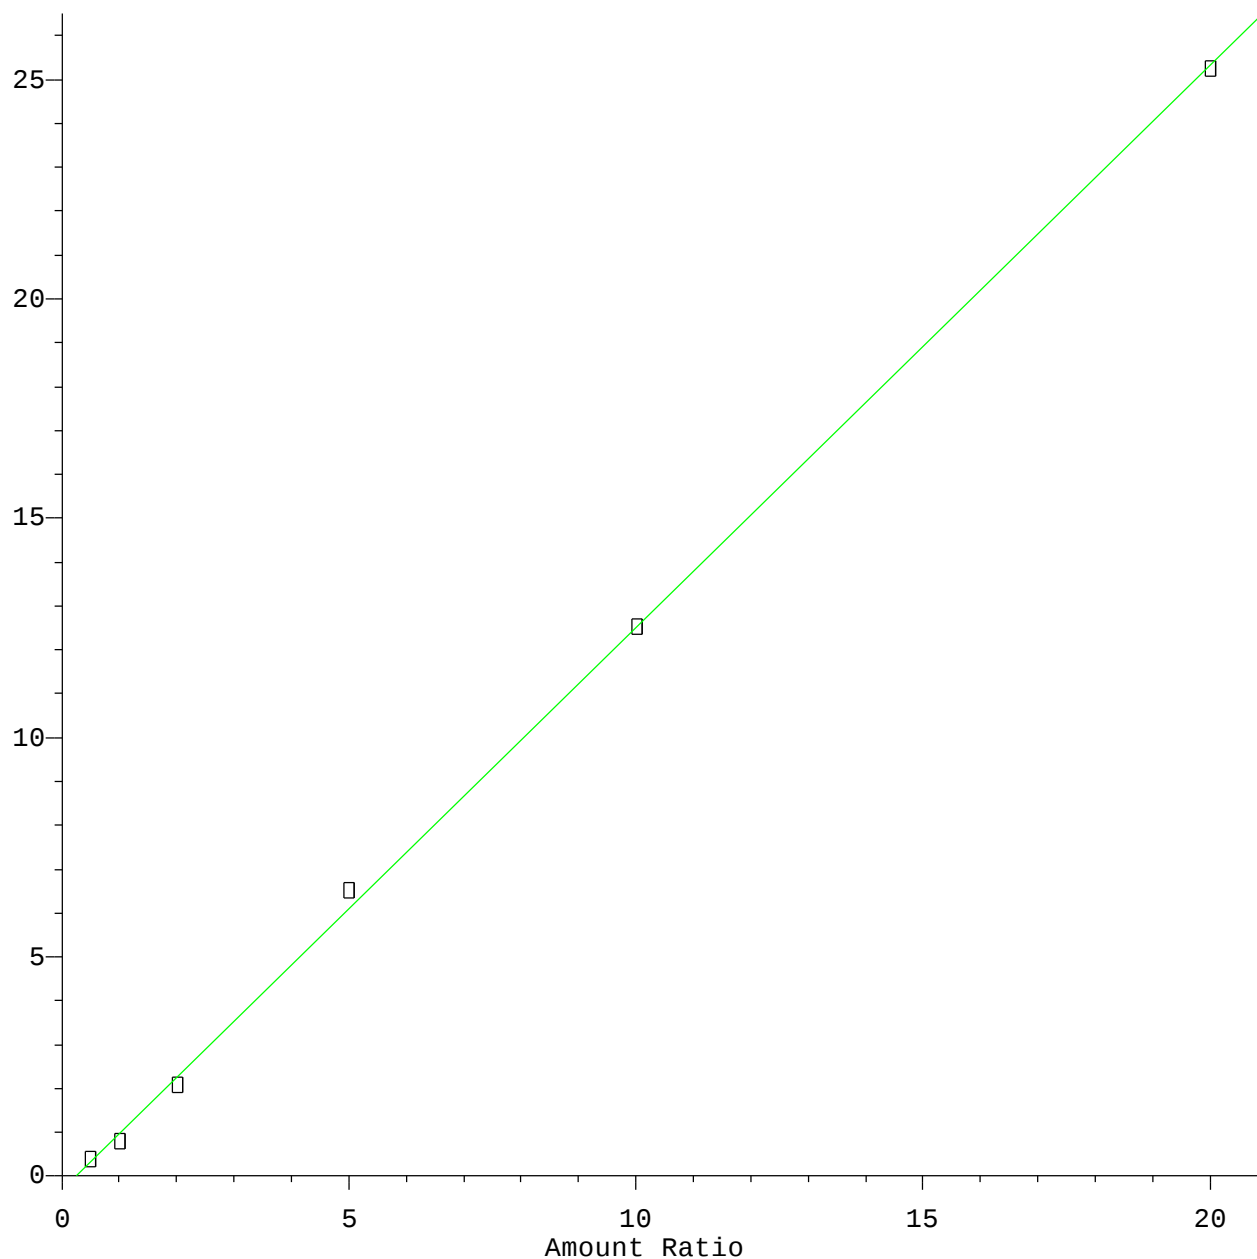


Resp Ratio = 1.28e+000 * Amt - 3.09e-001
Coef of Det (r²) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
Calibration Table Last Updated: Fri Oct 23 07:07:33 2020

p-Isopropyltoluene

Response Ratio

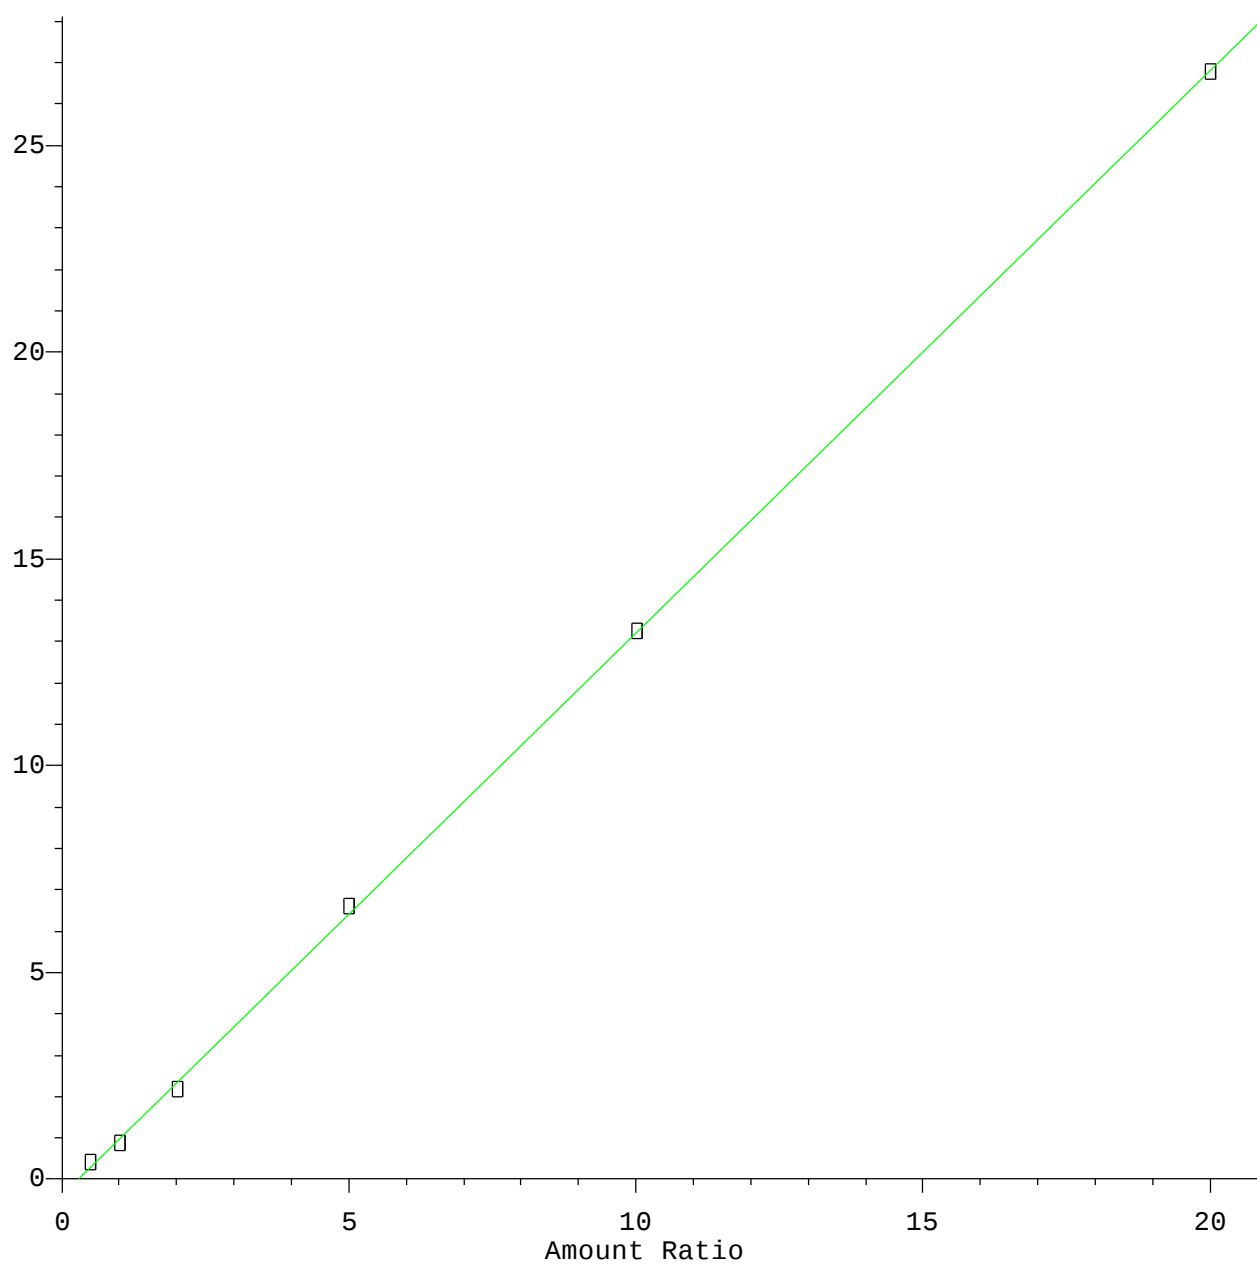


Resp Ratio = 1.36e+000 * Amt - 3.89e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
Calibration Table Last Updated: Fri Oct 23 07:07:33 2020

Naphthalene

Response Ratio

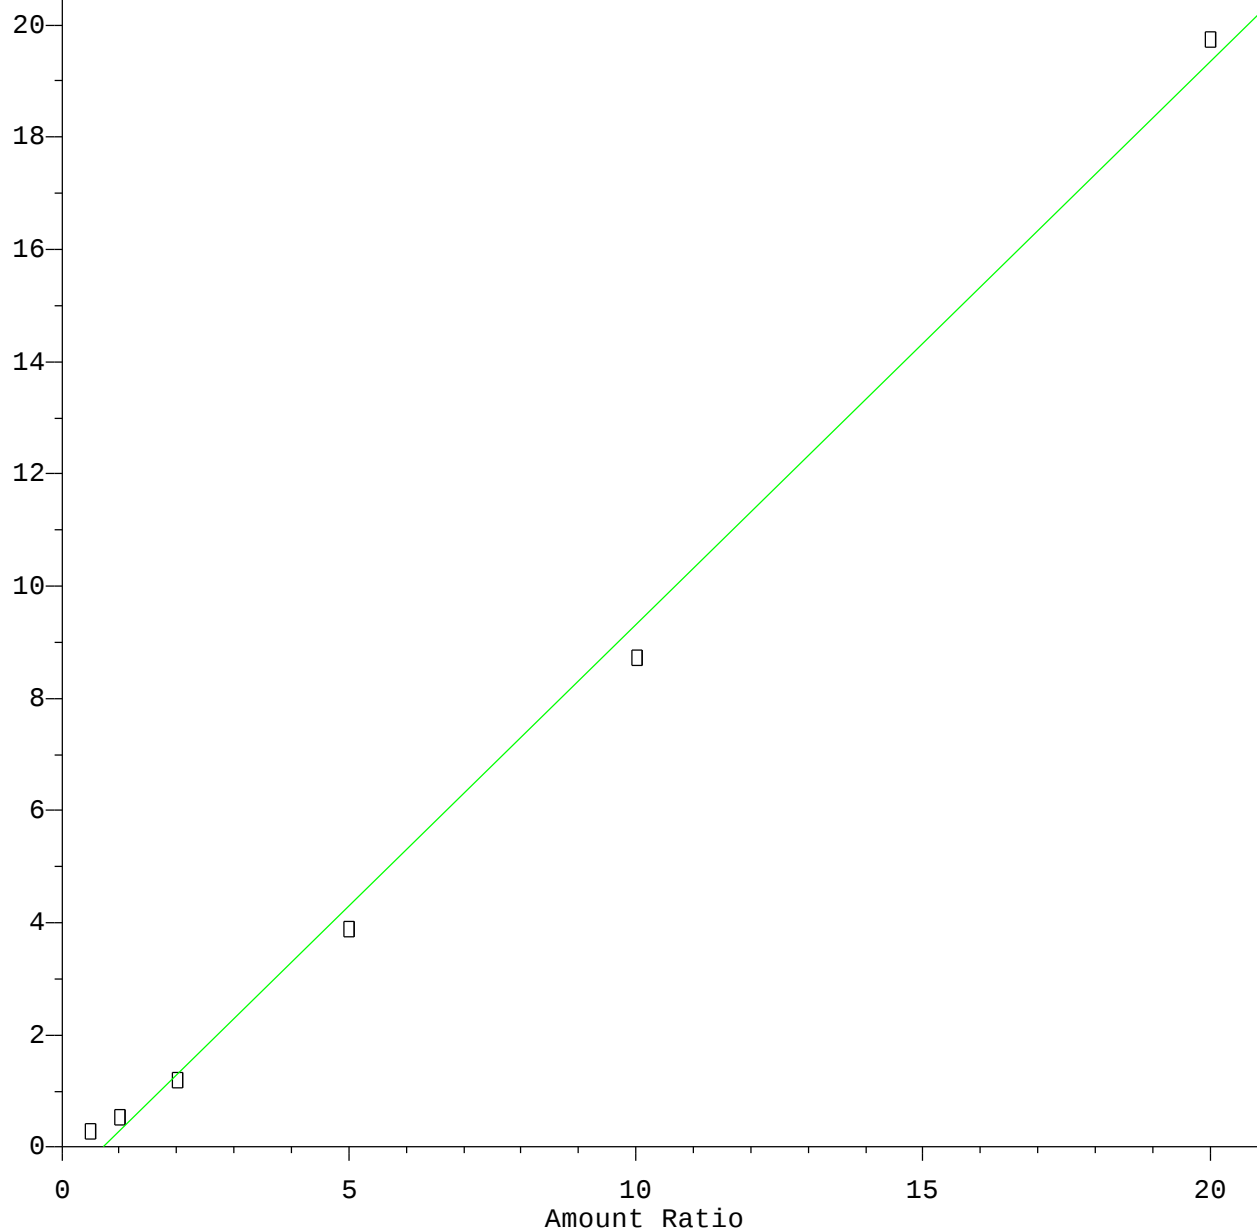


Resp Ratio = 1.00e+000 * Amt - 7.20e-001
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
Calibration Table Last Updated: Fri Oct 23 07:07:33 2020


Iodomethane

Response Ratio

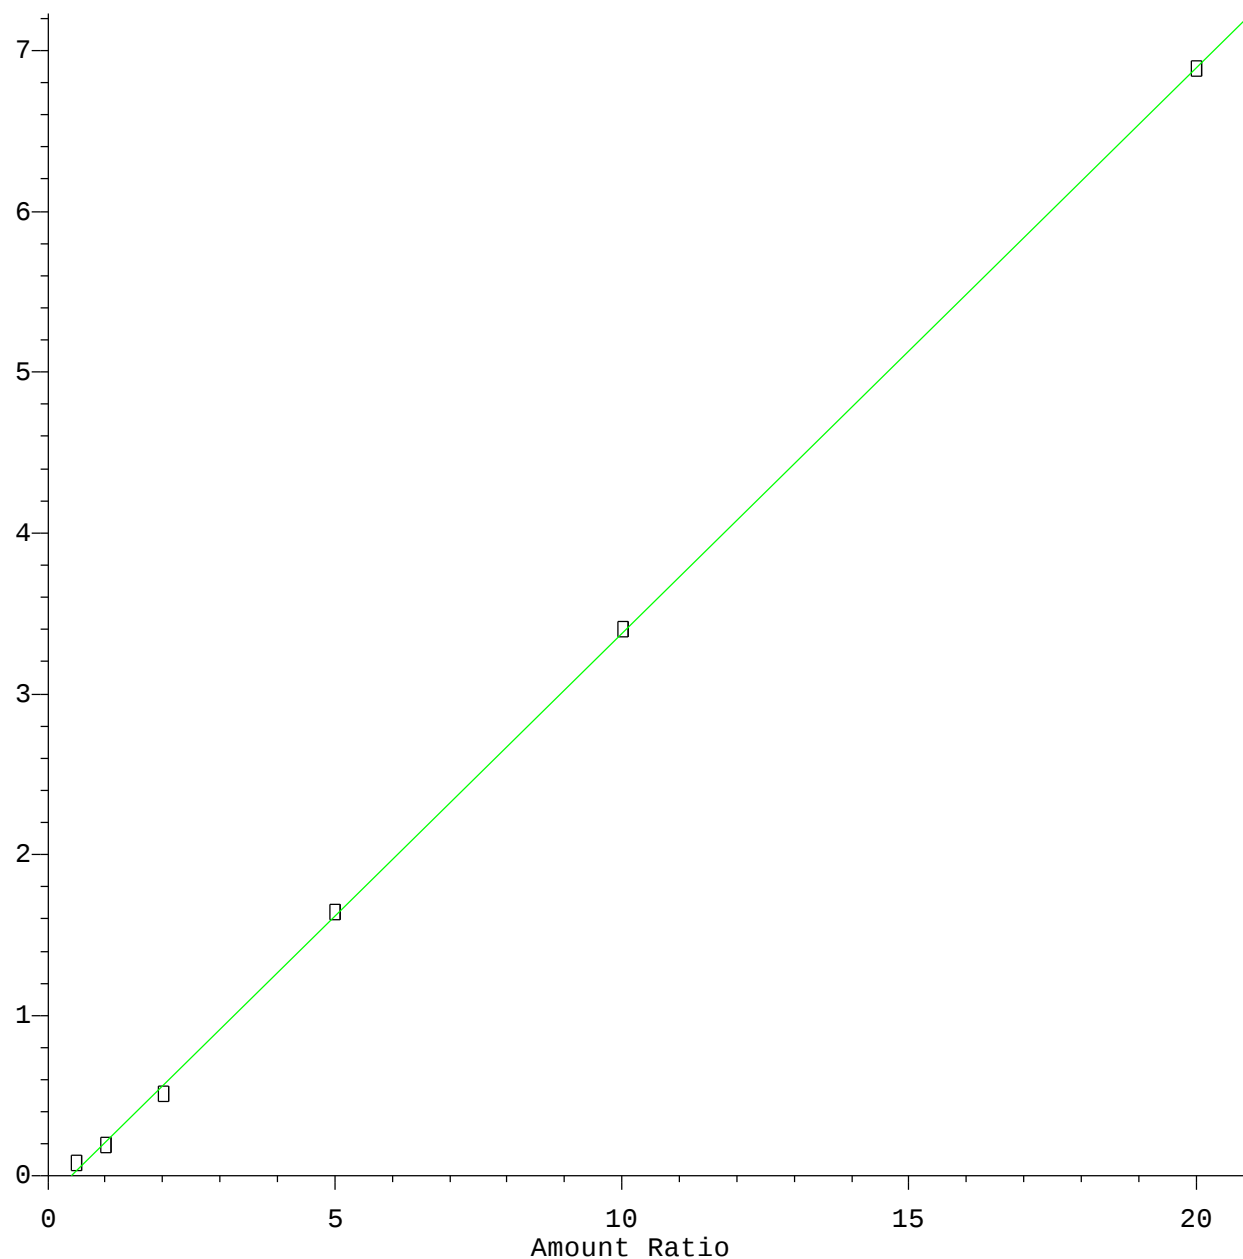

Resp Ratio = 3.52e-001 * Amt - 1.40e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
Calibration Table Last Updated: Fri Oct 23 07:07:33 2020

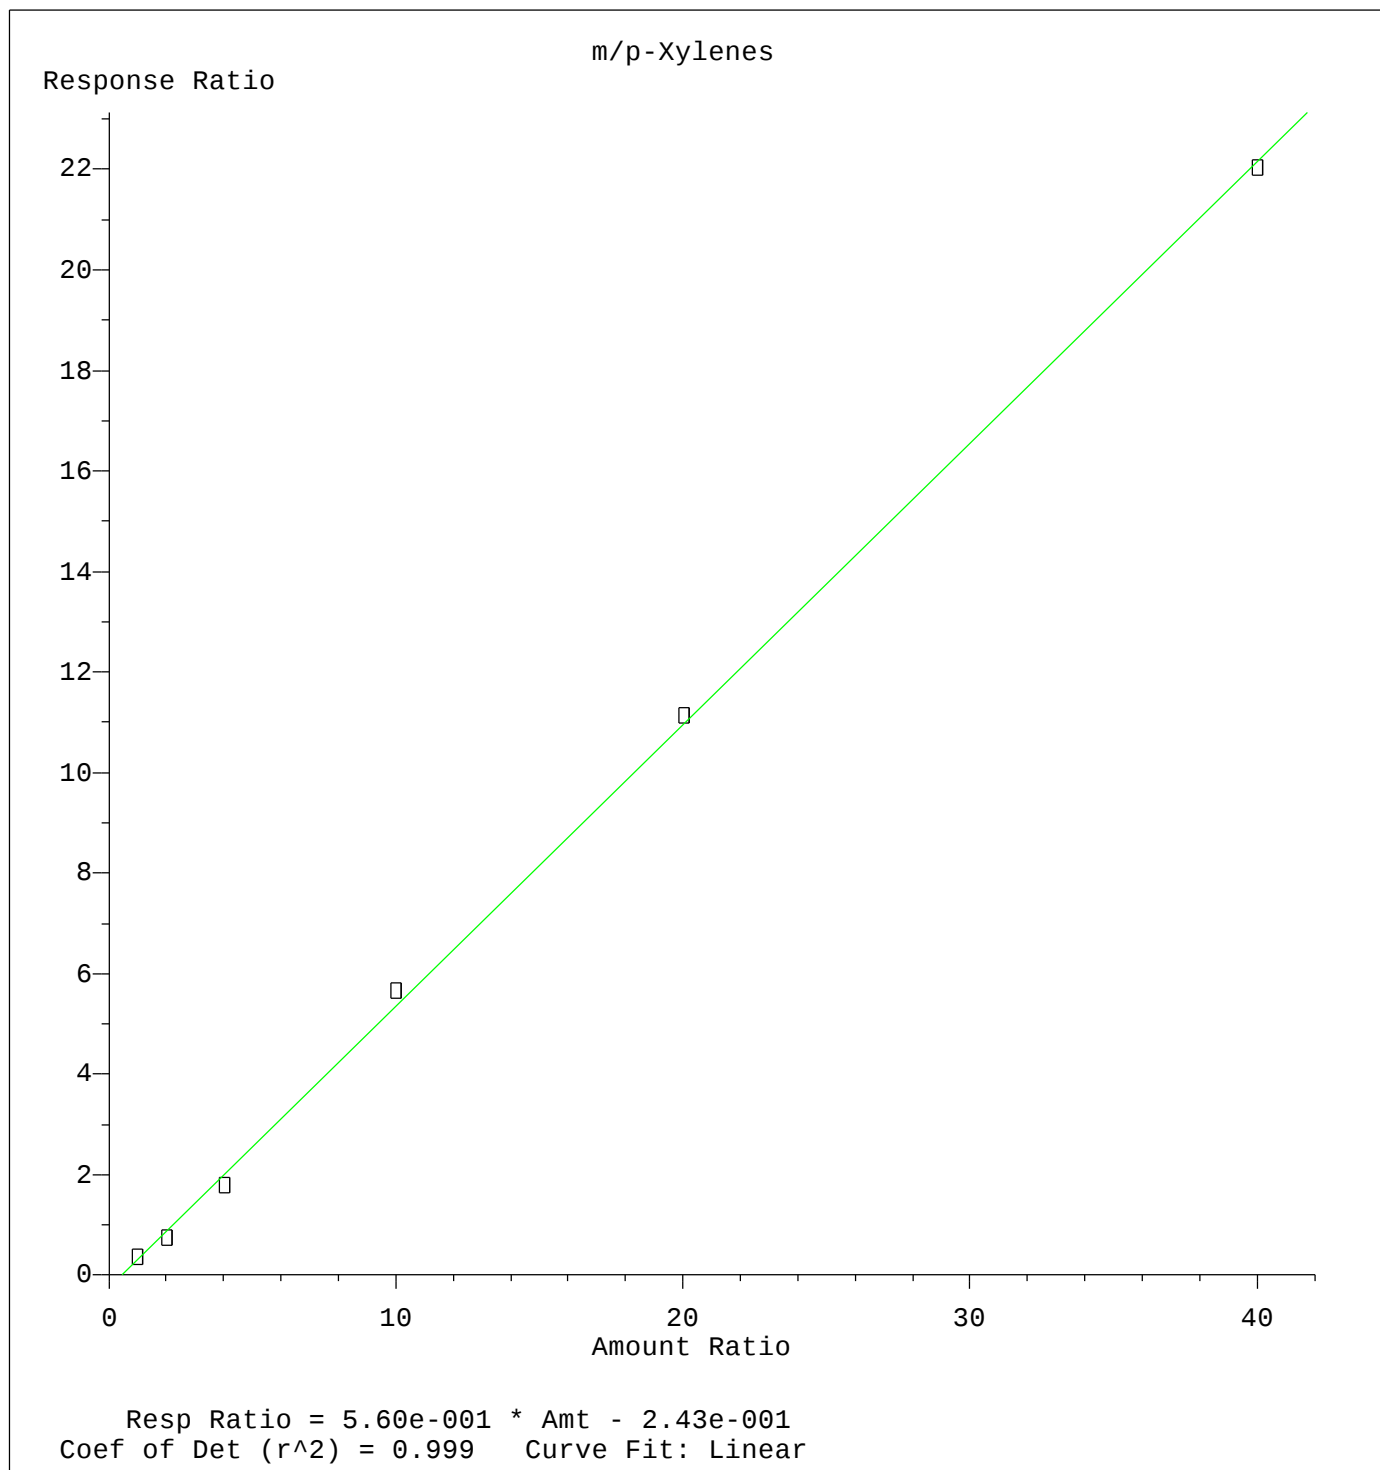

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
Calibration Table Last Updated: Fri Oct 23 07:07:33 2020