

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102220\
 Data File : VU040918.D
 Acq On : 22 Oct 2020 22:55
 Operator : SY/MD
 Sample : VU1022WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1022WBL01

Quant Time: Oct 23 07:27:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U102220DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Oct 23 07:07:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	6.13	96	53891	1.00	ug/l	0.00

System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.63	95	13949	0.71	ug/l	0.00
Spiked Amount 1.000			Recovery	=	71.00%	
68) 1,2-Dichlorobenzene-d4	12.19	152	14903	0.73	ug/l	0.00
Spiked Amount 1.000			Recovery	=	73.00%	


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102220\
Data File : VU040918.D
Acq On : 22 Oct 2020 22:55
Operator : SY/MD
Sample : VU1022WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1022WBL01

Quant Time: Oct 23 07:27:51 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U102220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Oct 23 07:07:33 2020
Response via : Initial Calibration

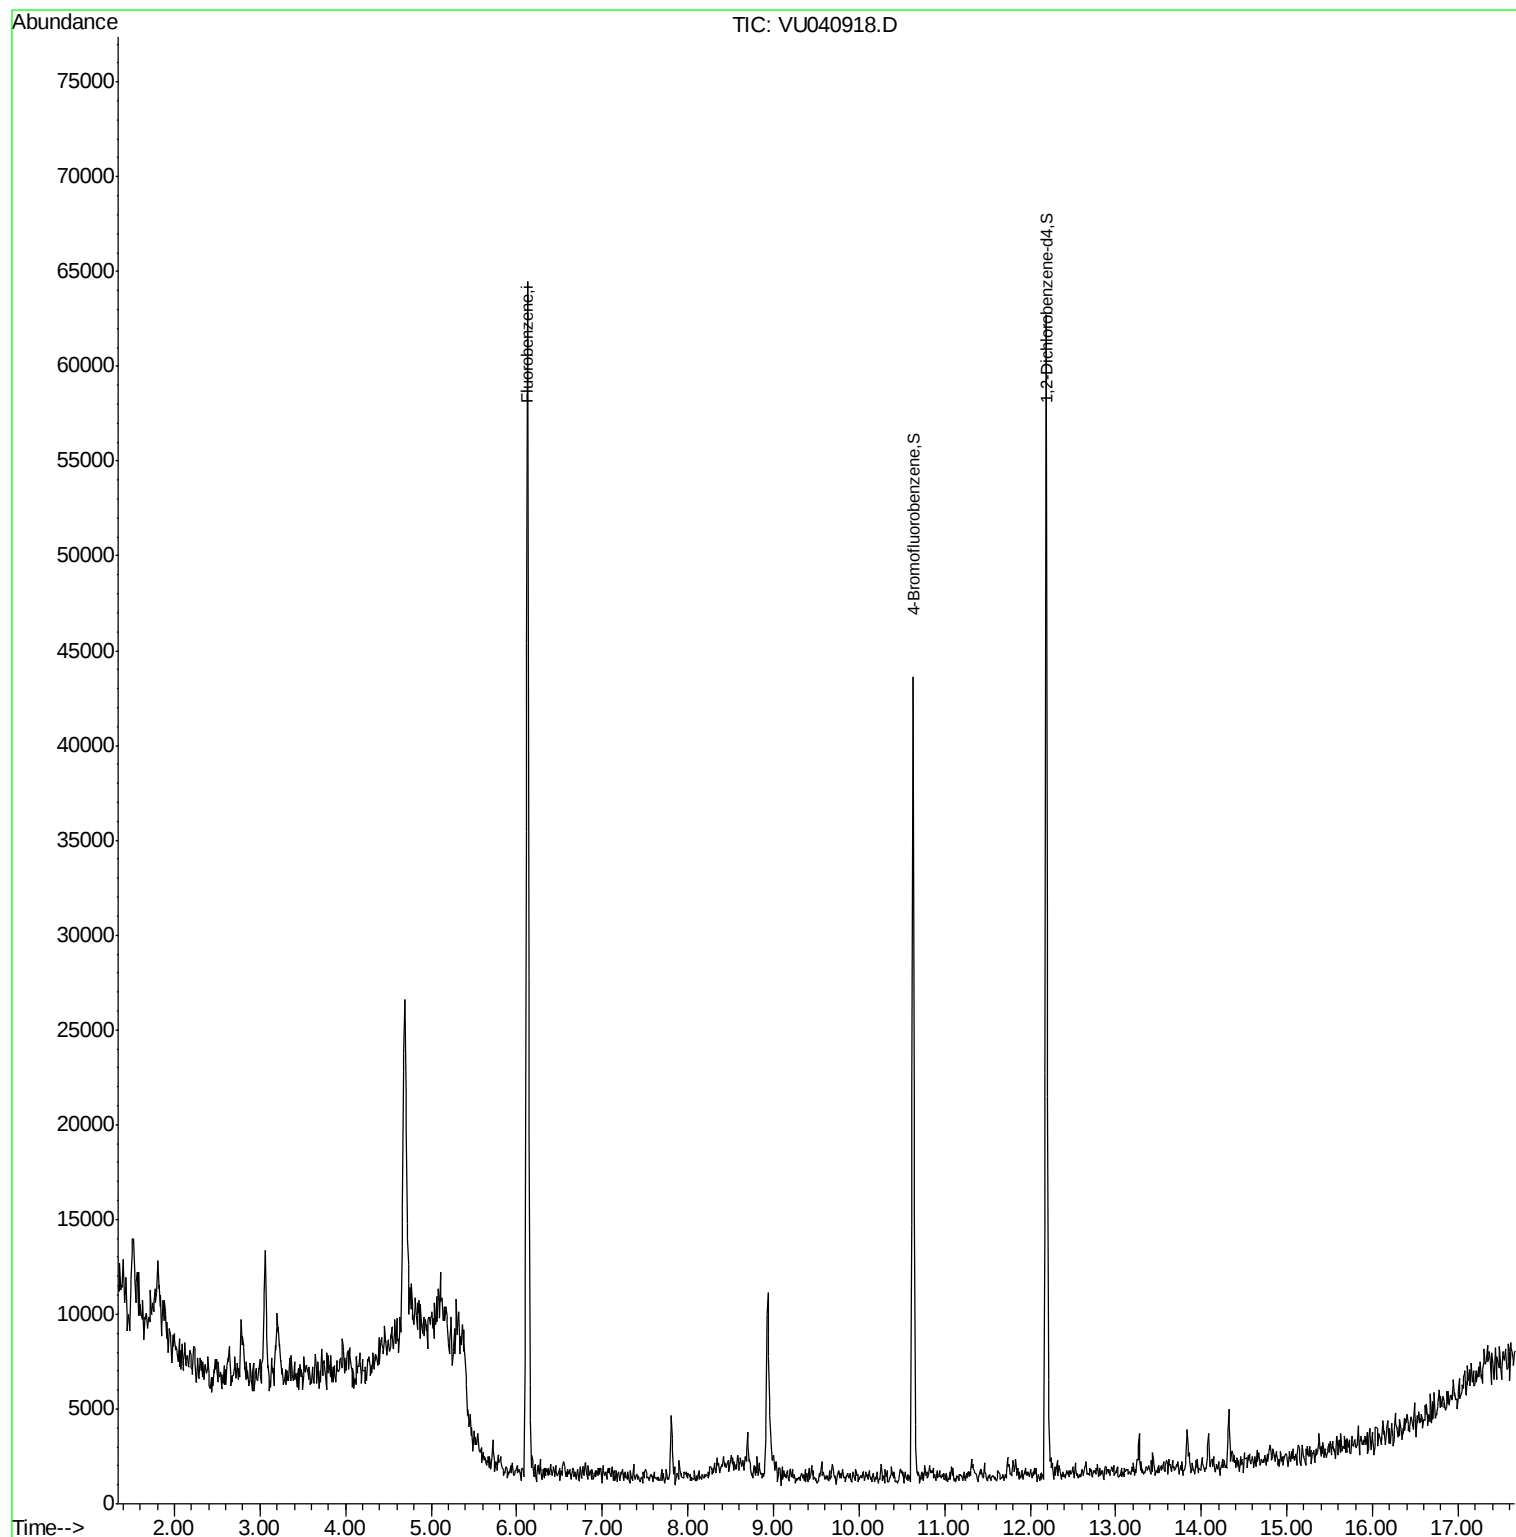

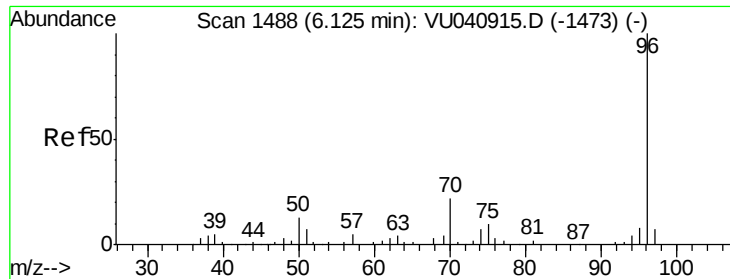

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 6.13 min Scan# 1489

Delta R.T. 0.00 min

Lab File: VU040918.D

Acq: 22 Oct 2020 22:55

Instrument :

MSVOA_U

ClientSampleId :

VU1022WBL01

Tot Ion: 96 Resp: 53891


Ion Ratio Lower Upper

96 100

70 20.8 16.3 24.5

95 9.0 7.3 10.9

97 5.6 0.0 0.0#



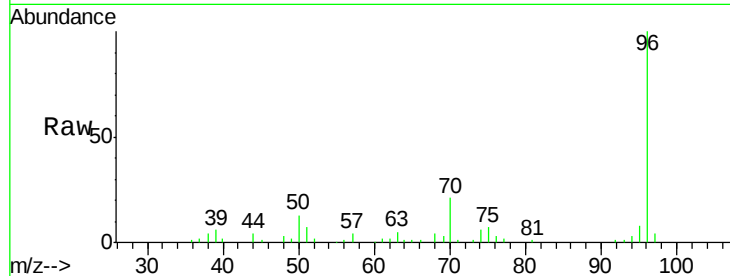


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

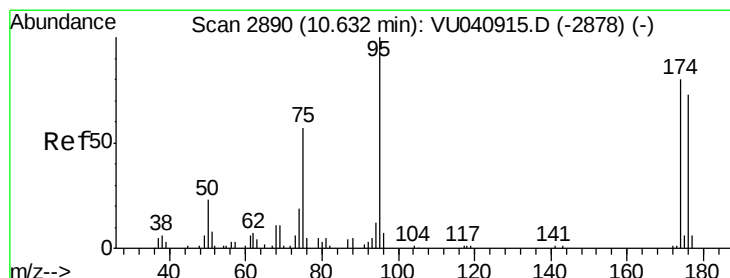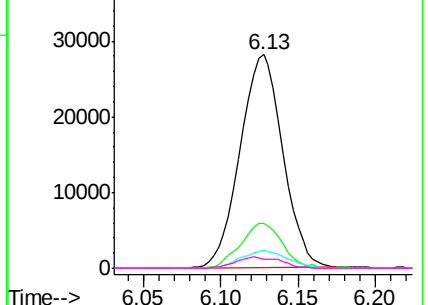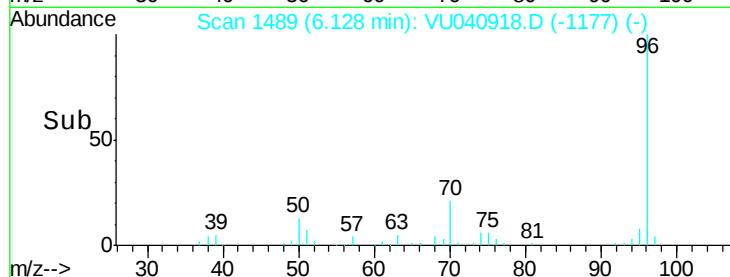

#57

4-Bromofluorobenzene

Concen: 0.709 ug/l

RT: 10.63 min Scan# 2890

Delta R.T. -0.00 min

Lab File: VU040918.D

Acq: 22 Oct 2020 22:55


Tgt Ion: 95 Resp: 13949

Ion Ratio Lower Upper

95 100

174 70.1 60.3 90.5



176 68.8 55.6 83.4

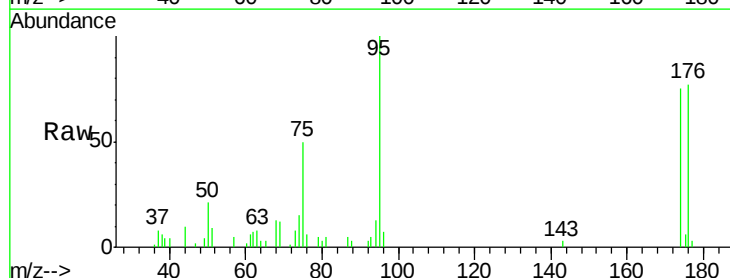


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

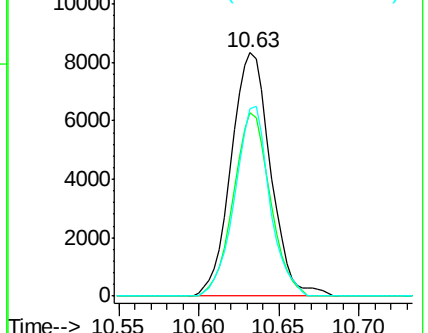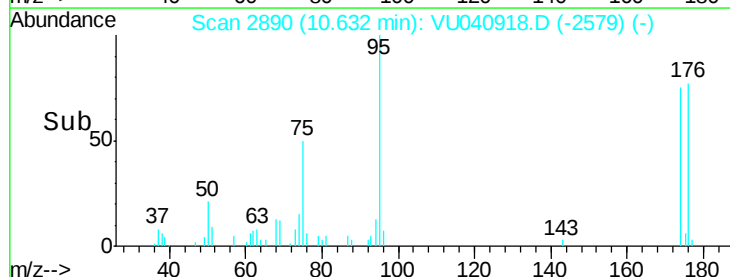


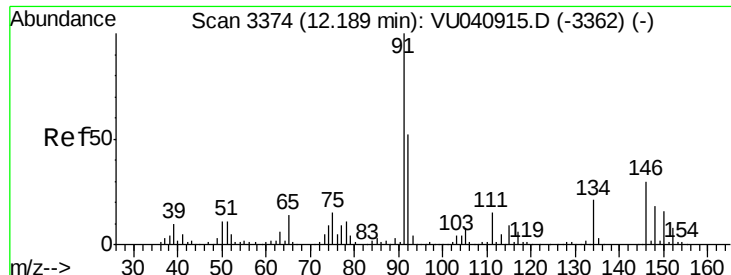

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.726 ug/l
 RT: 12.19 min Scan# 3374
 Delta R.T. -0.00 min
 Lab File: VU040918.D
 Acq: 22 Oct 2020 22:55

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1022WBL01

Tot Ion	Ratio	Lower	Upper
152	100		
115	66.6	0.0	323.4
150	156.5	0.0	653.8

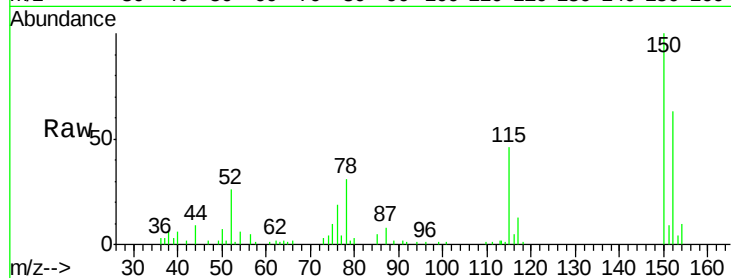

Abundance Ion 152.00 (151.70 to 152.70): V
 Ion 115.00 (114.70 to 115.70): V
 Ion 150.00 (149.70 to 150.70): V

