


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102221\
 Data File : VU045354.D
 Acq On : 22 Oct 2021 09:04
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U092821W.M
 Title : SW846 8260
 Last Update : Tue Sep 28 12:32:13 2021

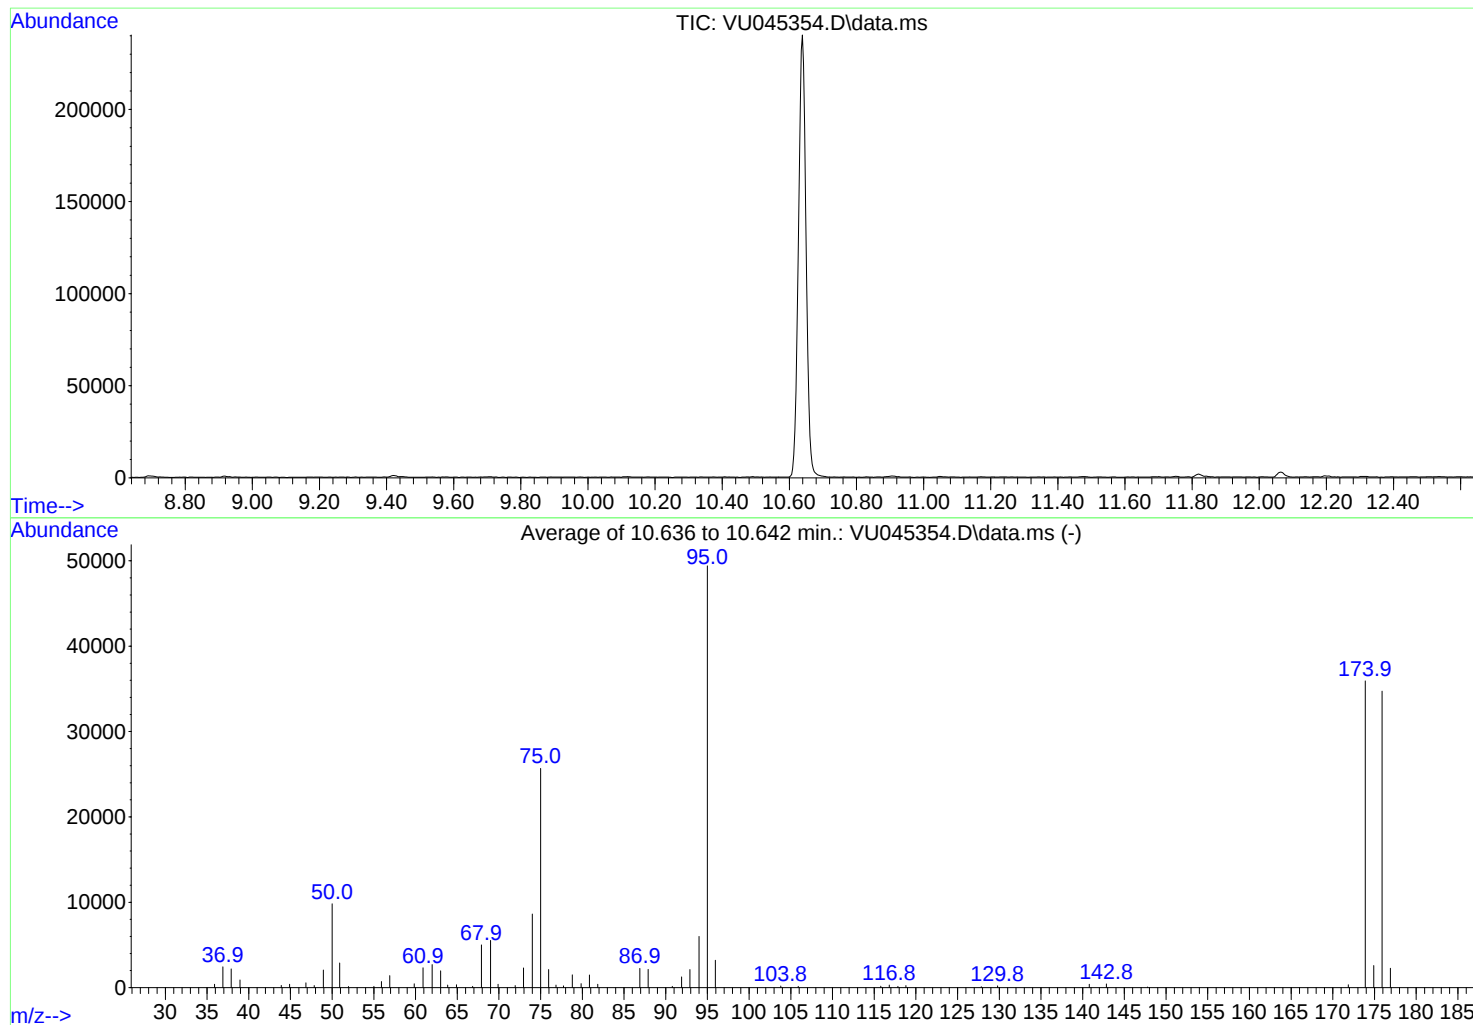

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	9828	PASS
75	95	30	60	52.0	25685	PASS
95	95	100	100	100.0	49411	PASS
96	95	5	9	6.5	3207	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.7	35933	PASS
175	174	5	9	7.2	2584	PASS
176	174	95	101	96.7	34736	PASS
177	176	5	9	6.6	2276	PASS