

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102318\
 Data File : VU027763.D
 Acq On : 23 Oct 2018 15:21
 Operator : MD/SY
 Sample : J5617-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PANTRY-COOLER

Quant Time: Oct 24 09:28:18 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U0102318DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Oct 23 09:12:15 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----	-----	-----	-----	-----	-----	-----
1) Fluorobenzene	5.75	96	11235	1.00	ug/l	0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.31	95	4183	0.98	ug/l	0.00
Spiked Amount 1.000			Recovery	=	98.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	3771	0.94	ug/l	0.00
Spiked Amount 1.000			Recovery	=	94.00%	
Target Compounds						Ovalue
27) Chloroform	4.68	83	26378	4.401	ug/l	95
-----	-----	-----	-----	-----	-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102318\
Data File : VU027763.D
Acq On : 23 Oct 2018 15:21
Operator : MD/SY
Sample : J5617-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PANTRY-COOLER

Quant Time: Oct 24 09:28:18 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U0102318DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Oct 23 09:12:15 2018
Response via : Initial Calibration

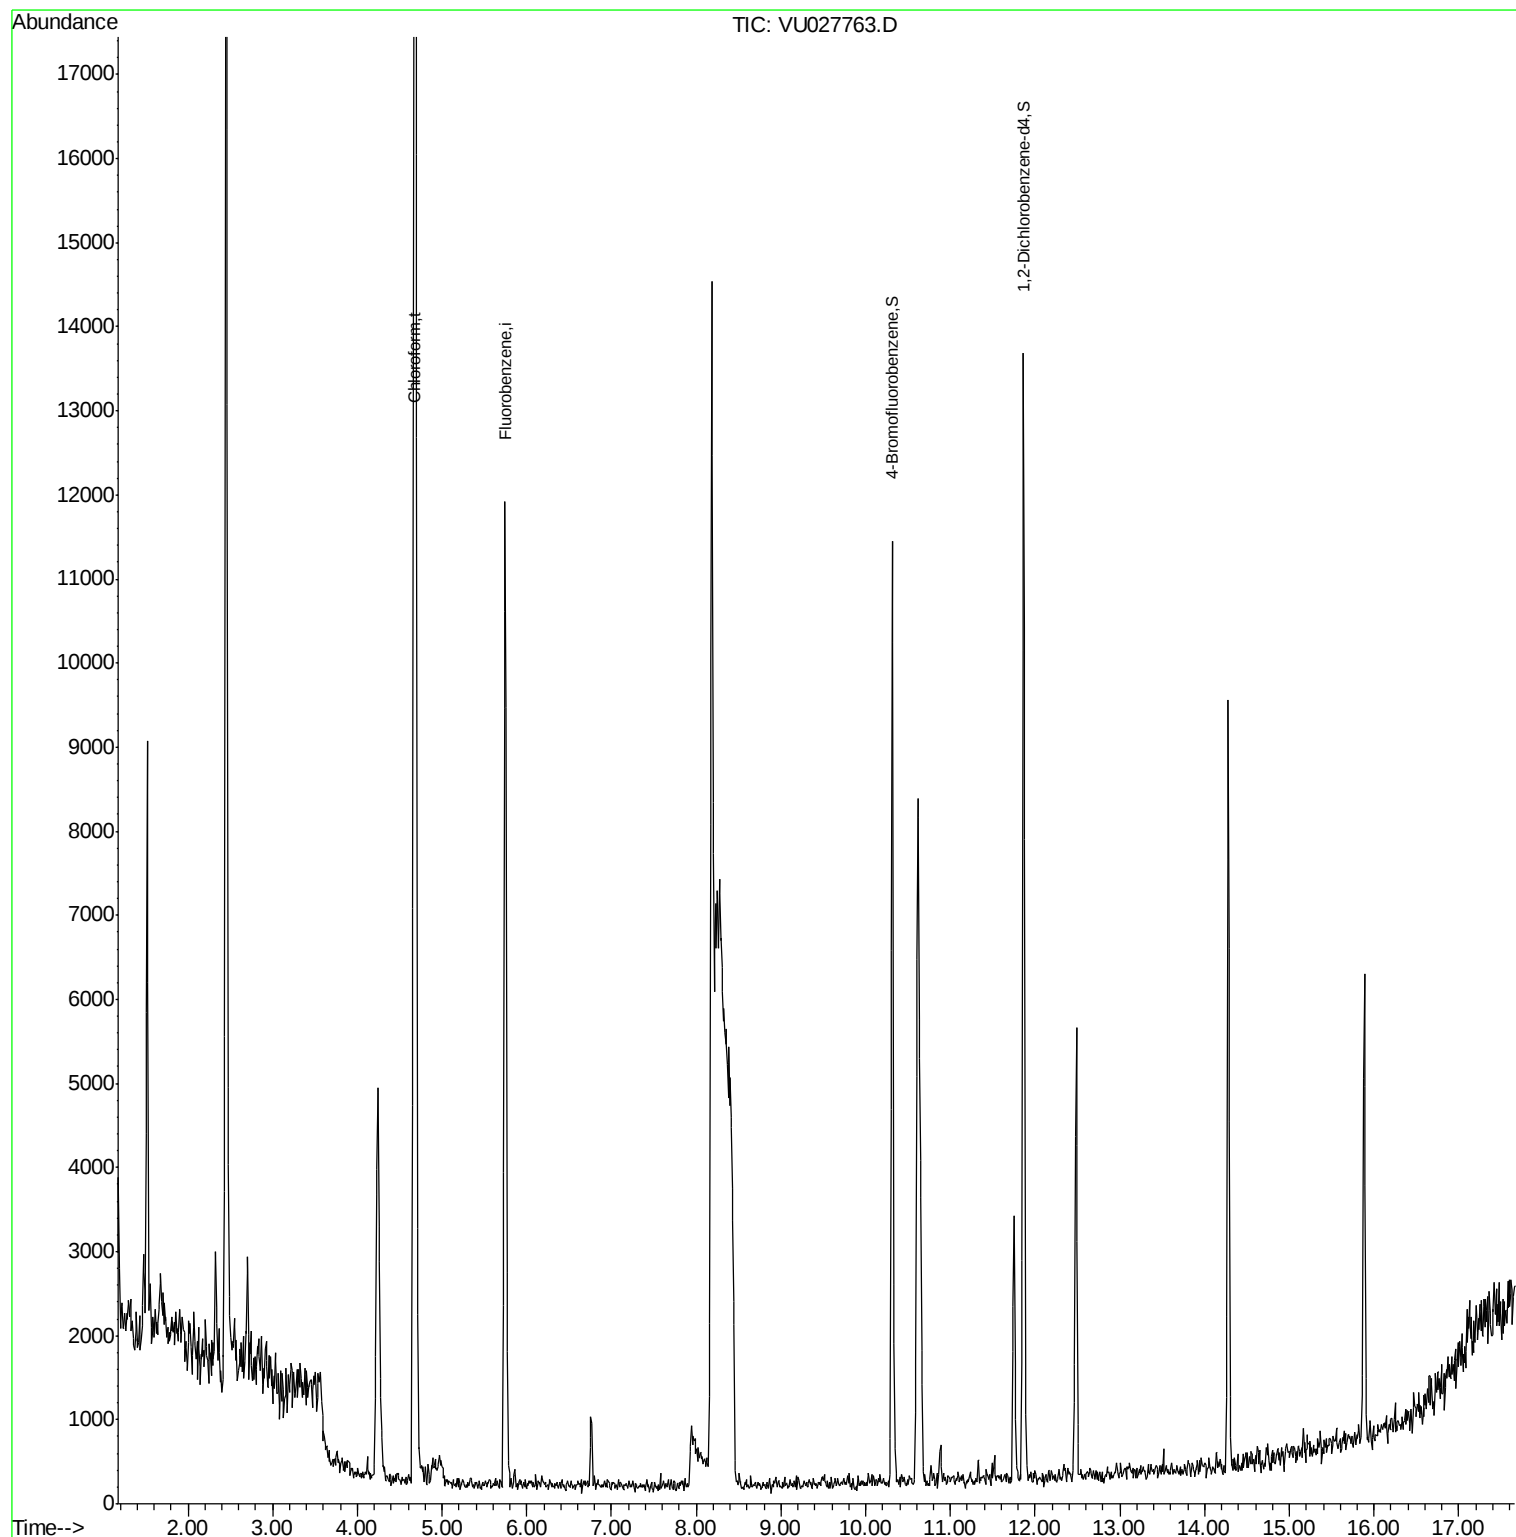

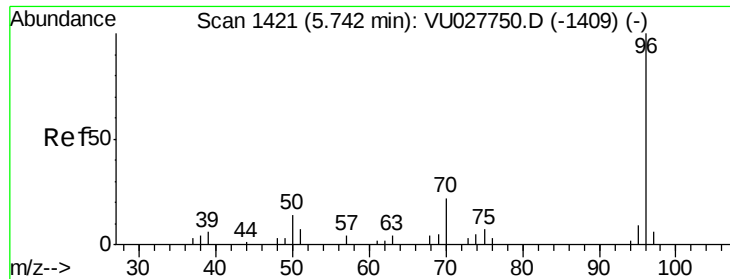

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.75 min Scan# 1422

Delta R.T. 0.00 min

Lab File: VU027763.D

Acq: 23 Oct 2018 15:21

Instrument :

MSVOA_U

ClientSampleId :

PANTRY-COOLER

Tot Ion: 96 Resp: 11235


Ion Ratio Lower Upper

96 100

70 23.5 17.7 26.5

95 9.2 7.0 10.6

97 6.1 0.0 0.0#



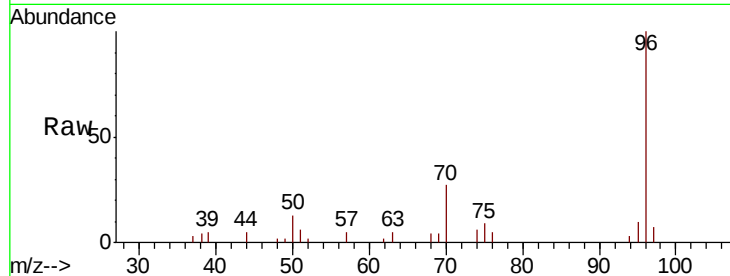


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

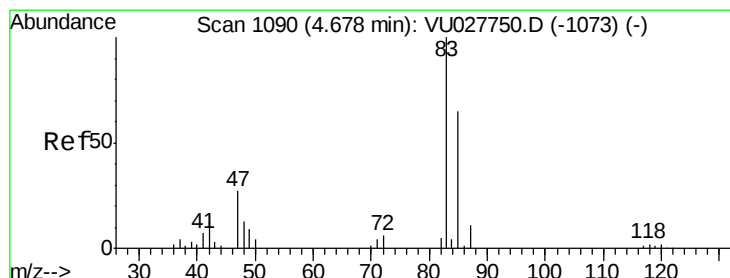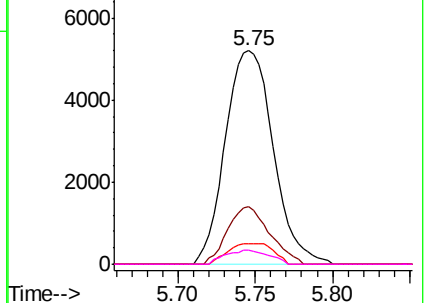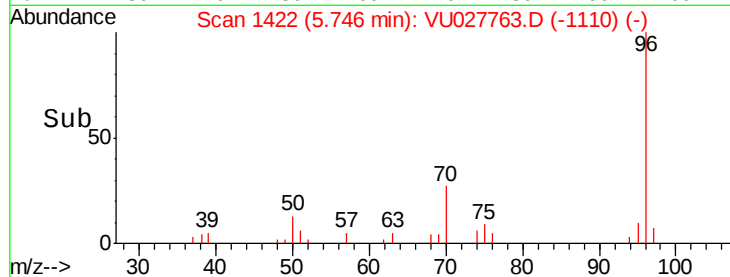

#27

Chloroform

Concen: 4.401 ug/l

RT: 4.68 min Scan# 1090

Delta R.T. 0.00 min

Lab File: VU027763.D


Acq: 23 Oct 2018 15:21

Tgt Ion: 83 Resp: 26378

Ion Ratio Lower Upper



83 100


85 60.9 0.0 130.2

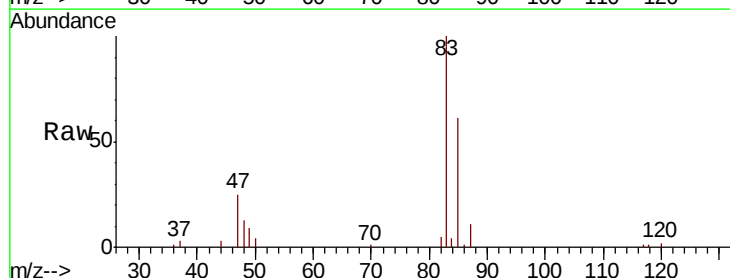

Abundance Ion 83.00 (82.70 to 83.70): VU0

Ion 85.00 (84.70 to 85.70): VU0



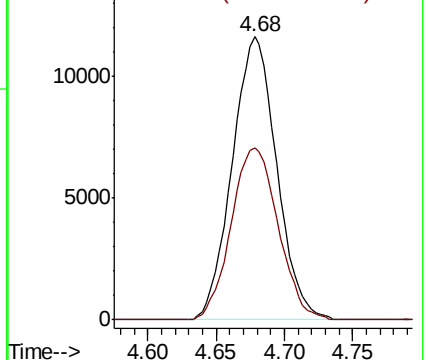
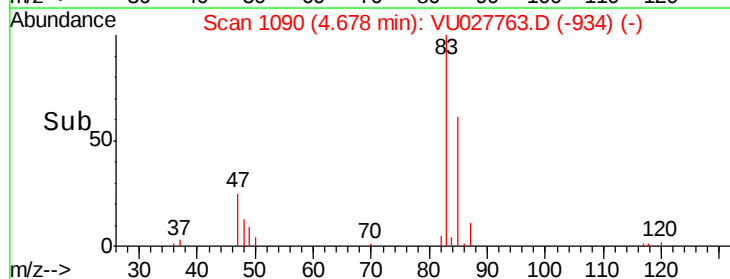


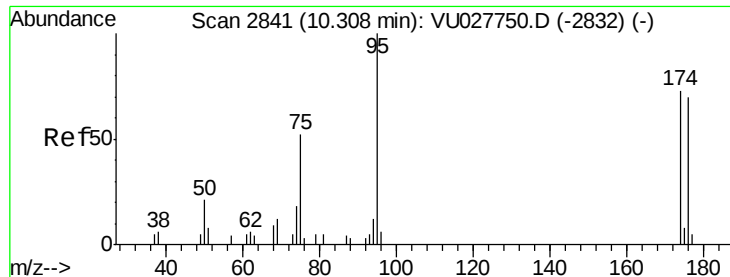

#57
 4-Bromofluorobenzene
 Concen: N.D. ug/l
 RT: 10.31 min Scan# 2842
 Delta R.T. 0.00 min
 Lab File: VU027763.D
 Acq: 23 Oct 2018 15:21

Instrument :
 MSVOA_U
 ClientSampleId :
 PANTRY-COOLER

Tot Ion: 95 Resp: 4183
 Ion Ratio Lower Upper
 95 100
 174 76.4 64.5 96.7
 176 81.7 58.3 87.5

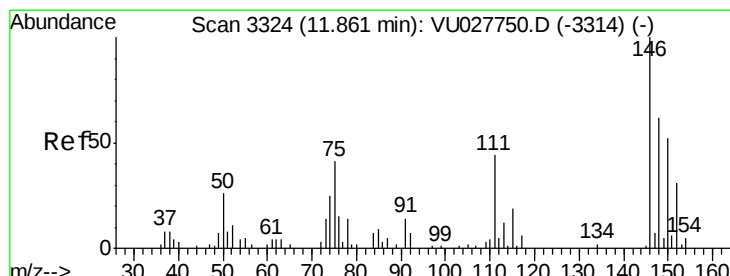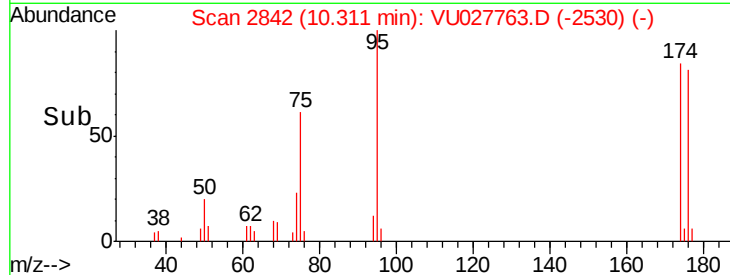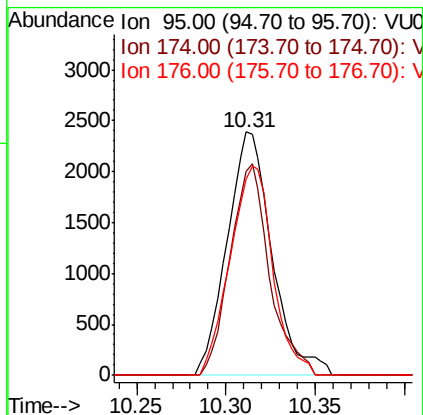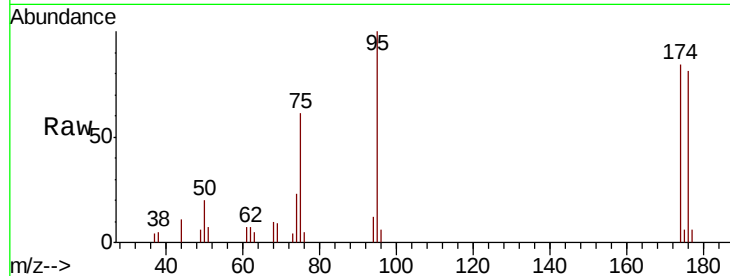

#68
 1,2-Dichlorobenzene-d4
 Concen: N.D. ug/l
 RT: 11.86 min Scan# 3324
 Delta R.T. 0.00 min
 Lab File: VU027763.D
 Acq: 23 Oct 2018 15:21

Tgt Ion: 152 Resp: 3771
 Ion Ratio Lower Upper
 152 100
 115 66.7 0.0 130.2
 150 161.2 0.0 650.6

