

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102318\
Data File : VU027757.D
Acq On : 23 Oct 2018 10:27
Operator : MD/SY
Sample : J5026-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
1713

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA U\METHOD\524U0102318DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.247	941	956	976	rBV2	4661	13288	1.66%	0.606%
2	4.675	1069	1089	1115	rBV	349760	801075	100.00%	36.558%
3	5.742	1409	1421	1442	rVB	15748	30956	3.86%	1.413%
4	6.758	1723	1737	1763	rBV	236421	434206	54.20%	19.816%
5	8.189	2169	2182	2185	rBV	4623	8178	1.02%	0.373%
6	8.479	2260	2272	2293	rVB	304143	514087	64.17%	23.461%
7	8.623	2308	2317	2331	rBV3	8666	13815	1.72%	0.630%
8	9.958	2719	2732	2752	rBV	185239	303951	37.94%	13.871%
9	10.311	2833	2842	2854	rVB2	16028	23856	2.98%	1.089%
10	10.623	2926	2939	2959	rBV2	3633	10628	1.33%	0.485%
11	11.861	3314	3324	3339	rVB2	17793	28923	3.61%	1.320%
12	14.279	4066	4076	4092	rVB2	4978	8259	1.03%	0.377%


Sum of corrected areas: 2191222

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102318\
Data File : VU027757.D
Acq On : 23 Oct 2018 10:27
Operator : MD/SY
Sample : J5026-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
1713

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U0102318DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

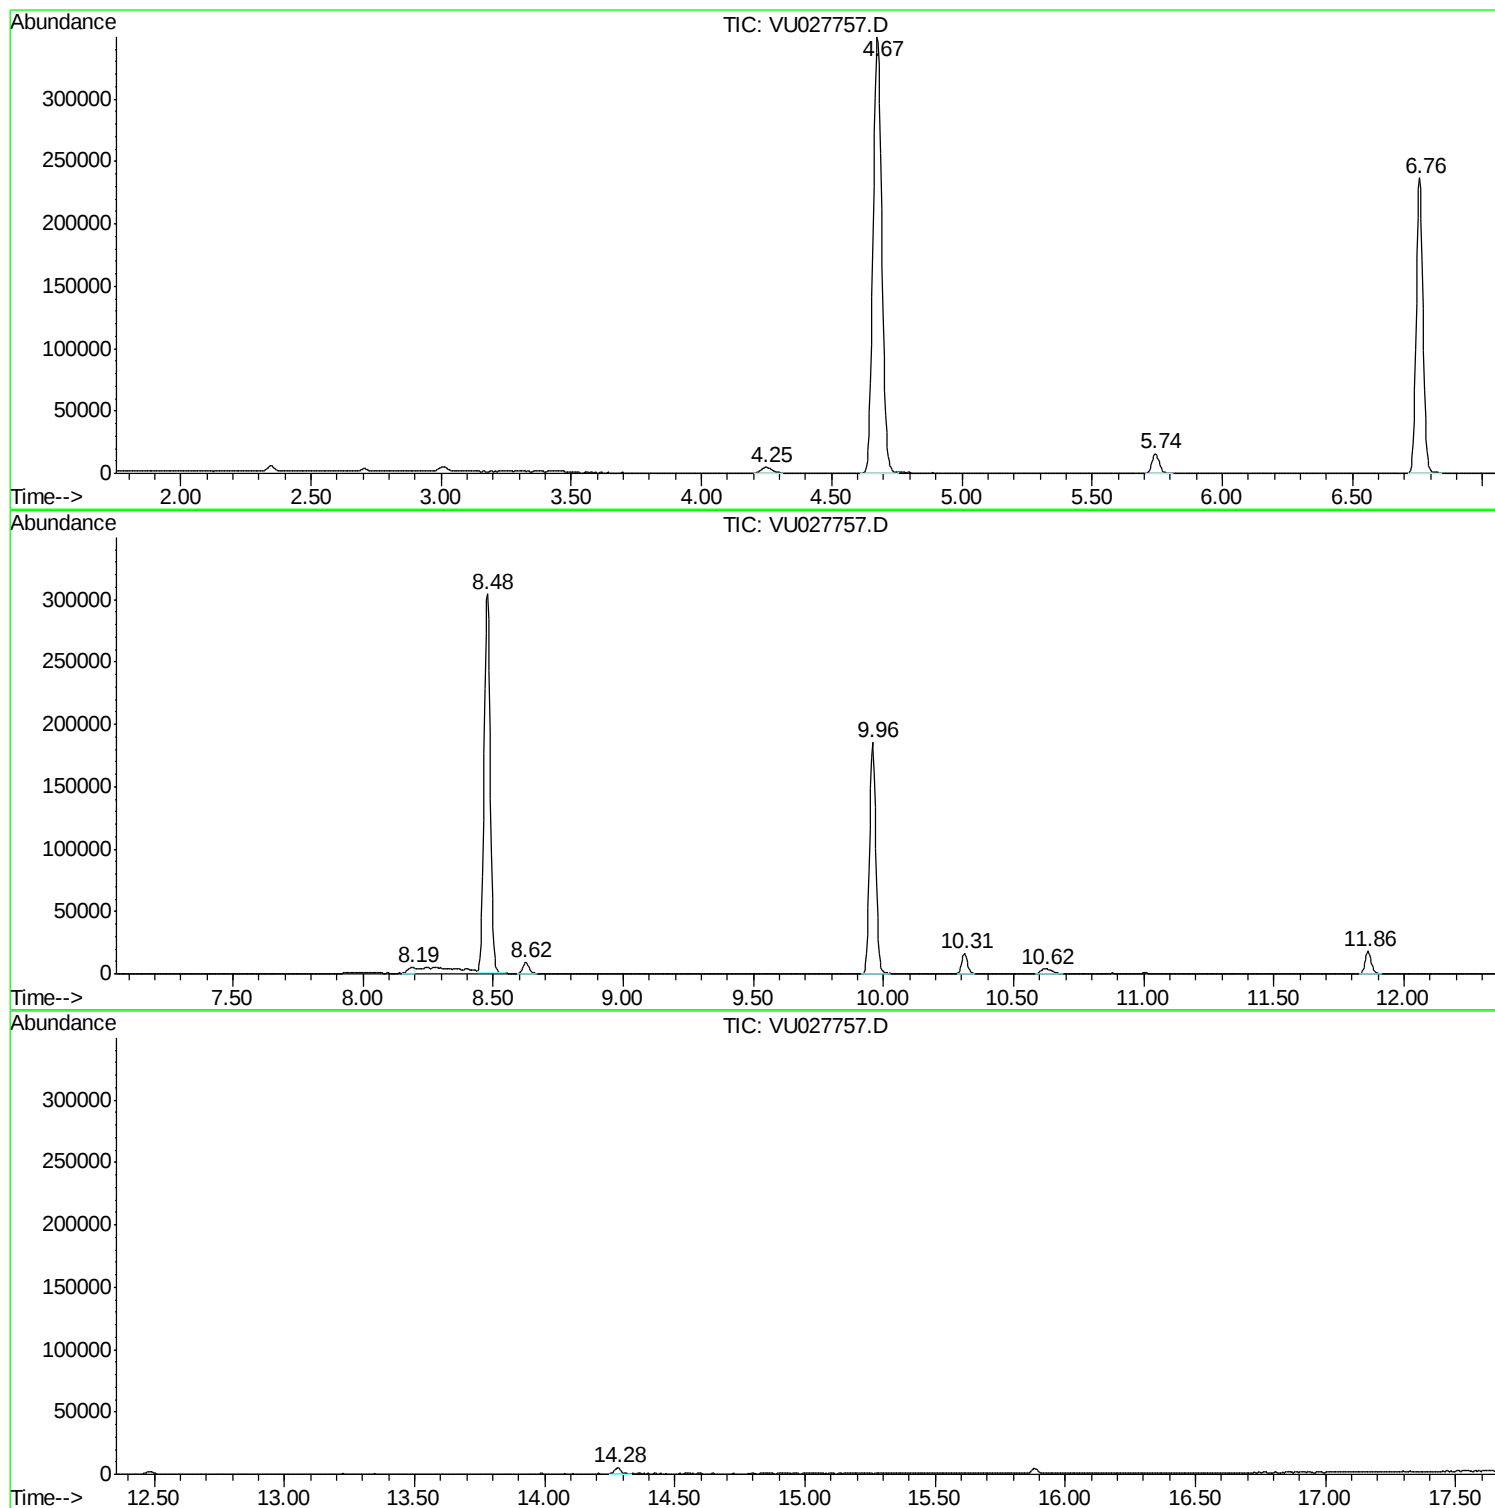

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102318\
Data File : VU027757.D
Acq On : 23 Oct 2018 10:27
Operator : MD/SY
Sample : J5026-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
1713










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U0102318DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown8.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.62	0.45 ug/l	13815	Fluorobenzene	5.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Benzene, 1,3-dimethyl-5-(1-methyl-...	148	C11H16	004706-90-5	17
2		5-Methyl-7-amino-s-triazolo(1,5-...	149	C6H7N5	033376-96-4	9
3		6,7-Dimethyl-triazolo(3,4-c)(1,2...	149	C6H7N5	061139-79-5	9
4		6,7-Dimethyl-triazolo(3,4-c)(1,2...	149	C6H7N5	061139-79-5	9
5		2-tert-Butyltoluene	148	C11H16	001074-92-6	9

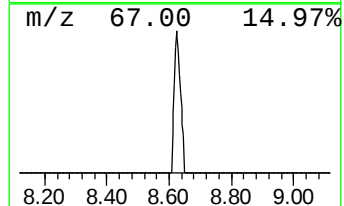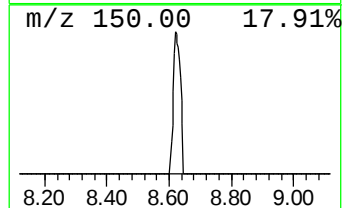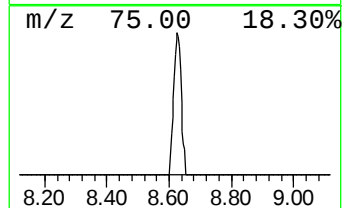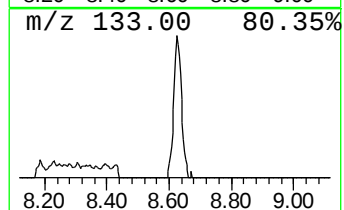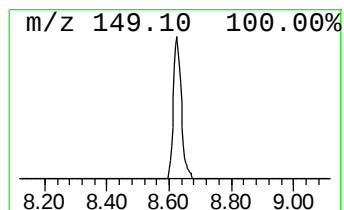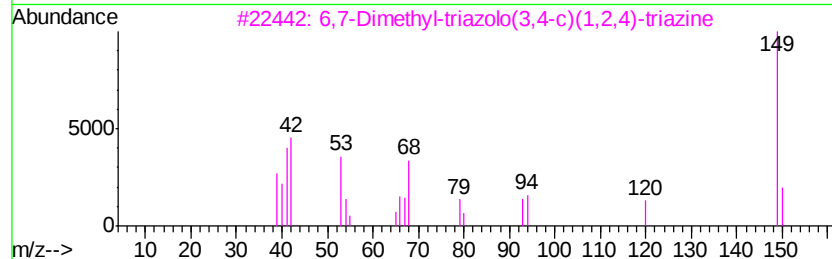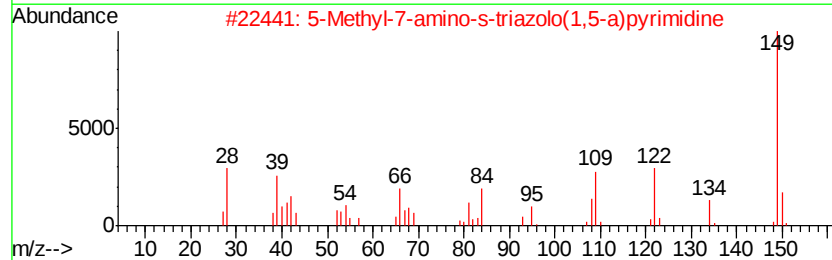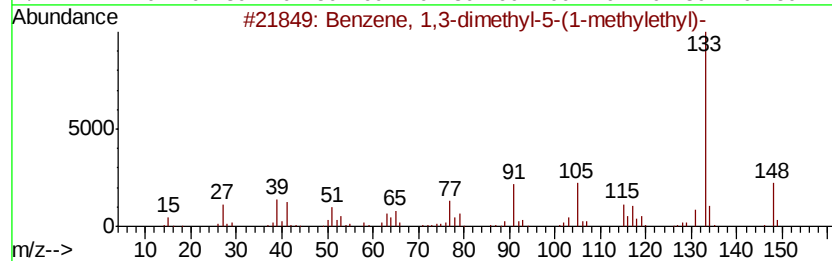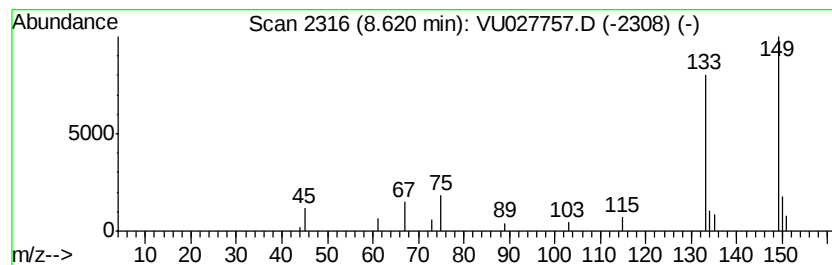

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU102318\
Data File : VU027757.D
Acq On : 23 Oct 2018 10:27
Operator : MD/SY
Sample : J5026-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
1713

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U0102318DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown8.62	8.62	0.5	ug/l	13815	1	5.74	30956	1.0