


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102318\
Data File : VU027745.D
Acq On : 22 Oct 2018 17:04
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U0102318DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Oct 23 09:12:15 2018

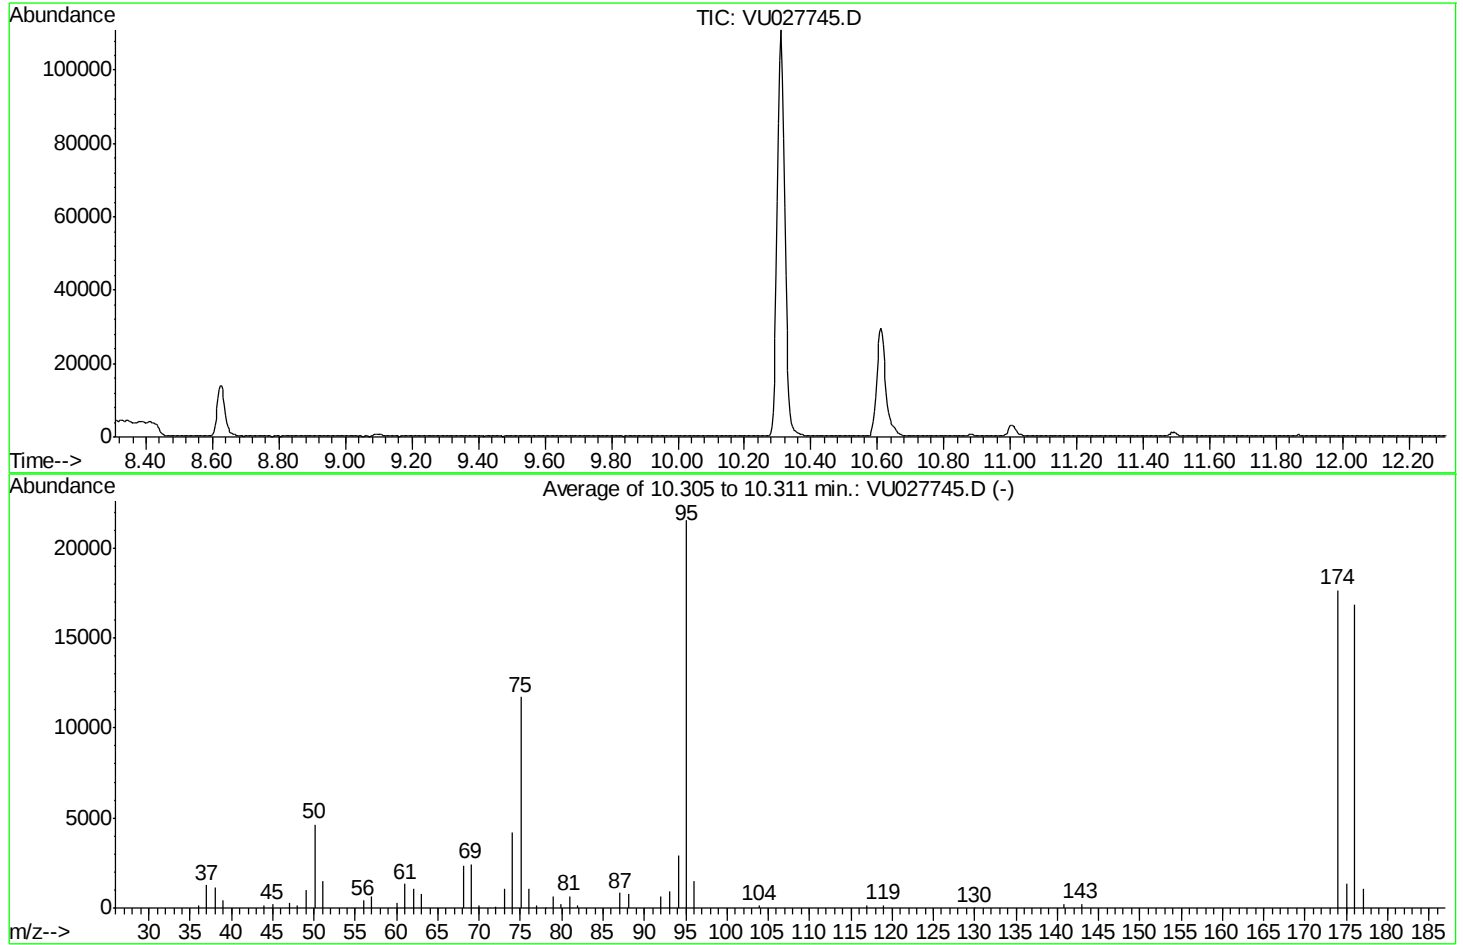

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	4657	PASS
75	95	30	60	54.4	11718	PASS
95	95	100	100	100.0	21530	PASS
96	95	5	9	6.9	1475	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.0	17659	PASS
175	174	5	9	7.7	1354	PASS
176	174	95	101	95.5	16857	PASS
177	176	5	9	6.3	1060	PASS