


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102318\
Data File : VU027753.D
Acq On : 23 Oct 2018 07:42
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U0102318DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Oct 23 09:12:15 2018

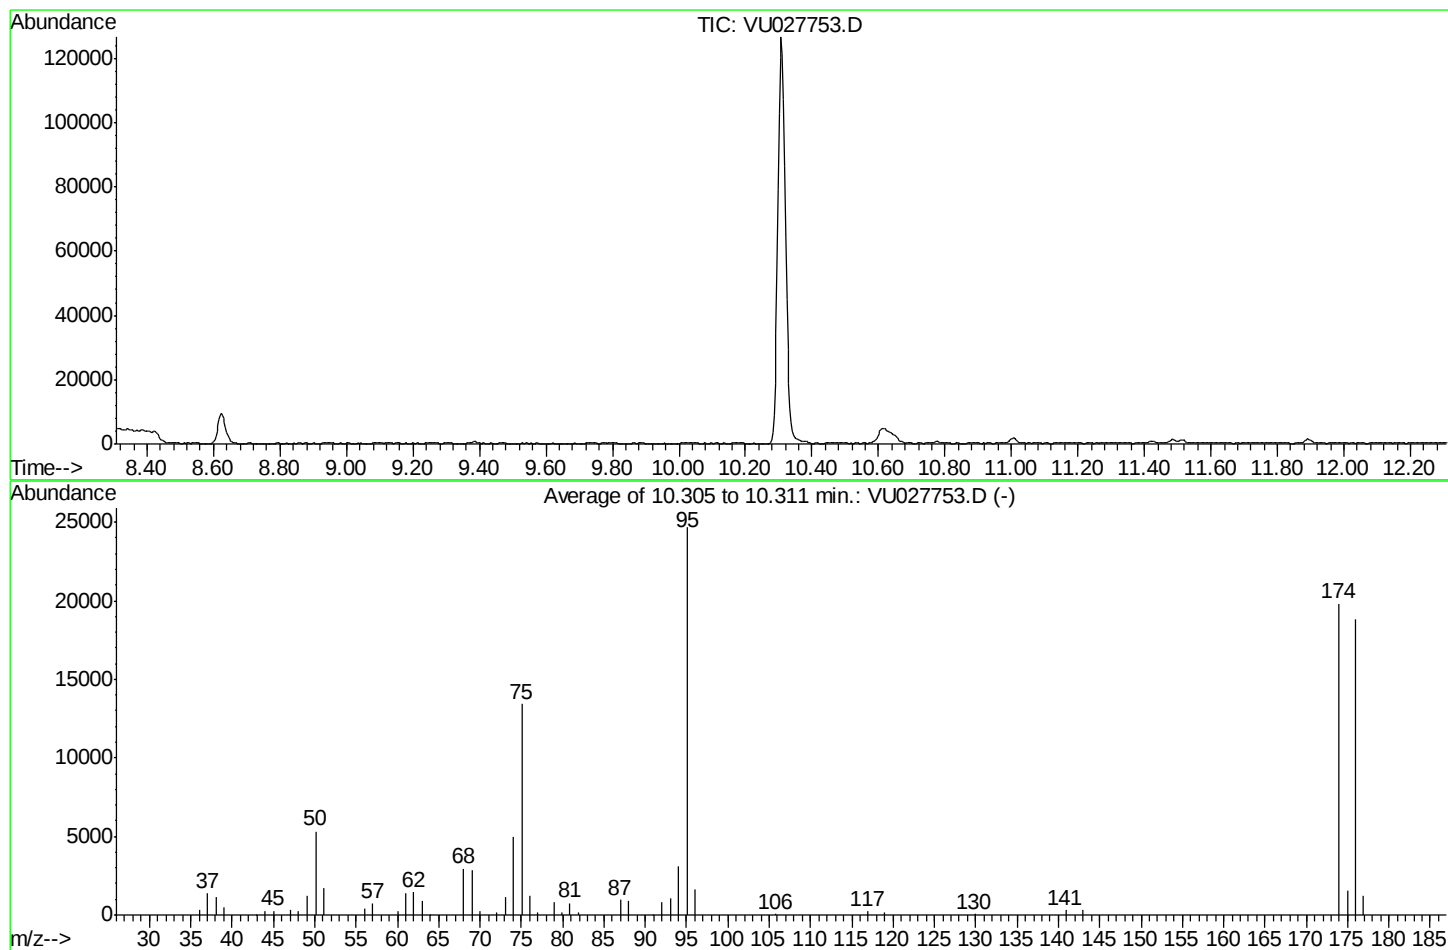

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	5315	PASS
75	95	30	60	54.4	13415	PASS
95	95	100	100	100.0	24677	PASS
96	95	5	9	6.5	1609	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.3	19818	PASS
175	174	5	9	7.7	1533	PASS
176	174	95	101	95.1	18848	PASS
177	176	5	9	6.5	1226	PASS