

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102319\
 Data File : VU035446.D
 Acq On : 24 Oct 2019 08:51
 Operator : JC/SP
 Sample : K5509-09
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0G60

Quant Time: Oct 24 14:25:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 24 14:19:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	194934	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	200733	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.85	152	59267	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.62	65	48889	4.11	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.20%
7) Chloroethane-d5	1.93	69	53522	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.60%
11) 1,1-Dichloroethene-d2	2.60	63	72057	3.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.60%
20) 2-Butanone-d5	4.70	46	219351	64.22	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.44%
24) Chloroform-d	5.11	84	106894	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
26) 1,2-Dichloroethane-d4	5.75	65	72268	6.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	120.00%
32) Benzene-d6	5.77	84	218807	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
36) 1,2-Dichloropropane-d6	6.74	67	82643	5.67	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.40%
41) Toluene-d8	7.93	98	174927	3.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.60%
43) trans-1,3-Dichloropropene-	8.22	79	26570	3.76	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.20%
46) 2-Hexanone-d5	8.69	63	143802	46.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.20%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	50659	3.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.00%
64) 1,2-Dichlorobenzene-d4	12.22	152	54979	5.09	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.80%


Target Compounds					Ovalue
13) Acetone	2.67	43	17844	7.510 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102319\
Data File : VU035446.D
Acq On : 24 Oct 2019 08:51
Operator : JC/SP
Sample : K5509-09
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0G60

Quant Time: Oct 24 14:25:30 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 24 14:19:48 2019
Response via : Initial Calibration

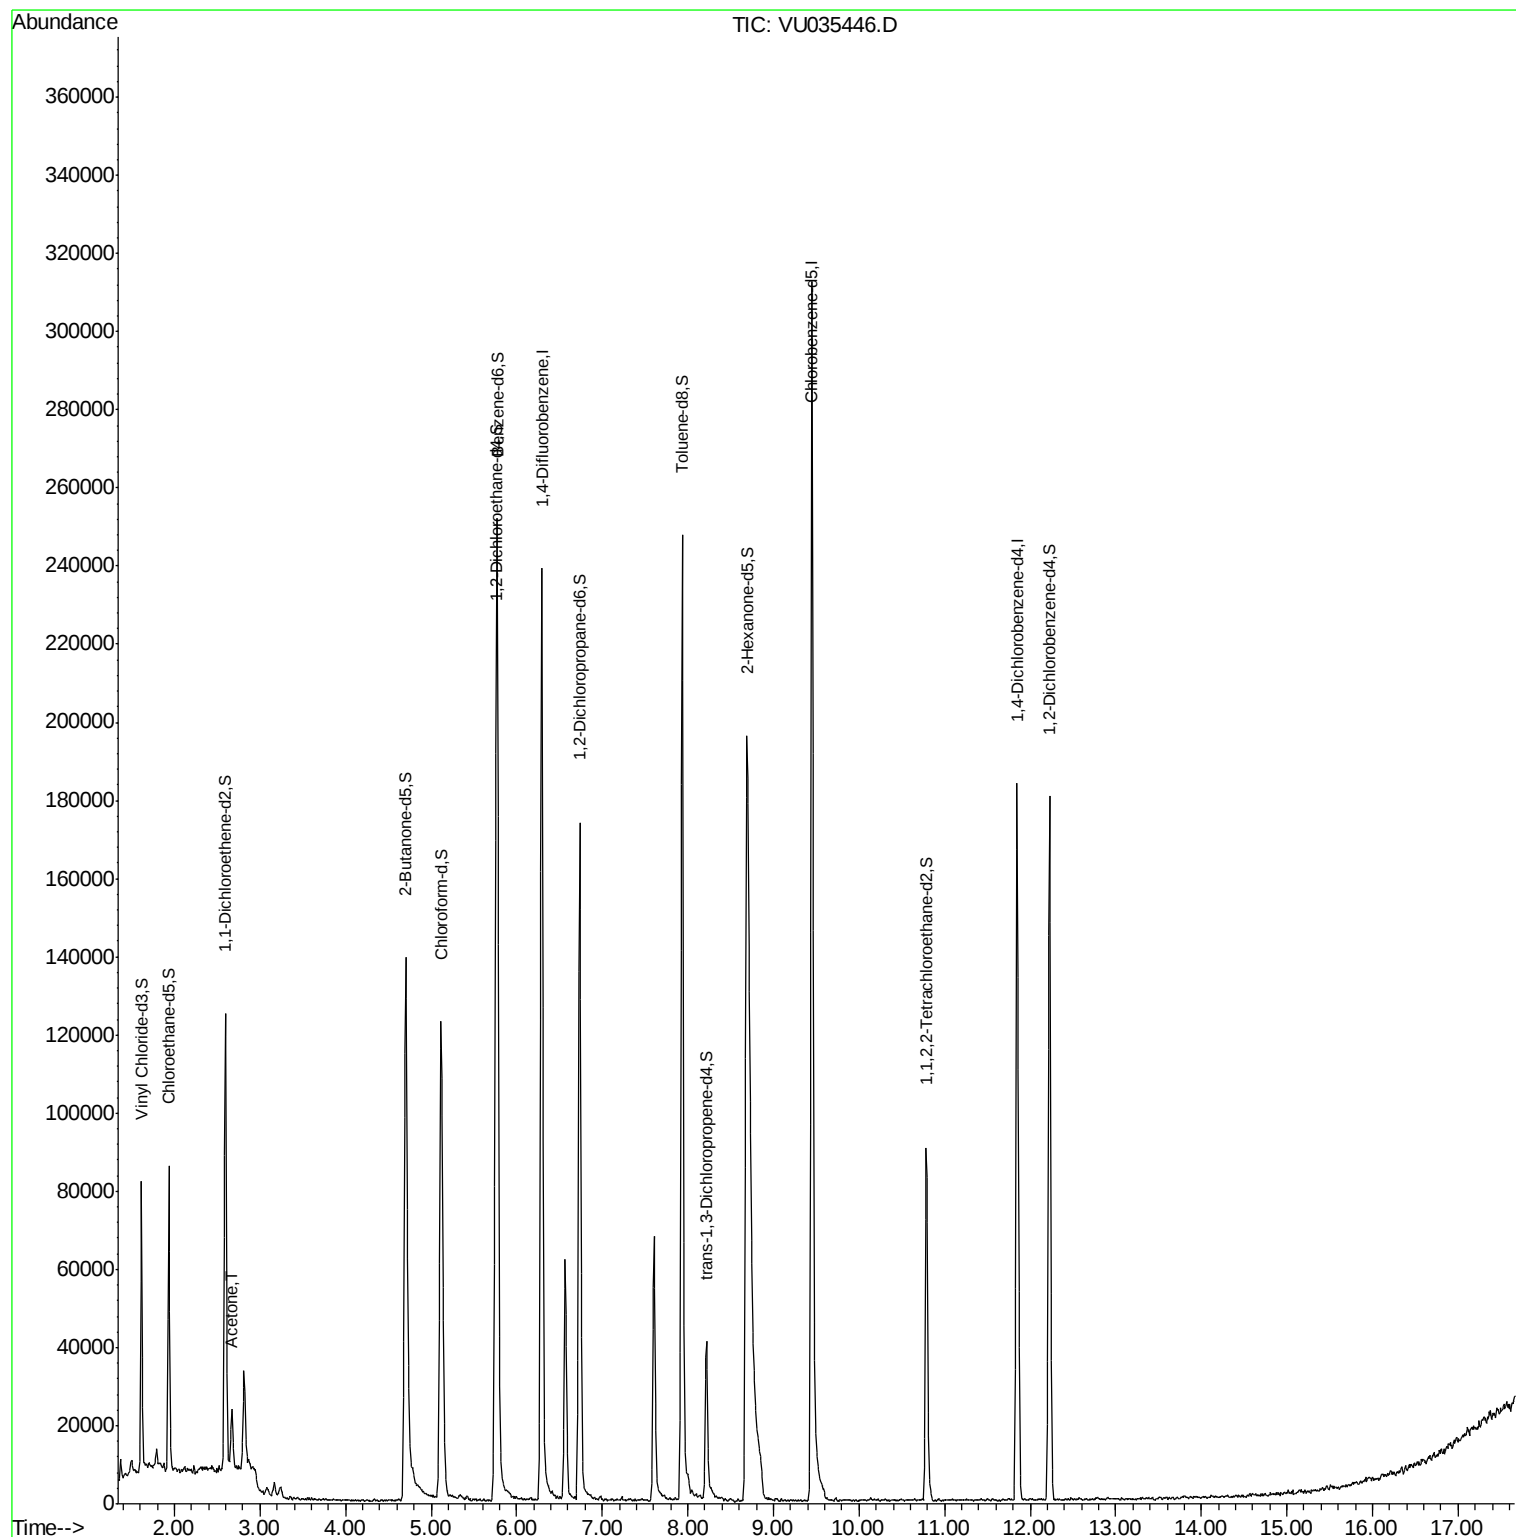

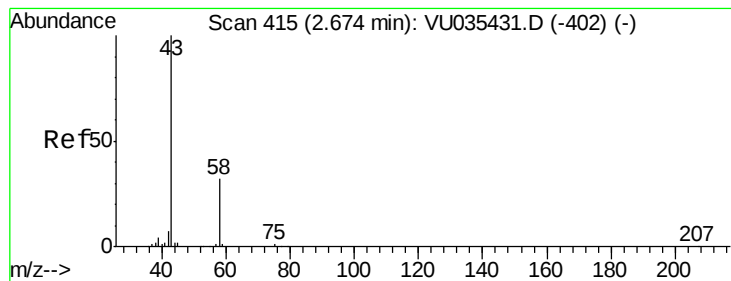

#13
 Acetone
 Concen: 7.510 ug/L
 RT: 2.67 min Scan# 414
 Delta R.T. -0.00 min
 Lab File: VU035446.D
 Acq: 24 Oct 2019 08:51

Instrument :
 MSVOA_U
 ClientSampleId :
 H0G60

Tot Ion: 43 Resp: 17844
 Ion Ratio Lower Upper
 43 100
 58 32.6 0.0 61.8

