


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102319\
Data File : VU035398.D
Acq On : 23 Oct 2019 08:27
Operator : JC/SP
Sample : BFB25
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB25

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR101719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Oct 25 17:02:56 2019

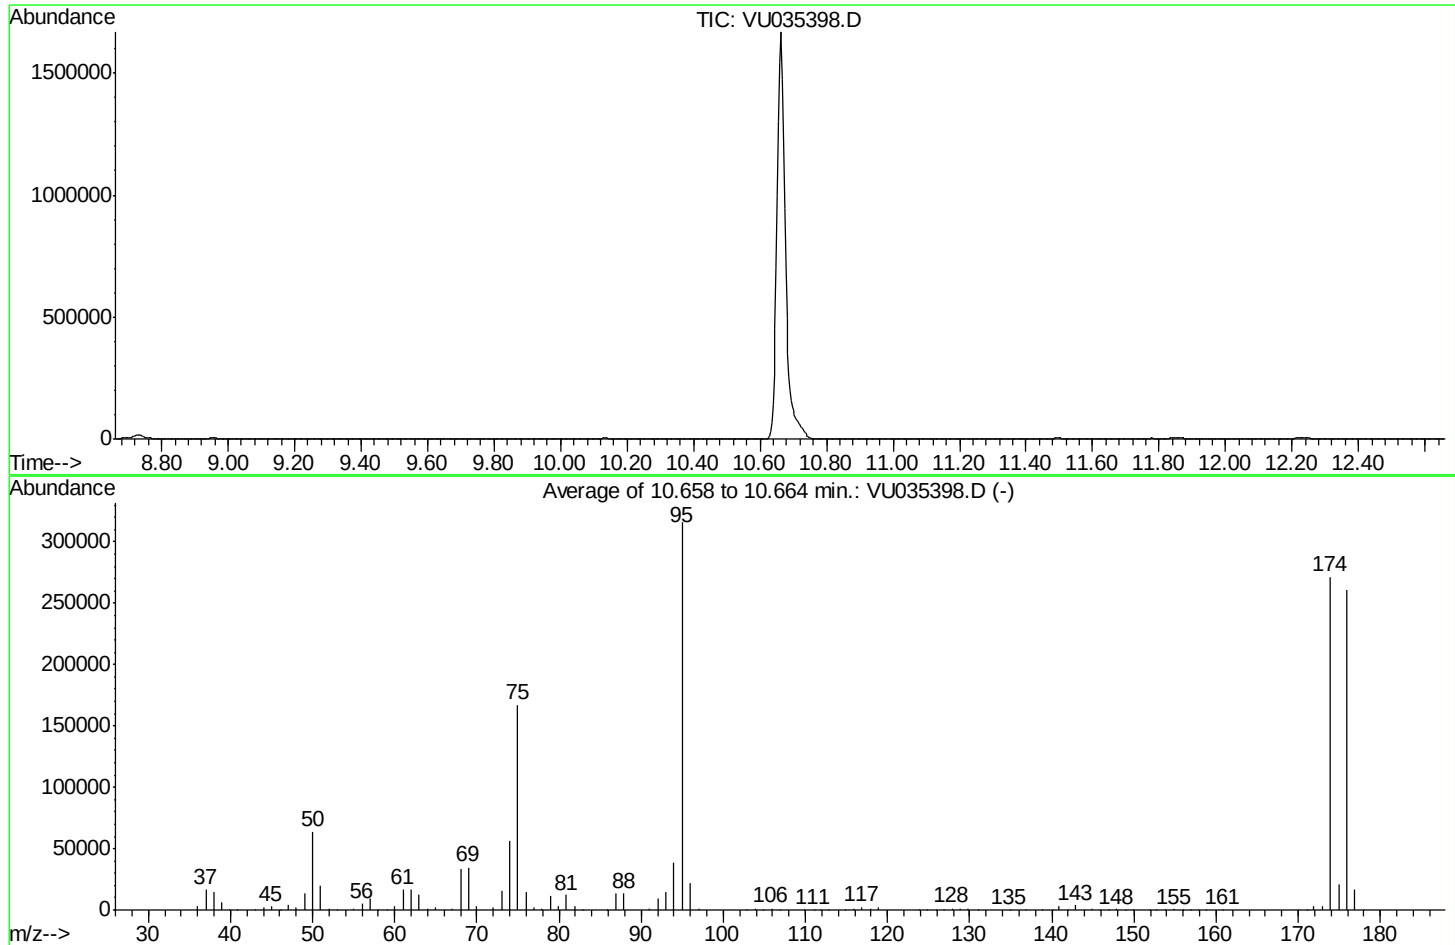

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	63736	PASS
75	95	30	80	52.9	167274	PASS
95	95	100	100	100.0	315968	PASS
96	95	5	9	6.9	21917	PASS
173	174	0.00	2	1.2	3201	PASS
174	95	50	120	85.9	271338	PASS
175	174	5	9	7.6	20517	PASS
176	174	95	101	96.0	260544	PASS
177	176	5	9	6.5	17026	PASS

m/z	Abundance
36.00	3057.0
37.00	15621.0
38.00	13977.0
39.00	5900.0
40.00	494.0
40.80	106.0
43.00	240.0
44.00	2262.0
45.00	2642.0
46.10	504.0
47.00	3732.0
48.00	2202.0
49.00	13343.0
50.00	62064.0
51.00	18896.0
52.10	985.0
53.00	189.0
55.00	981.0
56.00	4865.0
57.00	8696.0
58.00	293.0
60.00	3157.0
61.00	15880.0
62.00	15552.0
63.00	12842.0
64.00	1710.0
65.00	1975.0
66.10	202.0
67.00	934.0
68.00	33064.0
69.00	33616.0
70.00	2634.0
72.00	1795.0
73.00	15686.0
74.00	54784.0
75.00	160832.0
76.00	14188.0
76.90	1930.0
78.00	1253.0
78.90	10949.0
79.90	3213.0
80.90	11692.0
81.90	3105.0
82.80	265.0
85.90	525.0
86.90	13200.0
87.90	12910.0
91.00	1284.0
92.00	9642.0
93.00	13927.0
94.00	37392.0
95.00	302592.0
96.00	21496.0
97.00	761.0
102.90	145.0
103.90	1278.0
104.80	458.0
105.90	1502.0
106.80	367.0
109.80	310.0
111.00	320.0
111.90	210.0
112.80	239.0
114.80	336.0
115.90	1057.0
116.90	2284.0
117.90	1386.0
118.90	1780.0
123.80	204.0
125.80	100.0
126.70	108.0
127.80	1011.0
128.90	559.0
129.90	1126.0
130.90	381.0
134.80	512.0
136.80	520.0
140.00	195.0
140.90	3256.0
141.90	385.0
142.90	3612.0
143.90	240.0
144.90	905.0
145.80	470.0
146.90	243.0
147.90	667.0
149.00	211.0
149.80	240.0
151.80	188.0
152.70	133.0
153.70	177.0
154.90	918.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

155.90	181.0
156.90	450.0
157.90	181.0
158.80	279.0
160.80	435.0
169.90	164.0
171.00	298.0
171.90	2684.0
173.00	2913.0
173.90	254016.0
174.90	19384.0
175.90	243776.0
176.90	16184.0
177.90	424.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.00	3237.0
37.00	16816.0
38.00	14725.0
39.00	6249.0
40.00	453.0
40.80	119.0
43.00	183.0
44.00	2526.0
45.00	2895.0
46.10	489.0
47.00	3893.0
48.00	2298.0
49.00	14064.0
50.00	65840.0
51.00	20272.0
52.00	1089.0
52.90	217.0
55.00	988.0
56.00	4872.0
57.00	9531.0
58.00	343.0
60.00	3468.0
61.00	16832.0
62.00	16960.0
63.00	13384.0
64.00	1634.0
65.00	1797.0
66.10	211.0
67.00	999.0
68.00	34968.0
69.00	36088.0
70.00	3055.0
72.00	1951.0
73.00	16688.0
74.00	58008.0
75.00	173184.0
76.00	14986.0
76.90	2026.0
78.00	1222.0
78.90	11707.0
79.90	3451.0
80.90	12471.0
81.90	3234.0
82.80	258.0
85.90	451.0
86.90	13561.0
87.90	13715.0
90.90	1416.0
92.00	9993.0
93.00	14776.0
94.00	39464.0
95.00	325760.0
96.00	22696.0
97.00	834.0
102.90	157.0
103.90	1434.0
104.80	519.0
105.90	1551.0
106.80	361.0
109.80	310.0
111.00	321.0
111.80	211.0
112.80	236.0
114.90	357.0
115.90	1207.0
116.90	2447.0
117.90	1483.0
118.90	1851.0
123.90	233.0
124.80	120.0
125.80	174.0
126.80	107.0
127.80	1116.0
128.90	659.0
129.80	1119.0
130.90	401.0
134.80	546.0
136.80	539.0
140.00	240.0
140.90	3484.0
141.90	385.0
142.90	3922.0
143.90	270.0
144.90	933.0
145.90	465.0
146.80	252.0
147.90	724.0
149.00	178.0
149.80	270.0
151.80	210.0
152.70	150.0
153.70	234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

154.90	960.0
155.90	159.0
156.90	462.0
157.90	219.0
158.80	349.0
160.80	554.0
170.00	175.0
171.10	293.0
171.90	2913.0
173.00	3306.0
173.90	280128.0
174.90	21296.0
175.90	268736.0
176.90	17624.0
177.90	470.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.00	3135.0
37.00	16432.0
38.00	14249.0
39.00	5869.0
40.00	386.0
43.00	154.0
44.00	2539.0
45.00	2911.0
46.10	362.0
47.00	3956.0
48.00	2122.0
49.00	13807.0
50.00	63304.0
51.00	19792.0
52.00	1068.0
52.90	198.0
55.00	908.0
56.00	4633.0
57.00	9486.0
58.00	335.0
59.00	131.0
60.00	3444.0
61.00	16552.0
62.00	16464.0
63.00	13000.0
64.00	1371.0
65.00	1580.0
65.90	191.0
67.00	984.0
68.00	33248.0
69.00	35240.0
70.00	3239.0
72.00	1955.0
73.00	15618.0
74.00	56896.0
75.00	167808.0
76.00	14453.0
76.90	1851.0
77.80	1024.0
78.90	11564.0
79.90	3452.0
80.90	12320.0
81.90	3006.0
82.80	228.0
85.90	369.0
87.00	13202.0
87.90	13637.0
90.90	1440.0
92.00	9872.0
93.00	14333.0
94.00	37976.0
95.00	319552.0
96.00	21560.0
97.00	726.0
102.80	162.0
103.90	1496.0
104.90	514.0
105.90	1406.0
106.80	309.0
109.80	268.0
111.00	284.0
111.80	257.0
112.90	226.0
114.80	402.0
115.80	1217.0
116.90	2324.0
117.90	1443.0
118.90	1764.0
123.90	186.0
124.80	115.0
125.80	194.0
126.80	118.0
127.90	1151.0
128.90	627.0
129.80	994.0
131.00	383.0
134.90	553.0
136.80	543.0
138.80	110.0
140.10	225.0
140.90	3396.0
141.90	401.0
142.90	3984.0
143.90	269.0
144.90	723.0
145.90	434.0
146.80	216.0
147.90	805.0
149.00	174.0
149.90	288.0
151.90	194.0
152.80	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

153.80	296.0
154.90	908.0
156.00	123.0
157.00	471.0
157.80	240.0
158.80	376.0
160.80	541.0
170.00	168.0
171.90	2911.0
173.00	3385.0
173.90	279872.0
174.90	20872.0
175.90	269120.0
176.90	17272.0
177.90	439.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

Scan 2883 (10.610 min): VU035398.D
BFB25

m/z	Abundance
39.80	246.0
44.00	636.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25