

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU102320\
 Data File : VU040927.D
 Acq On : 23 Oct 2020 10:28
 Operator : SY/MD
 Sample : VU1023WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1023WBL01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.292	293	296	300	RBV5	2213	1708	1.09%	0.358%
2	3.063	527	536	540	RBV8	4210	6281	4.01%	1.317%
3	3.269	596	600	605	RBV6	1500	1725	1.10%	0.362%
4	3.642	713	716	721	RBV6	1772	1641	1.05%	0.344%
5	4.243	901	903	909	RVB6	2002	1800	1.15%	0.377%
6	4.417	954	957	961	RBV4	2400	1800	1.15%	0.377%
7	5.301	1226	1232	1236	RBV7	3384	4844	3.09%	1.015%
8	5.706	1350	1358	1359	RBV4	1875	1820	1.16%	0.382%
9	6.124	1473	1488	1504	RBV	81275	156557	100.00%	32.820%
10	7.809	2007	2012	2021	RVB7	3754	5352	3.42%	1.122%
11	7.902	2035	2041	2048	RBV2	1728	2082	1.33%	0.436%
12	8.700	2284	2289	2297	RVB5	2722	3760	2.40%	0.788%
13	8.935	2353	2362	2374	RBV5	8306	16068	10.26%	3.368%
14	9.449	2517	2522	2530	RVB4	1309	1599	1.02%	0.335%
15	10.111	2722	2728	2735	RVB5	1370	1933	1.23%	0.405%
16	10.632	2877	2890	2904	RBV	54126	88025	56.23%	18.453%
17	10.780	2932	2936	2943	RVB5	1734	1942	1.24%	0.407%
18	10.896	2967	2972	2980	RBV5	1436	2067	1.32%	0.433%
19	11.092	3027	3033	3041	RVB5	1522	1769	1.13%	0.371%
20	11.410	3128	3132	3142	RVB5	1329	1998	1.28%	0.419%
21	11.832	3257	3263	3270	RVB4	2257	3066	1.96%	0.643%
22	12.188	3362	3374	3391	RBV2	75636	131531	84.01%	27.573%
23	13.198	3678	3688	3689	RBV3	1565	1772	1.13%	0.371%
24	13.262	3703	3708	3714	RBV4	1933	1873	1.20%	0.393%
25	13.835	3875	3886	3891	RBV5	6343	8236	5.26%	1.727%
26	14.012	3932	3941	3946	RBV6	3059	4049	2.59%	0.849%
27	14.082	3951	3963	3974	RBV5	7172	12260	7.83%	2.570%
28	14.323	4030	4038	4047	RVB5	6107	9464	6.05%	1.984%


Sum of corrected areas: 477022

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU102320\
Data File : VU040927.D
Acq On : 23 Oct 2020 10:28
Operator : SY/MD
Sample : VU1023WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1023WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA U\METHOD\524U102220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

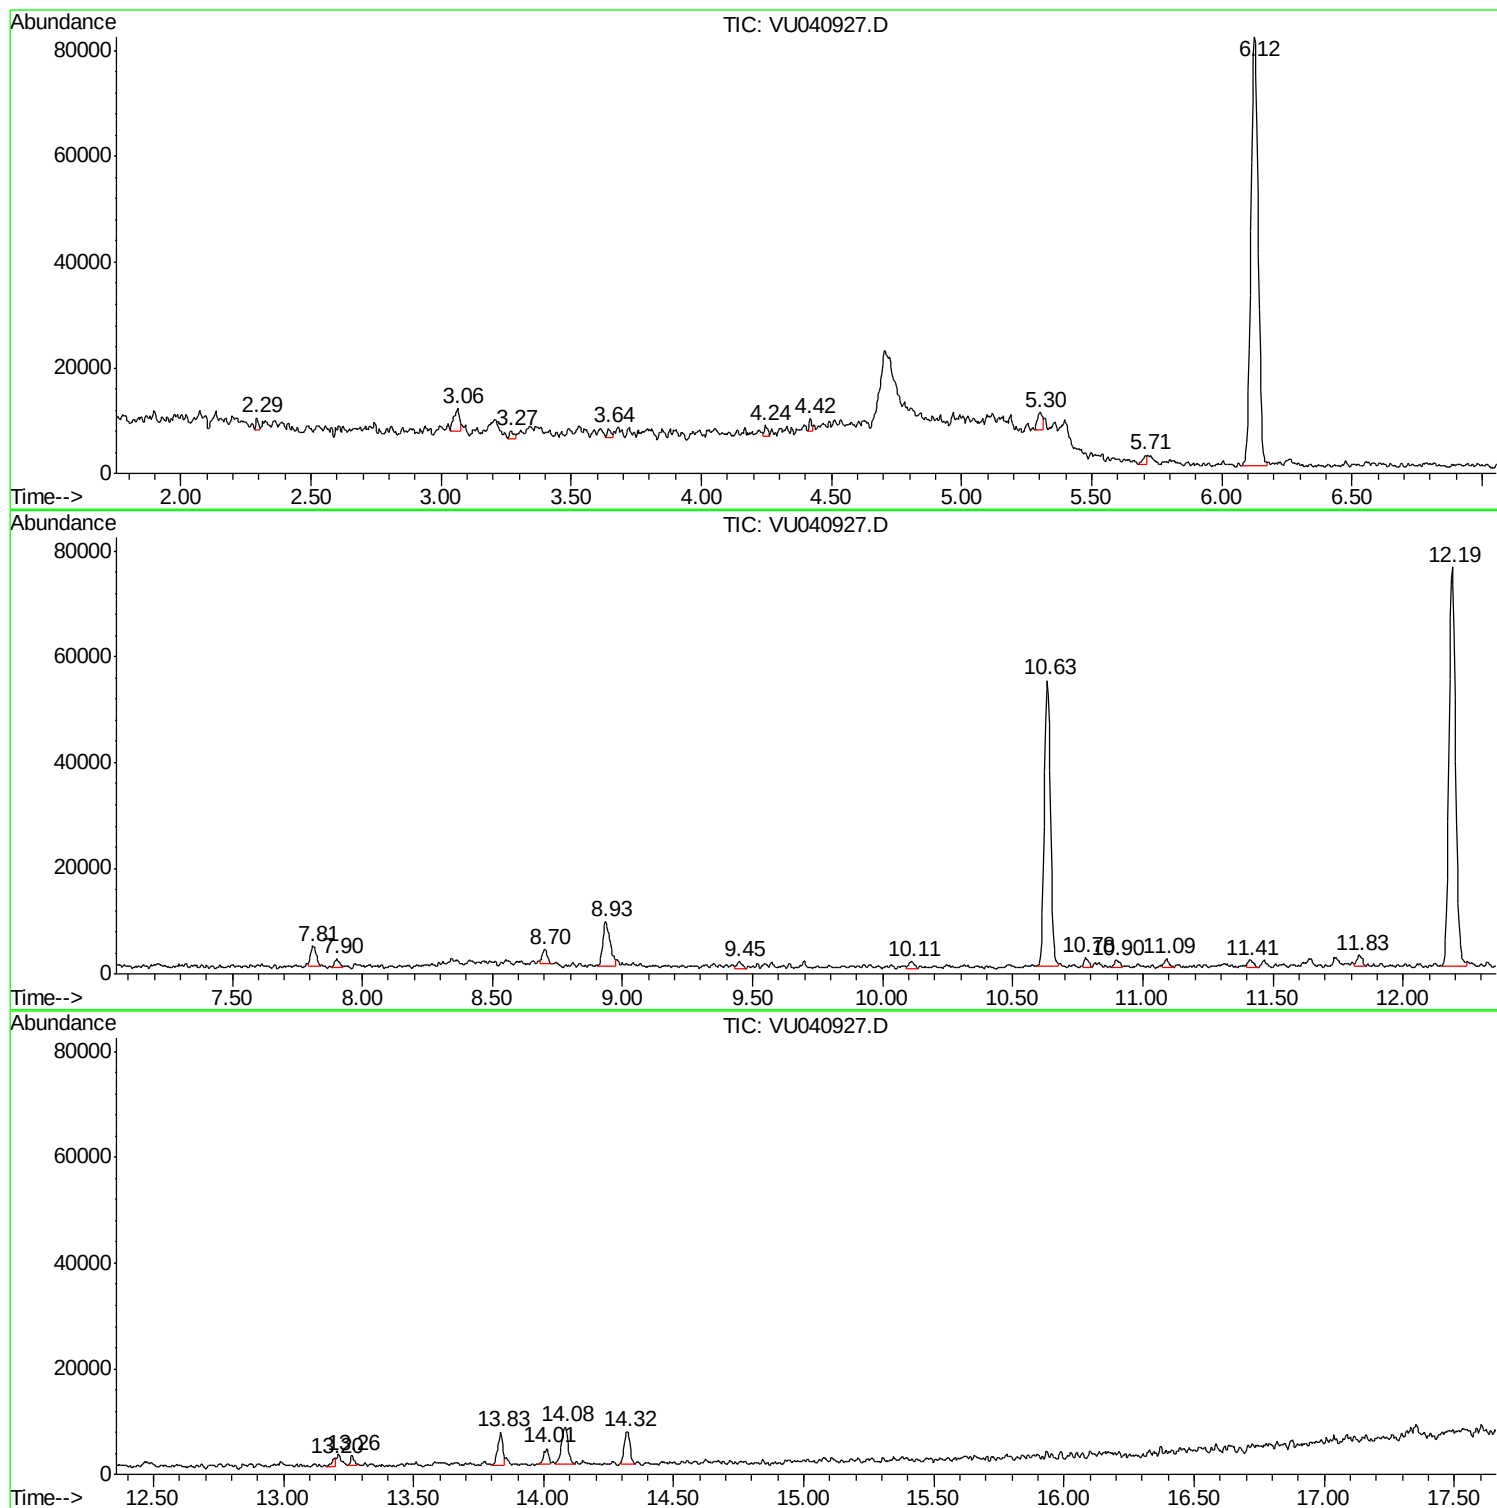

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU102320\
Data File : VU040927.D
Acq On : 23 Oct 2020 10:28
Operator : SY/MD
Sample : VU1023WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1023WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU102320\
Data File : VU040927.D
Acq On : 23 Oct 2020 10:28
Operator : SY/MD
Sample : VU1023WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1023WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U102220DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc