


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU102320\  
 Data File : VU040925.D  
 Acq On : 23 Oct 2020 09:08  
 Operator : SY/MD  
 Sample : BFB  
 Misc : 25.0mL/MSVOA U/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\524U102220DW.M  
 Title : METHOD 524.2 VOLATILES DRINKING WATER  
 Last Update : Fri Oct 23 07:07:33 2020

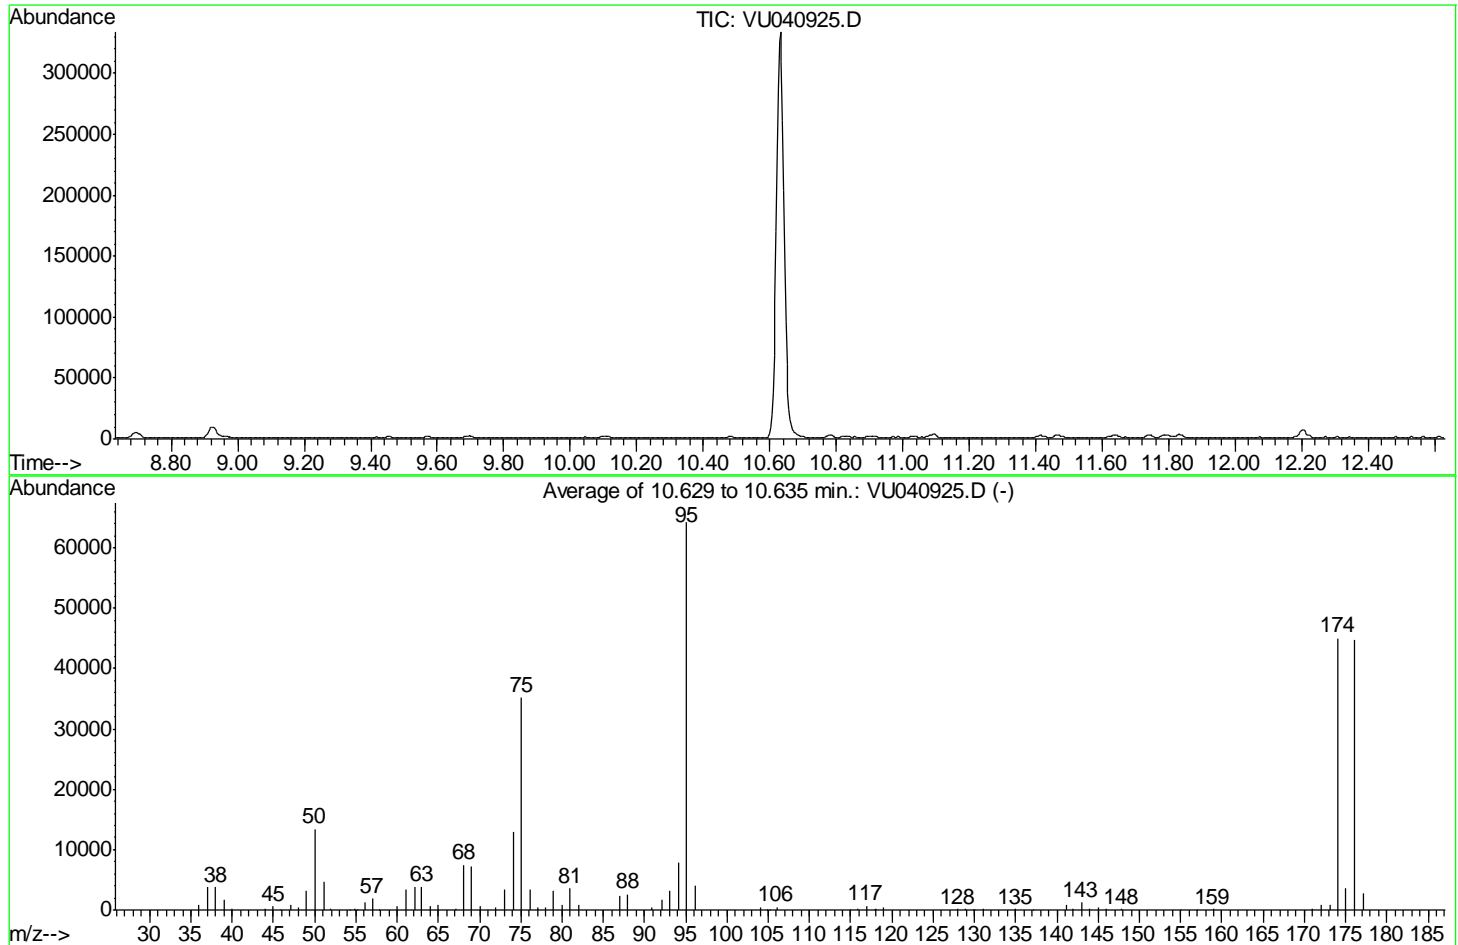

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	13456	PASS
75	95	30	60	54.7	35162	PASS
95	95	100	100	100.0	64224	PASS
96	95	5	9	6.2	3984	PASS
173	174	0.00	2	2.0	889	PASS
174	95	50	100	70.1	45053	PASS
175	174	5	9	8.0	3626	PASS
176	174	95	101	99.4	44770	PASS
177	176	5	9	6.1	2745	PASS