

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055850.D
 Acq On : 23 Oct 2023 13:03
 Operator : MD/SY
 Sample : VU1023WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK114

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	112	rBV	207856	246873	12.02%	1.587%
2	1.891	179	187	205	rVB	179235	262368	12.77%	1.686%
3	2.213	284	287	293	rBV6	1769	2010	0.10%	0.013%
4	2.560	382	395	413	rBV	390402	639371	31.12%	4.109%
5	2.756	453	456	458	rBV2	733	370	0.02%	0.002%
6	2.997	526	531	533	rVV2	609	519	0.03%	0.003%
7	3.036	535	543	556	rVB2	7244	13263	0.65%	0.085%
8	3.178	572	587	607	rBV2	21343	53520	2.61%	0.344%
9	3.303	623	626	634	rBV2	442	473	0.02%	0.003%
10	3.338	634	637	639	rBV2	620	439	0.02%	0.003%
11	3.354	639	642	645	rVV2	736	674	0.03%	0.004%
12	3.448	666	671	673	rBV2	291	259	0.01%	0.002%
13	3.528	688	696	700	rBV2	352	501	0.02%	0.003%
14	3.570	704	709	713	rBV2	298	344	0.02%	0.002%
15	3.924	816	819	823	rVB3	459	320	0.02%	0.002%
16	4.052	854	859	865	rVB2	324	309	0.02%	0.002%
17	4.235	913	916	920	rBV	468	339	0.02%	0.002%
18	4.377	958	960	965	rVV2	398	293	0.01%	0.002%
19	4.412	965	971	976	rVB2	442	504	0.02%	0.003%
20	4.441	976	980	982	rBV	401	257	0.01%	0.002%
21	4.470	986	989	995	rVV2	283	296	0.01%	0.002%
22	4.615	1022	1034	1074	rBV	160441	449358	21.87%	2.888%
23	4.959	1139	1141	1145	rVB3	699	494	0.02%	0.003%
24	5.055	1155	1171	1195	rBV	374524	837064	40.74%	5.379%
25	5.419	1278	1284	1285	rBV	344	294	0.01%	0.002%
26	5.512	1311	1313	1321	rVB3	423	471	0.02%	0.003%
27	5.721	1356	1378	1398	rBV2	738739	2054509	100.00%	13.203%
28	5.927	1440	1442	1445	rVB3	626	364	0.02%	0.002%
29	5.956	1449	1451	1454	rVV4	515	328	0.02%	0.002%
30	5.997	1462	1464	1467	rVB3	705	311	0.02%	0.002%
31	6.046	1476	1479	1485	rVB4	1109	989	0.05%	0.006%
32	6.078	1485	1489	1492	rBV3	307	310	0.02%	0.002%
33	6.245	1527	1541	1573	rBV	562308	1095135	53.30%	7.038%
34	6.528	1617	1629	1645	rBV3	25489	51413	2.50%	0.330%
35	6.589	1645	1648	1659	rVB5	1292	2104	0.10%	0.014%
36	6.634	1659	1662	1664	rBV3	462	335	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055850.D
 Acq On : 23 Oct 2023 13:03
 Operator : MD/SY
 Sample : VU1023WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK114

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.685	1664	1678	1709	rBV	466569	943456	45.92%	6.063%
38	7.087	1799	1803	1805	rBV2	367	315	0.02%	0.002%
39	7.190	1823	1835	1847	rBV2	8446	17671	0.86%	0.114%
40	7.325	1873	1877	1880	rVB2	532	417	0.02%	0.003%
41	7.393	1896	1898	1906	rVB2	367	282	0.01%	0.002%
42	7.435	1906	1911	1915	rBV2	330	317	0.02%	0.002%
43	7.563	1938	1951	1977	rBV	246853	452054	22.00%	2.905%
44	7.695	1985	1992	1995	rBV5	3647	4532	0.22%	0.029%
45	7.795	2017	2023	2026	rBV5	1090	1163	0.06%	0.007%
46	7.824	2029	2032	2040	rVB6	910	983	0.05%	0.006%
47	7.894	2040	2054	2077	rBV	909838	1598417	77.80%	10.272%
48	8.177	2129	2142	2165	rBV	170130	303366	14.77%	1.950%
49	8.306	2178	2182	2189	rVB4	654	736	0.04%	0.005%
50	8.377	2200	2204	2206	rBV	513	345	0.02%	0.002%
51	8.390	2206	2208	2211	rVB	549	295	0.01%	0.002%
52	8.473	2231	2234	2241	rVB3	539	544	0.03%	0.003%
53	8.550	2247	2258	2259	rBV3	2270	2517	0.12%	0.016%
54	8.586	2265	2269	2271	rBV	642	523	0.03%	0.003%
55	8.634	2271	2284	2323	rBV3	374494	964272	46.93%	6.197%
56	8.907	2366	2369	2370	rBV2	782	367	0.02%	0.002%
57	8.949	2380	2382	2388	rVB2	676	476	0.02%	0.003%
58	8.978	2388	2391	2396	rBV3	651	627	0.03%	0.004%
59	9.026	2404	2406	2409	rVB	697	361	0.02%	0.002%
60	9.055	2409	2415	2419	rBV2	427	417	0.02%	0.003%
61	9.091	2422	2426	2429	rBV3	591	478	0.02%	0.003%
62	9.123	2433	2436	2439	rVB2	465	331	0.02%	0.002%
63	9.171	2448	2451	2455	rVB3	744	490	0.02%	0.003%
64	9.238	2469	2472	2475	rVB2	496	354	0.02%	0.002%
65	9.328	2497	2500	2503	rBV2	408	297	0.01%	0.002%
66	9.415	2514	2527	2551	rBV	812465	1389381	67.63%	8.929%
67	9.544	2565	2567	2570	rBV4	475	277	0.01%	0.002%
68	9.653	2598	2601	2604	rVB2	547	372	0.02%	0.002%
69	9.689	2608	2612	2614	rBV2	1347	1068	0.05%	0.007%
70	10.033	2715	2719	2722	rBV2	401	270	0.01%	0.002%
71	10.090	2734	2737	2738	rBV2	611	316	0.02%	0.002%
72	10.299	2797	2802	2804	rBV	389	310	0.02%	0.002%
73	10.383	2821	2828	2829	rBV2	350	338	0.02%	0.002%
74	10.492	2858	2862	2867	rVB2	1353	1131	0.06%	0.007%
75	10.753	2930	2943	2967	rBV	709284	1175061	57.19%	7.551%
76	11.045	3031	3034	3036	rBV	445	326	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055850.D
 Acq On : 23 Oct 2023 13:03
 Operator : MD/SY
 Sample : VU1023WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK114

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.470	3161	3166	3178	rVB4	1450	2202	0.11%	0.014%
78	11.563	3193	3195	3201	rVB2	508	456	0.02%	0.003%
79	11.602	3201	3207	3211	rBV2	627	611	0.03%	0.004%
80	11.624	3211	3214	3217	rBV	402	342	0.02%	0.002%
81	11.756	3245	3255	3259	rBV3	1634	2464	0.12%	0.016%
82	11.811	3259	3272	3296	rBV	850263	1386247	67.47%	8.909%
83	12.045	3340	3345	3347	rBV3	797	757	0.04%	0.005%
84	12.103	3361	3363	3366	rVB2	527	259	0.01%	0.002%
85	12.135	3369	3373	3374	rBV	580	339	0.02%	0.002%
86	12.190	3377	3390	3416	rBV	927346	1553492	75.61%	9.983%
87	12.438	3463	3467	3472	rBV4	645	586	0.03%	0.004%
88	12.772	3569	3571	3574	rBV3	600	417	0.02%	0.003%
89	12.801	3578	3580	3583	rVB2	765	445	0.02%	0.003%
90	12.878	3601	3604	3606	rBV2	623	469	0.02%	0.003%
91	13.042	3651	3655	3661	rBV3	914	1003	0.05%	0.006%
92	13.081	3661	3667	3669	rBV3	621	619	0.03%	0.004%
93	13.129	3678	3682	3683	rBV2	445	315	0.02%	0.002%
94	13.235	3710	3715	3718	rBV4	1698	1757	0.09%	0.011%
95	13.315	3735	3740	3743	rBV3	846	790	0.04%	0.005%
96	13.730	3867	3869	3873	rBV2	484	259	0.01%	0.002%
97	13.856	3900	3908	3919	rBV4	3748	6802	0.33%	0.044%
98	14.110	3979	3987	3997	rBV5	4765	10067	0.49%	0.065%
99	14.335	4051	4057	4066	rBV6	4406	6316	0.31%	0.041%
100	14.573	4125	4131	4138	rVB5	1165	1693	0.08%	0.011%




Sum of corrected areas: 15560741

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055850.D
Acq On : 23 Oct 2023 13:03
Operator : MD/SY
Sample : VU1023WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

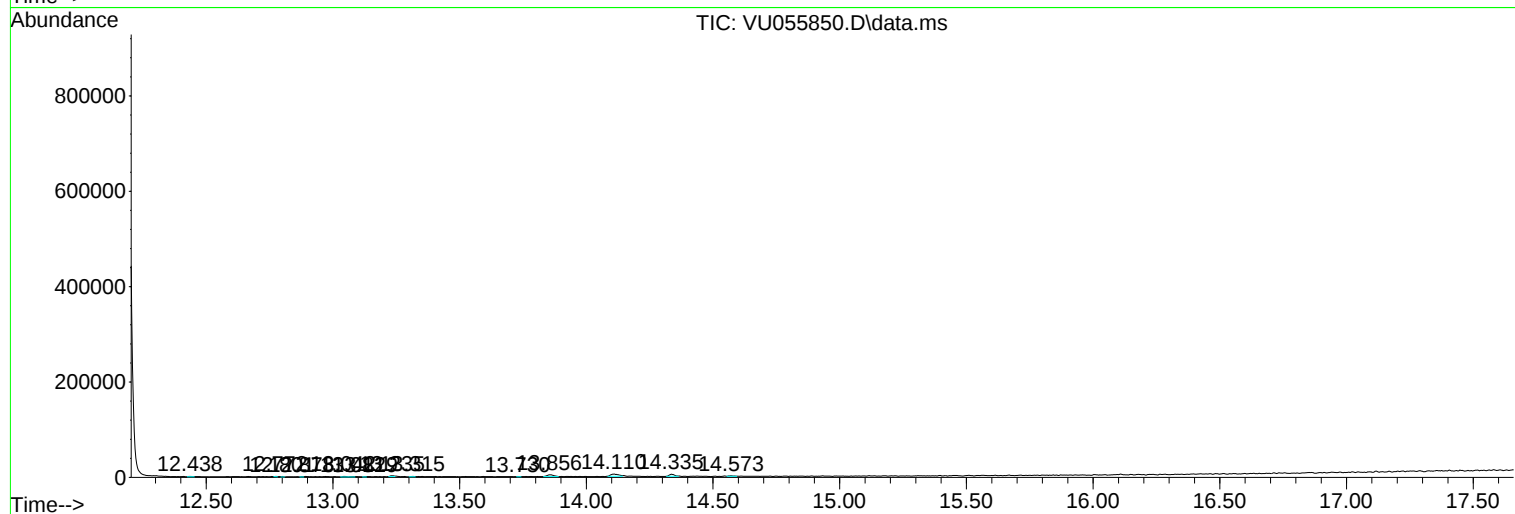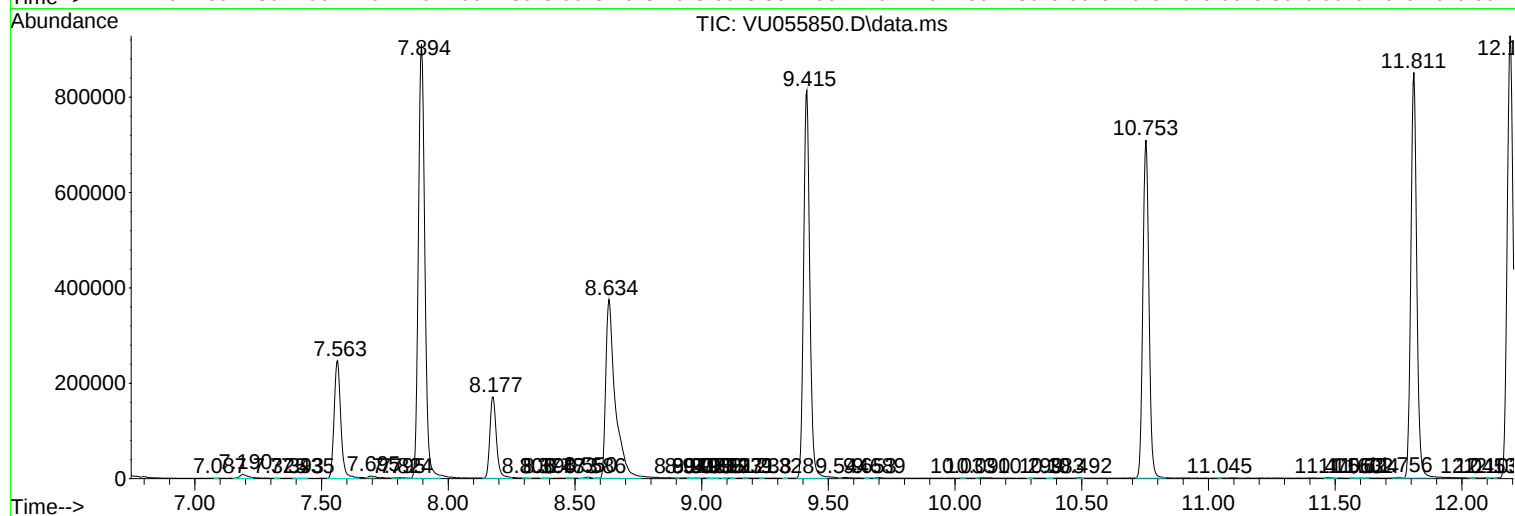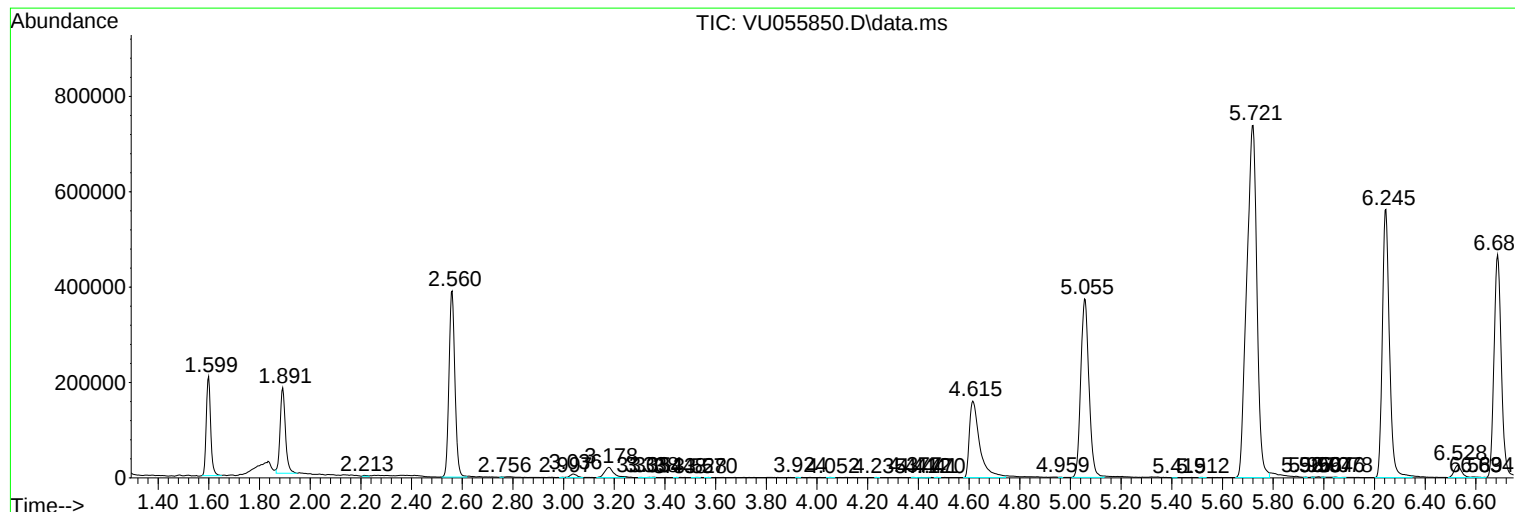

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055850.D
Acq On : 23 Oct 2023 13:03
Operator : MD/SY
Sample : VU1023WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055850.D
Acq On : 23 Oct 2023 13:03
Operator : MD/SY
Sample : VU1023WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK114

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------