

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055851.D
 Acq On : 23 Oct 2023 13:27
 Operator : MD/SY
 Sample : 04947-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	111	rBV	218117	261386	12.81%	1.682%
2	1.679	116	121	130	rVB	14022	16141	0.79%	0.104%
3	1.891	179	187	209	rVB	180135	261600	12.82%	1.684%
4	2.560	382	395	409	rBV	383235	625601	30.65%	4.026%
5	2.702	436	439	441	rBV	1062	700	0.03%	0.005%
6	2.740	449	451	455	rVB3	898	581	0.03%	0.004%
7	2.785	455	465	478	rVB2	4475	8655	0.42%	0.056%
8	2.907	497	503	505	rBV3	665	550	0.03%	0.004%
9	2.940	508	513	515	rBV3	354	353	0.02%	0.002%
10	2.956	516	518	522	rVB3	917	542	0.03%	0.003%
11	3.039	535	544	554	rVB3	3986	6504	0.32%	0.042%
12	3.174	582	586	588	rBV2	963	830	0.04%	0.005%
13	3.354	638	642	647	rVV3	933	981	0.05%	0.006%
14	3.432	661	666	668	rBV	366	323	0.02%	0.002%
15	3.448	668	671	676	rVB3	477	298	0.01%	0.002%
16	3.576	699	711	723	rBV3	10521	25138	1.23%	0.162%
17	3.991	832	840	843	rBV5	768	1153	0.06%	0.007%
18	4.139	883	886	891	rBV2	439	366	0.02%	0.002%
19	4.412	968	971	978	rBV2	381	383	0.02%	0.002%
20	4.615	1022	1034	1067	rBV	156942	445875	21.85%	2.869%
21	4.946	1135	1137	1141	rVB2	590	350	0.02%	0.002%
22	4.985	1147	1149	1154	rVB2	692	479	0.02%	0.003%
23	5.055	1154	1171	1196	rBV	373482	840775	41.20%	5.411%
24	5.341	1258	1260	1266	rVB4	1199	1000	0.05%	0.006%
25	5.464	1295	1298	1300	rBV	551	342	0.02%	0.002%
26	5.718	1357	1377	1403	rBV2	735084	2040781	100.00%	13.134%
27	5.968	1444	1455	1464	rBV8	6400	12883	0.63%	0.083%
28	6.136	1493	1507	1519	rBV5	7310	17442	0.85%	0.112%
29	6.245	1524	1541	1565	rBV	567918	1109258	54.35%	7.139%
30	6.528	1619	1629	1644	rVB5	15774	31876	1.56%	0.205%
31	6.595	1644	1650	1654	rBV6	1346	1586	0.08%	0.010%
32	6.685	1664	1678	1702	rBV	471252	931222	45.63%	5.993%
33	6.991	1769	1773	1776	rBV3	413	338	0.02%	0.002%
34	7.190	1823	1835	1849	rBV3	7762	17249	0.85%	0.111%
35	7.303	1866	1870	1872	rBV2	626	465	0.02%	0.003%
36	7.441	1910	1913	1919	rBV3	433	429	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055851.D
 Acq On : 23 Oct 2023 13:27
 Operator : MD/SY
 Sample : 04947-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.492	1924	1929	1931	rBV	410	322	0.02%	0.002%
38	7.560	1938	1950	1970	rBV	246467	447133	21.91%	2.878%
39	7.695	1985	1992	1995	rBV3	3770	4715	0.23%	0.030%
40	7.830	2031	2034	2037	rBV5	657	464	0.02%	0.003%
41	7.894	2040	2054	2071	rBV	887672	1566281	76.75%	10.080%
42	8.084	2110	2113	2115	rBV2	569	358	0.02%	0.002%
43	8.129	2125	2127	2130	rVB2	625	289	0.01%	0.002%
44	8.177	2130	2142	2166	rBV	169605	303302	14.86%	1.952%
45	8.341	2190	2193	2197	rVB3	609	469	0.02%	0.003%
46	8.370	2197	2202	2207	rBV5	715	1044	0.05%	0.007%
47	8.409	2211	2214	2218	rVB4	506	355	0.02%	0.002%
48	8.550	2250	2258	2267	rBV8	2582	3926	0.19%	0.025%
49	8.586	2267	2269	2273	rVB2	484	377	0.02%	0.002%
50	8.634	2273	2284	2320	rBV3	374669	954490	46.77%	6.143%
51	8.865	2354	2356	2359	rVB2	760	340	0.02%	0.002%
52	8.894	2363	2365	2368	rVB	781	340	0.02%	0.002%
53	8.914	2368	2371	2374	rVB5	656	454	0.02%	0.003%
54	8.994	2393	2396	2398	rVV2	474	289	0.01%	0.002%
55	9.074	2419	2421	2426	rVB4	535	400	0.02%	0.003%
56	9.142	2439	2442	2446	rBV3	429	356	0.02%	0.002%
57	9.193	2455	2458	2462	rVB2	414	333	0.02%	0.002%
58	9.235	2466	2471	2474	rVB2	361	340	0.02%	0.002%
59	9.354	2503	2508	2511	rBV2	403	360	0.02%	0.002%
60	9.415	2513	2527	2548	rBV	829201	1412720	69.22%	9.092%
61	9.602	2583	2585	2590	rVB5	752	471	0.02%	0.003%
62	9.701	2610	2616	2625	rVB5	2200	2514	0.12%	0.016%
63	9.759	2632	2634	2639	rVB2	664	418	0.02%	0.003%
64	9.788	2639	2643	2644	rBV	499	346	0.02%	0.002%
65	10.103	2738	2741	2743	rBV2	732	483	0.02%	0.003%
66	10.225	2775	2779	2784	rBV2	464	446	0.02%	0.003%
67	10.251	2784	2787	2792	rBV3	378	340	0.02%	0.002%
68	10.486	2854	2860	2863	rBV4	1251	1182	0.06%	0.008%
69	10.753	2929	2943	2963	rBV	739654	1209438	59.26%	7.783%
70	10.965	3006	3009	3013	rBV2	470	361	0.02%	0.002%
71	11.084	3041	3046	3049	rBV3	973	927	0.05%	0.006%
72	11.100	3049	3051	3052	rVV2	697	317	0.02%	0.002%
73	11.110	3052	3054	3057	rVB	712	393	0.02%	0.003%
74	11.145	3063	3065	3072	rVB3	536	445	0.02%	0.003%
75	11.180	3072	3076	3080	rBV2	439	410	0.02%	0.003%
76	11.238	3091	3094	3098	rBV2	392	299	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055851.D
 Acq On : 23 Oct 2023 13:27
 Operator : MD/SY
 Sample : 04947-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.258	3098	3100	3109	rVB	419	307	0.02%	0.002%
78	11.438	3153	3156	3160	rBV2	557	415	0.02%	0.003%
79	11.470	3161	3166	3173	rVV5	1486	1955	0.10%	0.013%
80	11.724	3240	3245	3246	rBV	329	299	0.01%	0.002%
81	11.743	3246	3251	3252	rBV5	1168	965	0.05%	0.006%
82	11.811	3259	3272	3295	rBV	852704	1400798	68.64%	9.015%
83	12.026	3337	3339	3341	rBV2	597	362	0.02%	0.002%
84	12.119	3366	3368	3372	rBV3	564	324	0.02%	0.002%
85	12.190	3376	3390	3423	rBV	909251	1528817	74.91%	9.839%
86	12.444	3467	3469	3473	rVB2	888	518	0.03%	0.003%
87	12.467	3473	3476	3477	rBV	858	509	0.02%	0.003%
88	12.637	3525	3529	3533	rBV2	644	790	0.04%	0.005%
89	12.730	3555	3558	3563	rBV2	410	441	0.02%	0.003%
90	12.762	3564	3568	3569	rBV2	808	493	0.02%	0.003%
91	12.946	3620	3625	3635	rBV6	3126	4676	0.23%	0.030%
92	13.164	3691	3693	3696	rBV	441	346	0.02%	0.002%
93	13.225	3709	3712	3715	rBV2	1488	1153	0.06%	0.007%
94	13.634	3836	3839	3840	rBV	541	325	0.02%	0.002%
95	13.856	3902	3908	3918	rVB10	2977	5075	0.25%	0.033%
96	13.965	3940	3942	3948	rBV	606	500	0.02%	0.003%
97	14.106	3982	3986	3987	rBV2	2032	1574	0.08%	0.010%
98	14.283	4038	4041	4044	rBV	573	363	0.02%	0.002%
99	14.309	4045	4049	4050	rVV2	691	532	0.03%	0.003%
100	14.341	4052	4059	4067	rVB4	2848	4464	0.22%	0.029%




Sum of corrected areas: 15538683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055851.D
Acq On : 23 Oct 2023 13:27
Operator : MD/SY
Sample : 04947-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

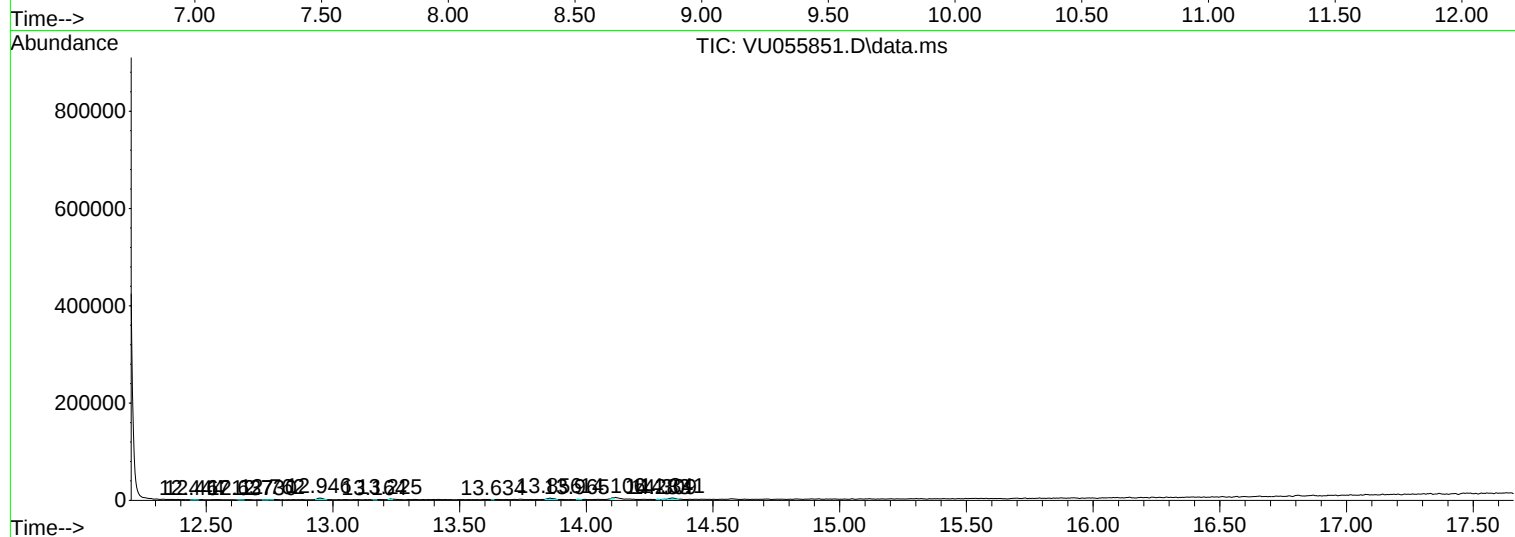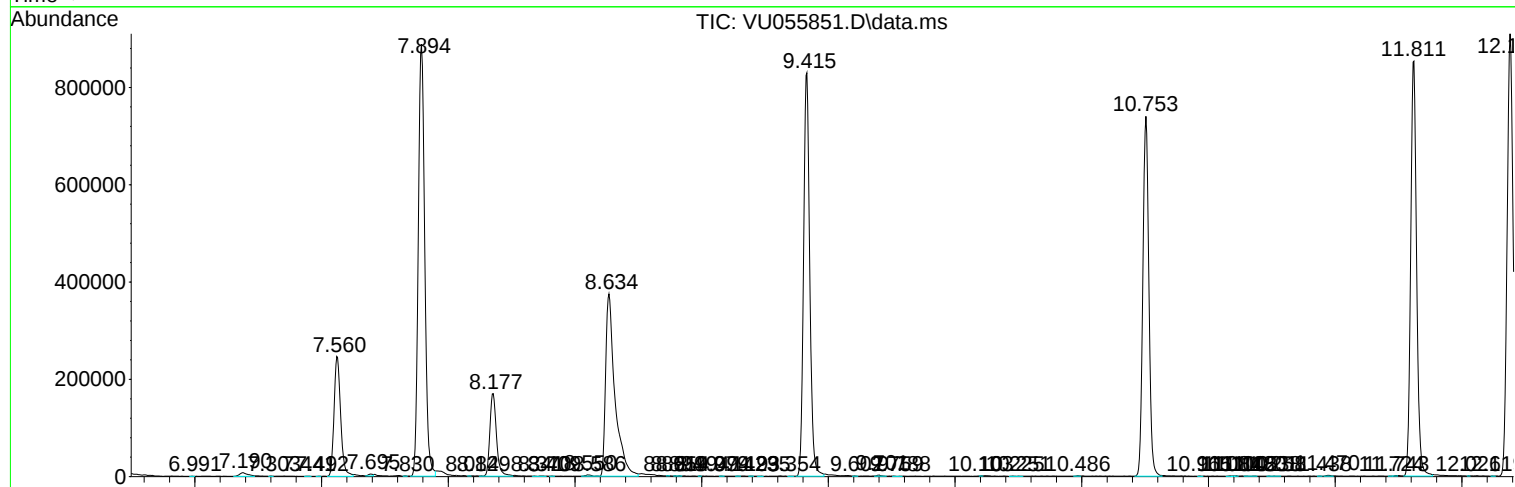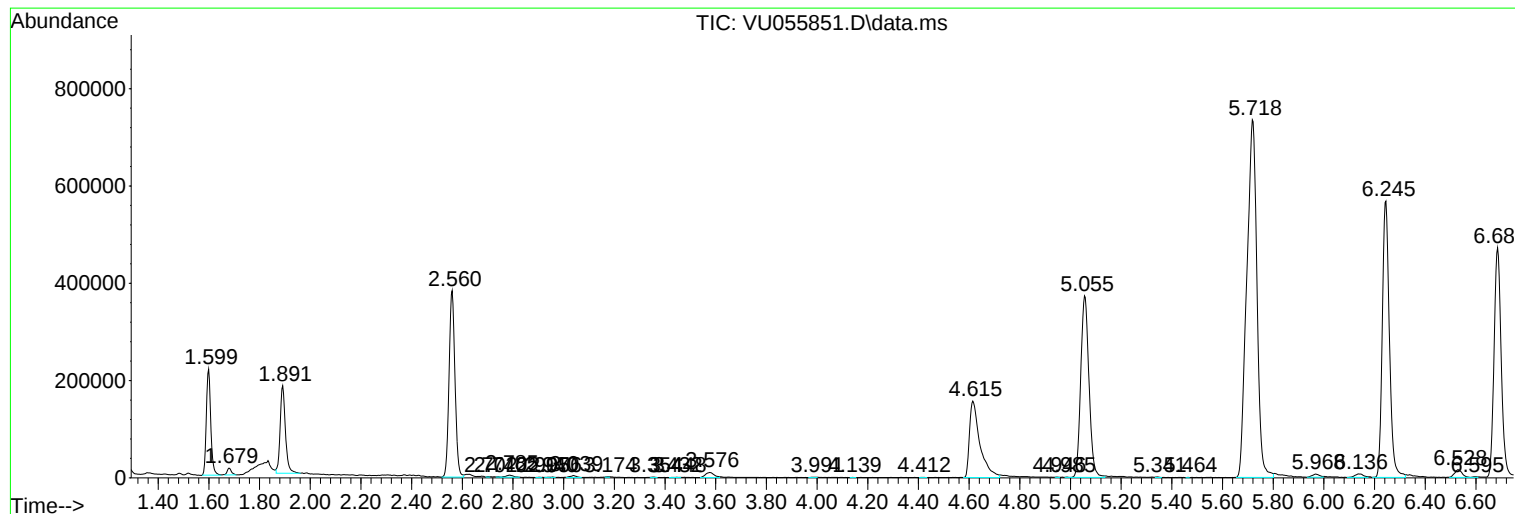

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055851.D
Acq On : 23 Oct 2023 13:27
Operator : MD/SY
Sample : 04947-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055851.D
Acq On : 23 Oct 2023 13:27
Operator : MD/SY
Sample : 04947-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------