

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055853.D
 Acq On : 23 Oct 2023 14:15
 Operator : MD/SY
 Sample : 04947-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	16	21	35	rVB3	12509	16205	0.78%	0.102%
2	1.486	56	61	66	rVB2	10395	10687	0.51%	0.067%
3	1.599	88	96	110	rVB	204313	246074	11.81%	1.548%
4	1.882	178	184	204	rVB	172605	255988	12.28%	1.611%
5	2.557	380	394	408	rBV	376931	613877	29.46%	3.862%
6	2.766	456	459	460	rBV2	771	527	0.03%	0.003%
7	2.817	473	475	479	rVB2	989	552	0.03%	0.003%
8	2.943	510	514	515	rBV	678	437	0.02%	0.003%
9	3.036	534	543	548	rBV6	4500	7811	0.37%	0.049%
10	3.123	566	570	573	rBV3	704	670	0.03%	0.004%
11	3.178	577	587	597	rBV6	3016	7107	0.34%	0.045%
12	3.296	619	624	626	rBV2	520	451	0.02%	0.003%
13	3.322	626	632	633	rBV3	777	678	0.03%	0.004%
14	3.341	634	638	639	rBV3	1577	1122	0.05%	0.007%
15	3.438	665	668	675	rVB2	587	459	0.02%	0.003%
16	3.505	683	689	693	rBV2	481	466	0.02%	0.003%
17	3.692	740	747	756	rVB4	1726	2675	0.13%	0.017%
18	4.393	960	965	972	rVB2	384	591	0.03%	0.004%
19	4.499	995	998	1000	rVV2	725	591	0.03%	0.004%
20	4.525	1000	1006	1014	rVB7	2022	3190	0.15%	0.020%
21	4.615	1023	1034	1061	rBV	154625	432978	20.78%	2.724%
22	4.952	1136	1139	1143	rVB2	630	446	0.02%	0.003%
23	5.055	1155	1171	1198	rBV	373966	837448	40.18%	5.269%
24	5.255	1229	1233	1236	rVB2	810	587	0.03%	0.004%
25	5.277	1237	1240	1244	rVB2	615	509	0.02%	0.003%
26	5.306	1246	1249	1251	rBV2	856	514	0.02%	0.003%
27	5.448	1289	1293	1298	rVB5	818	834	0.04%	0.005%
28	5.541	1318	1322	1325	rBV2	560	445	0.02%	0.003%
29	5.586	1332	1336	1342	rVB5	675	574	0.03%	0.004%
30	5.621	1344	1347	1354	rVB3	473	501	0.02%	0.003%
31	5.718	1356	1377	1420	rBV2	748722	2084040	100.00%	13.112%
32	5.972	1448	1456	1457	rBV4	2488	2427	0.12%	0.015%
33	6.033	1472	1475	1479	rBV4	970	879	0.04%	0.006%
34	6.129	1502	1505	1511	rVB4	985	696	0.03%	0.004%
35	6.158	1511	1514	1521	rVB4	731	828	0.04%	0.005%
36	6.242	1527	1540	1582	rBV	572958	1130532	54.25%	7.113%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055853.D
 Acq On : 23 Oct 2023 14:15
 Operator : MD/SY
 Sample : 04947-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.386	1583	1585	1588	rVB3	1034	494	0.02%	0.003%
38	6.531	1618	1630	1644	rBV6	22043	49265	2.36%	0.310%
39	6.685	1664	1678	1697	rBV	474564	938631	45.04%	5.906%
40	6.894	1738	1743	1745	rBV3	959	726	0.03%	0.005%
41	6.972	1761	1767	1772	rBV4	1015	1081	0.05%	0.007%
42	7.152	1815	1823	1824	rBV3	483	591	0.03%	0.004%
43	7.190	1824	1835	1848	rBV5	7514	16854	0.81%	0.106%
44	7.271	1856	1860	1863	rBV3	520	435	0.02%	0.003%
45	7.563	1937	1951	1971	rBV	248630	455559	21.86%	2.866%
46	7.782	2016	2019	2021	rBV2	756	451	0.02%	0.003%
47	7.894	2039	2054	2072	rBV	894567	1576427	75.64%	9.919%
48	8.177	2130	2142	2173	rBV	173747	311394	14.94%	1.959%
49	8.486	2235	2238	2242	rVB3	683	607	0.03%	0.004%
50	8.553	2250	2259	2267	rBV3	11018	18041	0.87%	0.114%
51	8.637	2272	2285	2325	rBV4	414160	1026608	49.26%	6.459%
52	8.933	2374	2377	2383	rVB6	1179	961	0.05%	0.006%
53	8.988	2391	2394	2397	rBV2	574	462	0.02%	0.003%
54	9.209	2460	2463	2470	rVB5	775	563	0.03%	0.004%
55	9.415	2514	2527	2554	rBV	852194	1461665	70.14%	9.197%
56	9.579	2570	2578	2583	rVB6	2053	3392	0.16%	0.021%
57	9.701	2607	2616	2627	rVB6	3991	7441	0.36%	0.047%
58	10.106	2737	2742	2743	rBV	943	652	0.03%	0.004%
59	10.367	2818	2823	2825	rBV3	521	499	0.02%	0.003%
60	10.489	2852	2861	2868	rBV4	2304	3264	0.16%	0.021%
61	10.547	2875	2879	2881	rBV3	911	649	0.03%	0.004%
62	10.608	2895	2898	2902	rBV3	1020	775	0.04%	0.005%
63	10.679	2914	2920	2923	rBV2	534	615	0.03%	0.004%
64	10.753	2930	2943	2973	rBV	744633	1237193	59.37%	7.784%
65	10.885	2980	2984	2986	rBV4	955	678	0.03%	0.004%
66	10.910	2987	2992	3002	rVB7	2689	3628	0.17%	0.023%
67	10.994	3014	3018	3020	rBV2	583	489	0.02%	0.003%
68	11.045	3028	3034	3036	rBV4	792	832	0.04%	0.005%
69	11.370	3130	3135	3138	rBV3	433	431	0.02%	0.003%
70	11.405	3140	3146	3147	rBV4	978	729	0.03%	0.005%
71	11.473	3160	3167	3178	rVB6	2173	3376	0.16%	0.021%
72	11.560	3185	3194	3197	rBV4	758	1038	0.05%	0.007%
73	11.611	3203	3210	3213	rBV5	1415	1487	0.07%	0.009%
74	11.750	3248	3253	3256	rVB5	1318	1074	0.05%	0.007%
75	11.811	3259	3272	3296	rBV	867714	1436079	68.91%	9.036%
76	12.004	3330	3332	3336	rVB4	1168	886	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055853.D
 Acq On : 23 Oct 2023 14:15
 Operator : MD/SY
 Sample : 04947-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	12.097	3351	3361	3369	rBV8	8571	14437	0.69%	0.091%
78	12.190	3377	3390	3414	rBV	932559	1561702	74.94%	9.826%
79	12.425	3458	3463	3466	rBV4	1353	1222	0.06%	0.008%
80	12.576	3502	3510	3517	rBV3	6732	10486	0.50%	0.066%
81	12.682	3530	3543	3549	rBV4	7037	11667	0.56%	0.073%
82	12.766	3564	3569	3573	rBV5	994	1312	0.06%	0.008%
83	12.865	3598	3600	3604	rVB3	951	609	0.03%	0.004%
84	12.978	3630	3635	3646	rVB5	5111	7538	0.36%	0.047%
85	13.106	3672	3675	3683	rVB6	1834	2267	0.11%	0.014%
86	13.222	3707	3711	3715	rBV5	1690	1825	0.09%	0.011%
87	13.293	3726	3733	3734	rBV5	5478	4749	0.23%	0.030%
88	13.367	3750	3756	3760	rBV7	1365	1413	0.07%	0.009%
89	13.412	3766	3770	3775	rVB5	981	946	0.05%	0.006%
90	13.457	3775	3784	3792	rBV4	8708	13807	0.66%	0.087%
91	13.605	3826	3830	3832	rVB	636	460	0.02%	0.003%
92	13.733	3867	3870	3879	rVB5	1357	1371	0.07%	0.009%
93	13.782	3879	3885	3895	rVB7	3825	5844	0.28%	0.037%
94	13.846	3895	3905	3913	rBV7	4822	8975	0.43%	0.056%
95	13.904	3920	3923	3925	rBV2	1366	960	0.05%	0.006%
96	14.100	3977	3984	3988	rBV4	3939	5155	0.25%	0.032%
97	14.270	4035	4037	4038	rBV2	858	418	0.02%	0.003%
98	14.286	4039	4042	4049	rVB5	2151	1961	0.09%	0.012%
99	14.338	4051	4058	4062	rBV7	2579	3586	0.17%	0.023%
100	14.444	4088	4091	4092	rBV2	719	411	0.02%	0.003%


Sum of corrected areas: 15893539

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055853.D
Acq On : 23 Oct 2023 14:15
Operator : MD/SY
Sample : 04947-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

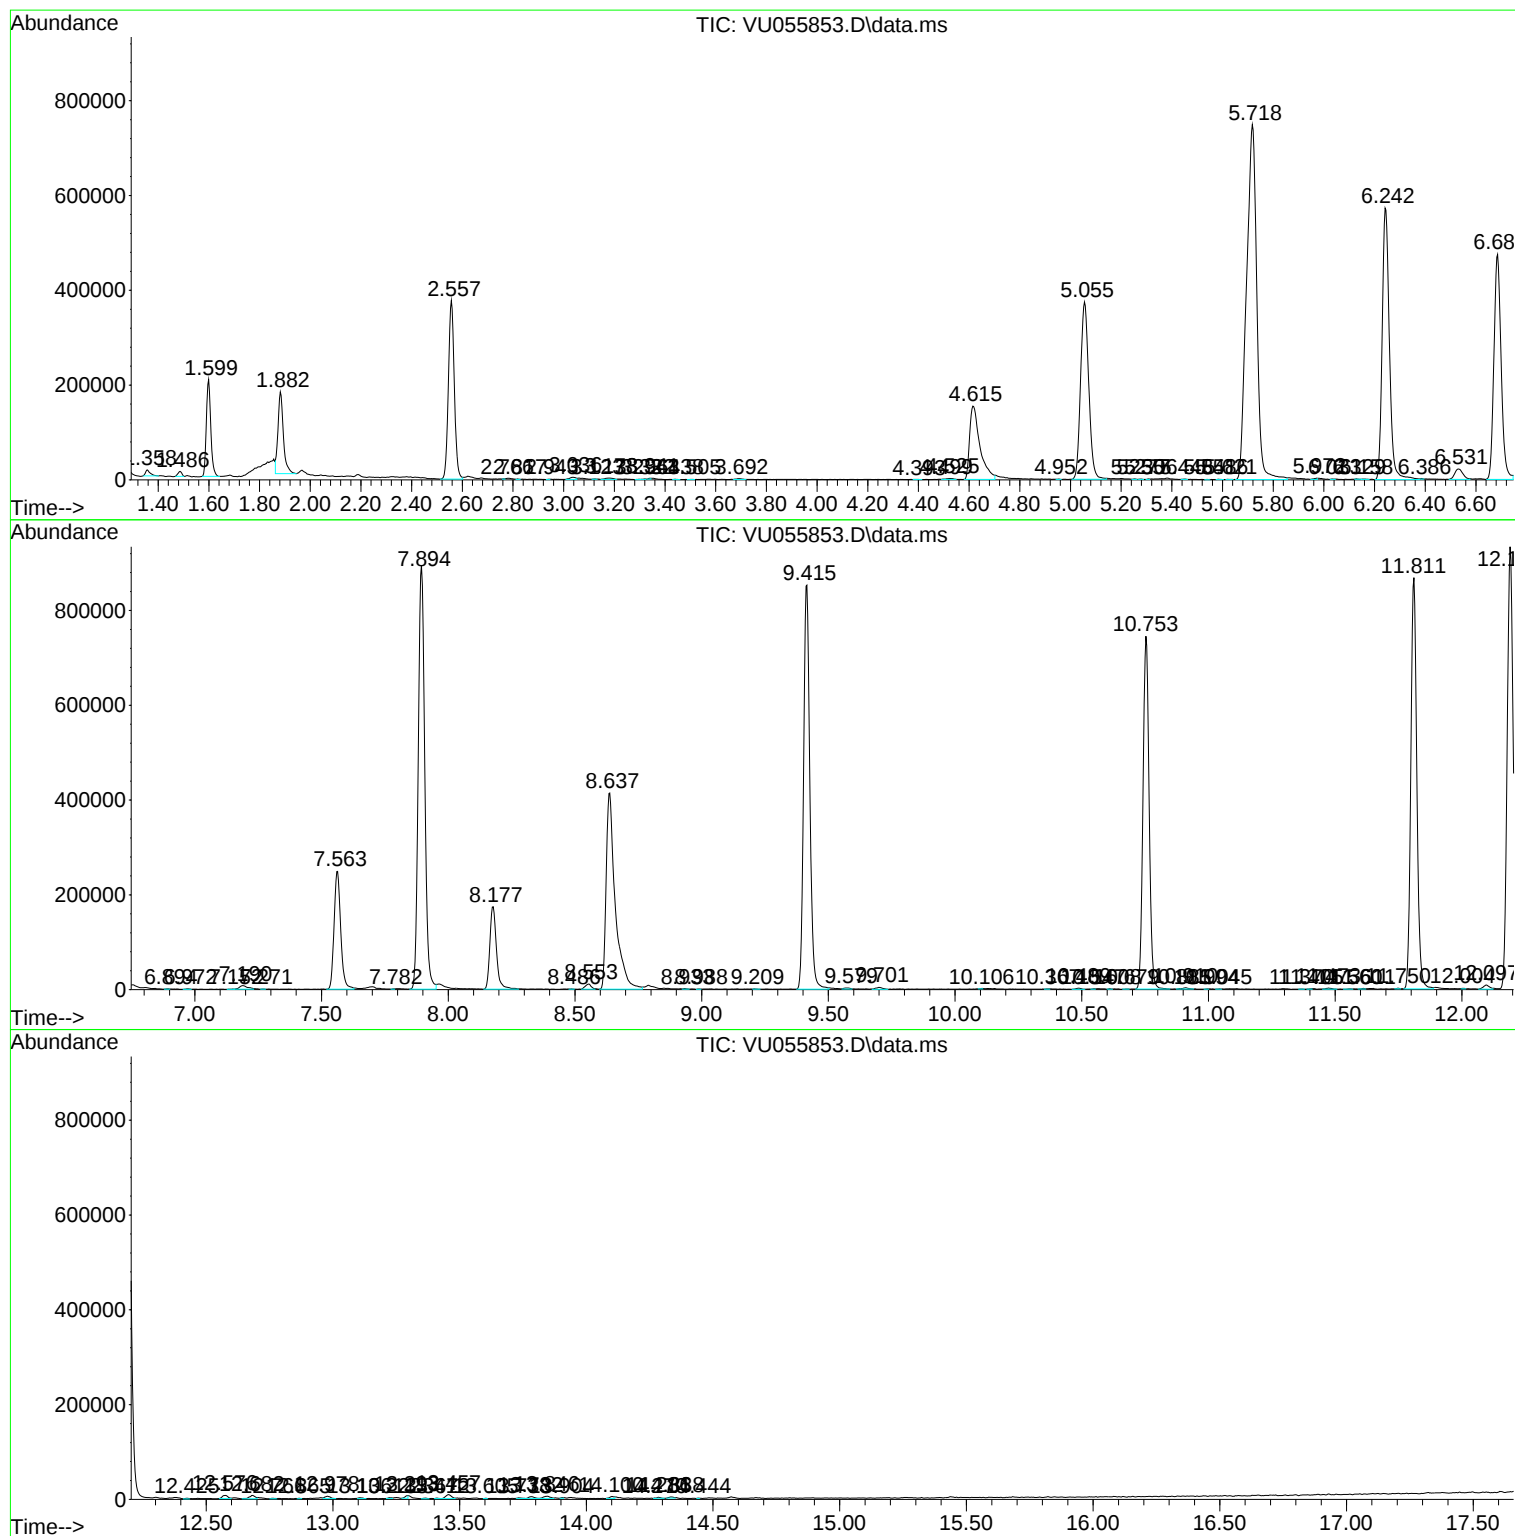

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055853.D
Acq On : 23 Oct 2023 14:15
Operator : MD/SY
Sample : 04947-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055853.D
Acq On : 23 Oct 2023 14:15
Operator : MD/SY
Sample : 04947-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------