

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055854.D
 Acq On : 23 Oct 2023 14:40
 Operator : MD/SY
 Sample : 04947-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055854.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	16	21	23	rBV2	5587	5795	0.24%	0.032%
2	1.486	56	61	67	rVB4	5620	6188	0.26%	0.034%
3	1.518	67	71	75	rBV2	3052	2691	0.11%	0.015%
4	1.602	88	97	112	rBV2	539557	665928	27.79%	3.645%
5	1.679	115	121	129	rVB	31409	35957	1.50%	0.197%
6	1.891	179	187	204	rVB	178613	255047	10.64%	1.396%
7	2.560	379	395	406	rBV	382669	630251	26.30%	3.450%
8	2.618	406	413	438	rVB	75083	137678	5.75%	0.754%
9	2.785	458	465	478	rVB4	5218	10199	0.43%	0.056%
10	2.898	497	500	502	rVV2	572	377	0.02%	0.002%
11	2.959	514	519	525	rVB5	570	639	0.03%	0.003%
12	3.039	532	544	551	rBV6	4477	8957	0.37%	0.049%
13	3.126	564	571	573	rBV3	3058	3347	0.14%	0.018%
14	3.348	627	640	660	rVB	43569	91862	3.83%	0.503%
15	3.550	698	703	704	rBV2	576	491	0.02%	0.003%
16	3.576	704	711	713	rBV3	1655	2113	0.09%	0.012%
17	3.686	741	745	751	rVB4	537	748	0.03%	0.004%
18	3.975	832	835	839	rBV4	609	448	0.02%	0.002%
19	4.042	851	856	858	rBV3	717	694	0.03%	0.004%
20	4.258	917	923	925	rVV3	404	361	0.02%	0.002%
21	4.419	968	973	974	rBV	443	387	0.02%	0.002%
22	4.460	974	986	989	rBV5	2398	4222	0.18%	0.023%
23	4.525	996	1006	1021	rVB4	6848	16648	0.69%	0.091%
24	4.660	1021	1048	1085	rBV2	856338	2396129	100.00%	13.116%
25	4.936	1131	1134	1138	rBV4	521	458	0.02%	0.003%
26	4.956	1138	1140	1143	rVB2	822	337	0.01%	0.002%
27	5.055	1154	1171	1194	rBV	378081	837975	34.97%	4.587%
28	5.203	1215	1217	1220	rBV3	761	534	0.02%	0.003%
29	5.319	1250	1253	1255	rBV2	759	615	0.03%	0.003%
30	5.383	1262	1273	1288	rVB4	7935	17546	0.73%	0.096%
31	5.451	1288	1294	1297	rBV5	928	920	0.04%	0.005%
32	5.599	1338	1340	1344	rVB2	677	443	0.02%	0.002%
33	5.624	1344	1348	1350	rBV2	637	523	0.02%	0.003%
34	5.718	1357	1377	1406	rBV2	741870	2086433	87.08%	11.421%
35	5.917	1437	1439	1443	rVB5	1879	1250	0.05%	0.007%
36	5.984	1452	1460	1468	rVB5	3167	5984	0.25%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055854.D
 Acq On : 23 Oct 2023 14:40
 Operator : MD/SY
 Sample : 04947-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.039	1474	1477	1480	rBV3	439	373	0.02%	0.002%
38	6.097	1493	1495	1498	rVB2	642	344	0.01%	0.002%
39	6.123	1498	1503	1504	rBV2	831	586	0.02%	0.003%
40	6.158	1504	1514	1526	rBV9	2793	5811	0.24%	0.032%
41	6.245	1529	1541	1562	rBV	551702	1071593	44.72%	5.866%
42	6.489	1614	1617	1618	rBV2	876	441	0.02%	0.002%
43	6.528	1619	1629	1643	rVB4	20527	41259	1.72%	0.226%
44	6.599	1648	1651	1654	rBV3	723	559	0.02%	0.003%
45	6.685	1663	1678	1701	rBV	467877	939146	39.19%	5.141%
46	6.894	1735	1743	1748	rBV5	3089	4270	0.18%	0.023%
47	7.078	1796	1800	1801	rBV	768	516	0.02%	0.003%
48	7.123	1809	1814	1817	rBV4	609	538	0.02%	0.003%
49	7.155	1817	1824	1825	rVV3	1056	878	0.04%	0.005%
50	7.187	1825	1834	1852	rVB3	7565	16493	0.69%	0.090%
51	7.328	1876	1878	1885	rVV4	377	335	0.01%	0.002%
52	7.386	1895	1896	1903	rVB2	581	399	0.02%	0.002%
53	7.496	1925	1930	1935	rBV3	917	957	0.04%	0.005%
54	7.563	1935	1951	1975	rBV2	247940	451949	18.86%	2.474%
55	7.695	1986	1992	2000	rBV4	4133	6580	0.27%	0.036%
56	7.750	2007	2009	2013	rVB4	1111	650	0.03%	0.004%
57	7.795	2015	2023	2034	rVB6	3230	6301	0.26%	0.034%
58	7.894	2040	2054	2087	rBV	892342	1593754	66.51%	8.724%
59	8.177	2130	2142	2166	rBV	174474	305634	12.76%	1.673%
60	8.328	2188	2189	2192	rVB	967	424	0.02%	0.002%
61	8.489	2233	2239	2241	rBV5	908	840	0.04%	0.005%
62	8.550	2252	2258	2267	rVB9	2763	4537	0.19%	0.025%
63	8.634	2272	2284	2318	rBV3	378190	965601	40.30%	5.286%
64	8.785	2326	2331	2345	rVB6	13408	24430	1.02%	0.134%
65	9.029	2404	2407	2411	rBV3	650	462	0.02%	0.003%
66	9.103	2427	2430	2432	rBV3	767	505	0.02%	0.003%
67	9.264	2478	2480	2485	rVV4	1241	1038	0.04%	0.006%
68	9.290	2485	2488	2491	rVB3	621	395	0.02%	0.002%
69	9.338	2500	2503	2511	rBV5	873	979	0.04%	0.005%
70	9.415	2513	2527	2549	rBV	801474	1374372	57.36%	7.523%
71	9.566	2571	2574	2577	rBV3	1054	740	0.03%	0.004%
72	9.643	2597	2598	2602	rVB3	645	348	0.01%	0.002%
73	9.968	2696	2699	2701	rVB	777	457	0.02%	0.003%
74	10.251	2782	2787	2792	rBV5	1925	2502	0.10%	0.014%
75	10.351	2812	2818	2825	rBV6	3003	4785	0.20%	0.026%
76	10.483	2856	2859	2862	rBV4	860	672	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055854.D
 Acq On : 23 Oct 2023 14:40
 Operator : MD/SY
 Sample : 04947-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	10.534	2872	2875	2878	rBV2	1283	1122	0.05%	0.006%
78	10.569	2879	2886	2902	rVB5	7885	15137	0.63%	0.083%
79	10.753	2929	2943	2967	rBV	732985	1201172	50.13%	6.575%
80	11.232	3089	3092	3093	rBV2	620	339	0.01%	0.002%
81	11.698	3226	3237	3248	rBV10	3782	7804	0.33%	0.043%
82	11.740	3248	3250	3256	rVB4	990	974	0.04%	0.005%
83	11.811	3259	3272	3296	rBV	831266	1377121	57.47%	7.538%
84	12.094	3347	3360	3366	rBV10	7068	15687	0.65%	0.086%
85	12.190	3378	3390	3411	rBV	924430	1553940	64.85%	8.506%
86	12.618	3519	3523	3527	rBV3	1161	923	0.04%	0.005%
87	12.679	3536	3542	3548	rBV5	2683	3748	0.16%	0.021%
88	12.859	3596	3598	3603	rBV4	745	731	0.03%	0.004%
89	12.901	3603	3611	3620	rBV7	6100	10685	0.45%	0.058%
90	13.286	3728	3731	3732	rBV3	1060	600	0.03%	0.003%
91	13.508	3798	3800	3806	rVB2	584	435	0.02%	0.002%
92	13.704	3856	3861	3863	rBV2	1476	1477	0.06%	0.008%
93	13.839	3900	3903	3904	rBV3	1740	1016	0.04%	0.006%
94	14.110	3978	3987	3995	rBV6	3154	6132	0.26%	0.034%
95	14.335	4053	4057	4066	rVB6	2406	3415	0.14%	0.019%
96	14.704	4169	4172	4175	rBV3	973	669	0.03%	0.004%
97	14.788	4196	4198	4201	rBV2	730	390	0.02%	0.002%
98	14.865	4220	4222	4223	rBV	747	343	0.01%	0.002%
99	14.936	4241	4244	4248	rVB3	1507	1035	0.04%	0.006%
100	15.206	4325	4328	4332	rBV5	1261	982	0.04%	0.005%




Sum of corrected areas: 18268505

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055854.D
Acq On : 23 Oct 2023 14:40
Operator : MD/SY
Sample : 04947-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

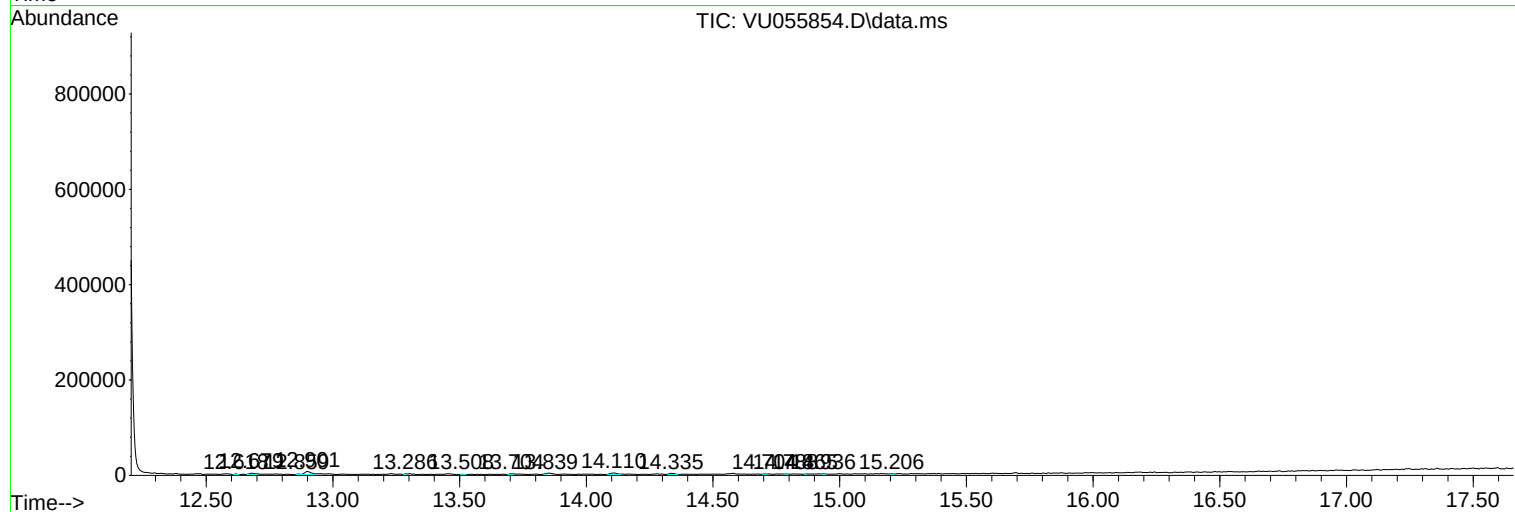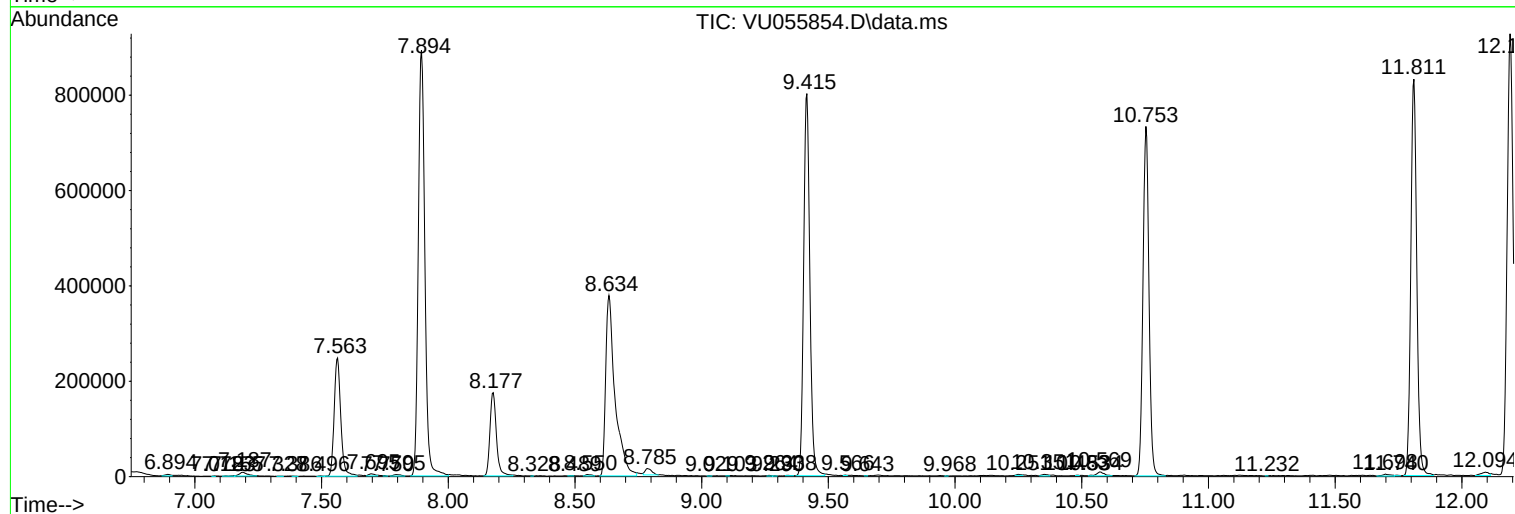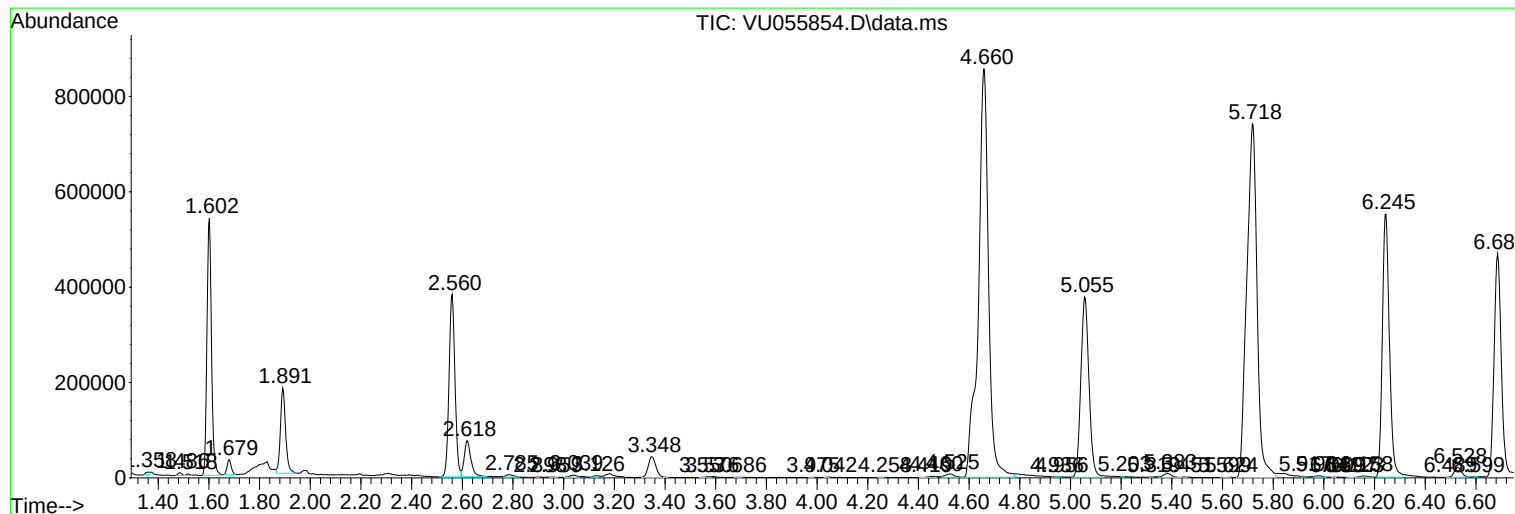

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055854.D
Acq On : 23 Oct 2023 14:40
Operator : MD/SY
Sample : 04947-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055854.D
Acq On : 23 Oct 2023 14:40
Operator : MD/SY
Sample : 04947-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------