

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055855.D
 Acq On : 23 Oct 2023 15:04
 Operator : MD/SY
 Sample : 04947-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.602	88	97	113	rBV2	1190142	1424872	68.30%	8.817%
2	1.891	180	187	204	rVB	170517	241515	11.58%	1.495%
3	2.560	382	395	408	rBV	363154	599969	28.76%	3.713%
4	3.010	532	535	536	rBV	415	211	0.01%	0.001%
5	3.039	536	544	550	rVV9	3225	5484	0.26%	0.034%
6	3.132	561	573	578	rBV8	3191	6381	0.31%	0.039%
7	3.348	627	640	659	rBV3	41602	87699	4.20%	0.543%
8	3.476	678	680	682	rBV2	352	162	0.01%	0.001%
9	3.586	713	714	717	rVB2	337	152	0.01%	0.001%
10	3.608	717	721	725	rBV2	451	463	0.02%	0.003%
11	3.943	817	825	827	rBV2	526	730	0.03%	0.005%
12	3.959	827	830	832	rVV	474	277	0.01%	0.002%
13	4.004	842	844	855	rVB3	1338	1402	0.07%	0.009%
14	4.046	855	857	862	rVB	359	190	0.01%	0.001%
15	4.075	862	866	867	rBV2	612	426	0.02%	0.003%
16	4.177	894	898	901	rBV	394	311	0.01%	0.002%
17	4.316	939	941	945	rVB2	583	267	0.01%	0.002%
18	4.419	971	973	975	rBV	248	148	0.01%	0.001%
19	4.454	980	984	986	rBV2	453	324	0.02%	0.002%
20	4.493	993	996	999	rBV	639	462	0.02%	0.003%
21	4.512	999	1002	1003	rBV2	975	640	0.03%	0.004%
22	4.579	1021	1023	1024	rBV2	335	168	0.01%	0.001%
23	4.618	1024	1035	1037	rBV2	161265	244283	11.71%	1.512%
24	5.055	1156	1171	1195	rBV	356932	805139	38.60%	4.982%
25	5.438	1288	1290	1295	rVB3	689	384	0.02%	0.002%
26	5.467	1296	1299	1301	rVB2	682	330	0.02%	0.002%
27	5.480	1301	1303	1304	rBV2	396	141	0.01%	0.001%
28	5.554	1323	1326	1327	rBV	345	184	0.01%	0.001%
29	5.579	1332	1334	1335	rBV	348	163	0.01%	0.001%
30	5.721	1356	1378	1415	rBV2	718396	2086079	100.00%	12.909%
31	6.023	1470	1472	1473	rBV	399	154	0.01%	0.001%
32	6.245	1527	1541	1561	rBV	549534	1062794	50.95%	6.577%
33	6.528	1619	1629	1645	rVB2	16489	33756	1.62%	0.209%
34	6.685	1664	1678	1711	rBV	455866	913326	43.78%	5.652%
35	6.939	1754	1757	1759	rVB2	448	201	0.01%	0.001%
36	6.975	1767	1768	1770	rBV	206	69	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055855.D
 Acq On : 23 Oct 2023 15:04
 Operator : MD/SY
 Sample : 04947-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	6.988	1770	1772	1773	rBV	170	73	0.00%	0.000%
38	7.013	1777	1780	1781	rBV	292	187	0.01%	0.001%
39	7.062	1792	1795	1800	rVB3	640	450	0.02%	0.003%
40	7.090	1802	1804	1806	rBV	352	174	0.01%	0.001%
41	7.132	1815	1817	1818	rBV2	357	146	0.01%	0.001%
42	7.190	1828	1835	1845	rBV5	5552	9565	0.46%	0.059%
43	7.306	1868	1871	1874	rVB2	478	287	0.01%	0.002%
44	7.319	1874	1875	1877	rBV	268	119	0.01%	0.001%
45	7.341	1877	1882	1884	rBV	320	219	0.01%	0.001%
46	7.393	1896	1898	1900	rVB	288	101	0.00%	0.001%
47	7.438	1910	1912	1913	rBV2	317	96	0.00%	0.001%
48	7.560	1936	1950	1975	rBV	236803	438559	21.02%	2.714%
49	7.894	2041	2054	2079	rBV	855997	1524531	73.08%	9.434%
50	8.177	2131	2142	2163	rBV	165007	289967	13.90%	1.794%
51	8.332	2187	2190	2193	rBV2	616	292	0.01%	0.002%
52	8.377	2201	2204	2209	rBV3	708	665	0.03%	0.004%
53	8.406	2212	2213	2216	rBV2	444	207	0.01%	0.001%
54	8.547	2252	2257	2260	rBV4	1559	1602	0.08%	0.010%
55	8.634	2271	2284	2322	rBV4	383393	962392	46.13%	5.955%
56	9.039	2408	2410	2411	rBV	520	219	0.01%	0.001%
57	9.068	2416	2419	2421	rBV2	792	449	0.02%	0.003%
58	9.087	2423	2425	2426	rBV2	320	84	0.00%	0.001%
59	9.155	2444	2446	2451	rVB	306	173	0.01%	0.001%
60	9.174	2451	2452	2455	rVB2	364	129	0.01%	0.001%
61	9.187	2455	2456	2457	rBV2	322	113	0.01%	0.001%
62	9.261	2476	2479	2482	rBV2	560	367	0.02%	0.002%
63	9.280	2482	2485	2490	rVV3	481	550	0.03%	0.003%
64	9.328	2493	2500	2504	rBV3	671	745	0.04%	0.005%
65	9.415	2513	2527	2548	rBV	819321	1371837	65.76%	8.489%
66	9.698	2608	2615	2619	rBV2	1767	2165	0.10%	0.013%
67	9.840	2656	2659	2662	rBV3	508	424	0.02%	0.003%
68	10.087	2733	2736	2737	rBV	489	255	0.01%	0.002%
69	10.123	2744	2747	2748	rBV3	920	443	0.02%	0.003%
70	10.312	2805	2806	2809	rVB	386	97	0.00%	0.001%
71	10.357	2817	2820	2826	rBV4	948	757	0.04%	0.005%
72	10.521	2869	2871	2875	rVB2	402	245	0.01%	0.002%
73	10.553	2876	2881	2887	rVB2	754	758	0.04%	0.005%
74	10.753	2930	2943	2962	rBV	728906	1193380	57.21%	7.385%
75	10.885	2982	2984	2989	rBV4	1028	857	0.04%	0.005%
76	10.968	3008	3010	3014	rVB2	760	363	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055855.D
 Acq On : 23 Oct 2023 15:04
 Operator : MD/SY
 Sample : 04947-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M

Title : VOC Analysis

77	11.238	3091	3094	3096	rBV	308	191	0.01%	0.001%
78	11.251	3096	3098	3099	rBV	240	108	0.01%	0.001%
79	11.412	3145	3148	3154	rVB3	1008	627	0.03%	0.004%
80	11.476	3162	3168	3172	rBV3	978	1158	0.06%	0.007%
81	11.502	3175	3176	3177	rVB	691	133	0.01%	0.001%
82	11.512	3177	3179	3180	rBV2	399	150	0.01%	0.001%
83	11.592	3201	3204	3206	rBV3	487	237	0.01%	0.001%
84	11.807	3259	3271	3292	rBV	837443	1353012	64.86%	8.373%
85	12.081	3346	3356	3357	rBV7	5625	6650	0.32%	0.041%
86	12.190	3378	3390	3417	rVB	899579	1473597	70.64%	9.119%
87	12.675	3538	3541	3546	rBV3	1176	945	0.05%	0.006%




Sum of corrected areas: 16160106

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055855.D
Acq On : 23 Oct 2023 15:04
Operator : MD/SY
Sample : 04947-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

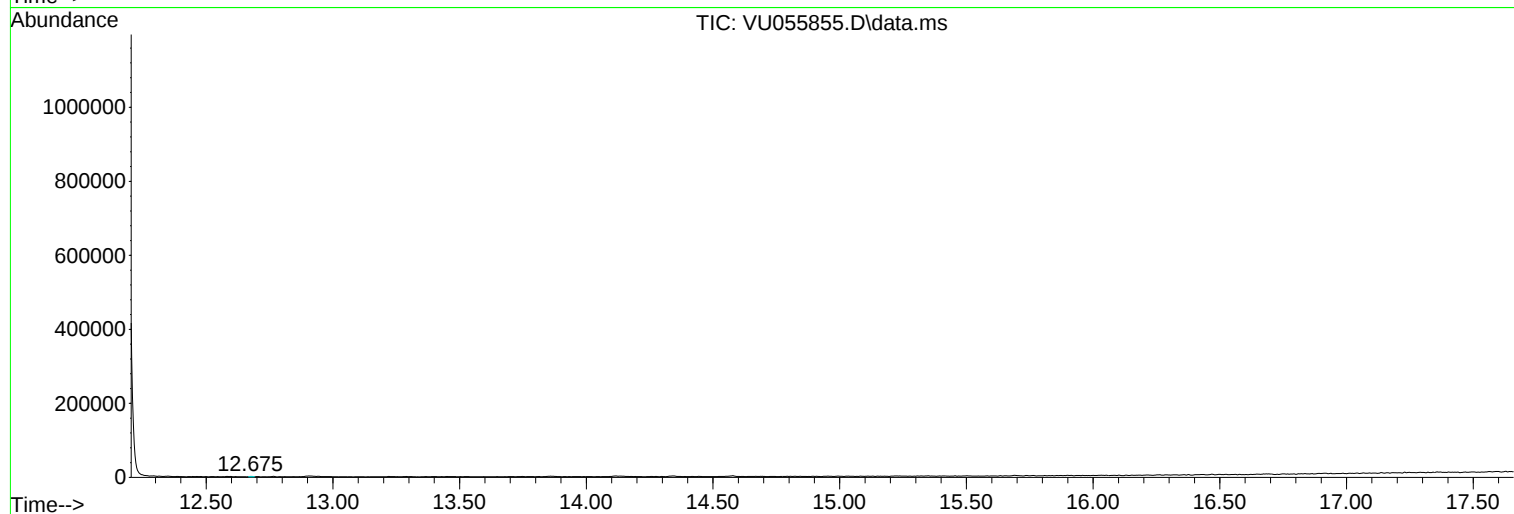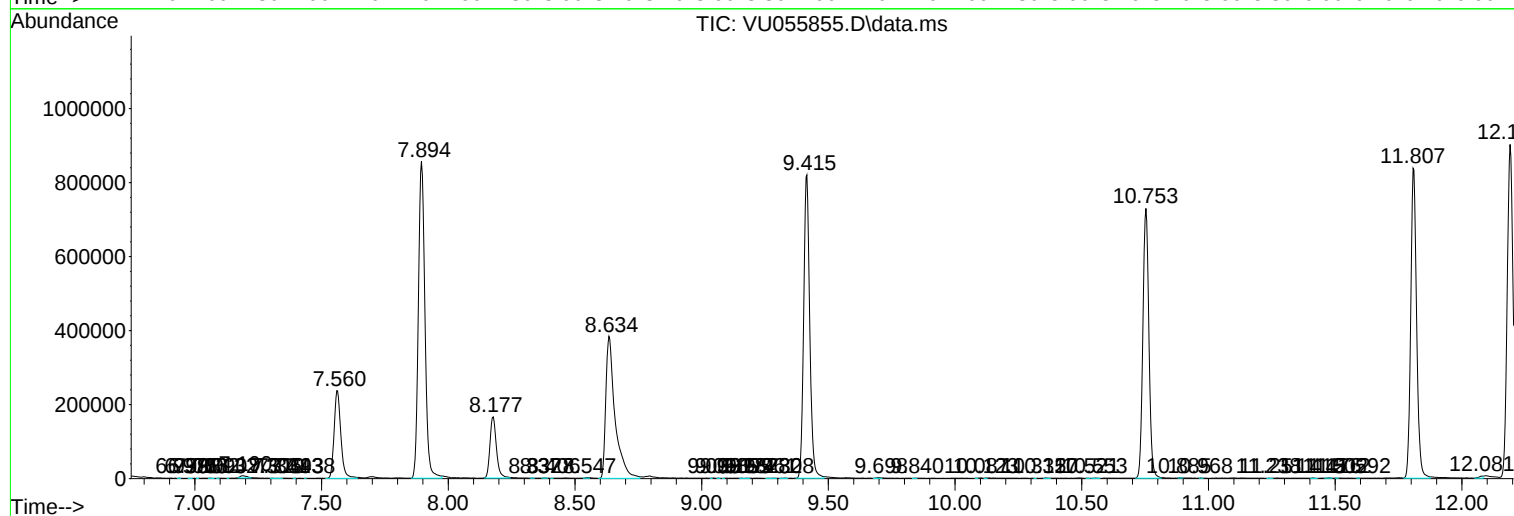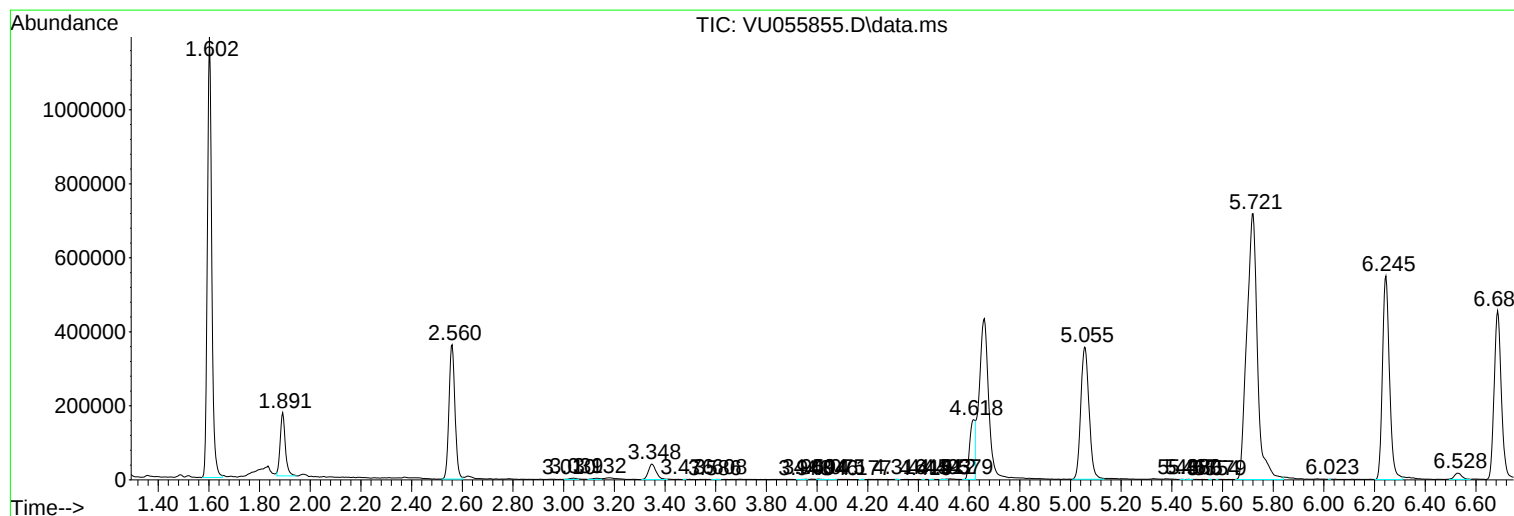

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055855.D
Acq On : 23 Oct 2023 15:04
Operator : MD/SY
Sample : 04947-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055855.D
Acq On : 23 Oct 2023 15:04
Operator : MD/SY
Sample : 04947-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------