

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055856.D
 Acq On : 23 Oct 2023 15:28
 Operator : MD/SY
 Sample : 04947-07 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	112	rBV	213347	257675	11.46%	1.474%
2	1.888	179	186	202	rVB	167643	239682	10.66%	1.371%
3	2.557	382	394	416	rBV	363215	596914	26.54%	3.415%
4	2.779	461	463	466	rBV2	778	468	0.02%	0.003%
5	2.943	509	514	518	rBV4	624	559	0.02%	0.003%
6	3.036	534	543	555	rVB4	7494	13486	0.60%	0.077%
7	3.097	559	562	567	rVB2	488	436	0.02%	0.002%
8	3.181	572	588	605	rBV	21799	56736	2.52%	0.325%
9	3.351	629	641	656	rVV3	14247	28139	1.25%	0.161%
10	3.499	681	687	691	rBV2	464	444	0.02%	0.003%
11	3.570	704	709	716	rVB2	605	519	0.02%	0.003%
12	3.679	740	743	748	rVV	505	347	0.02%	0.002%
13	3.756	765	767	771	rBV2	375	346	0.02%	0.002%
14	3.798	777	780	786	rVB2	508	383	0.02%	0.002%
15	3.952	824	828	831	rVV	384	426	0.02%	0.002%
16	3.972	831	834	838	rVV3	629	455	0.02%	0.003%
17	3.991	838	840	845	rVB2	497	327	0.01%	0.002%
18	4.042	851	856	859	rVB2	588	546	0.02%	0.003%
19	4.216	906	910	914	rBV2	345	339	0.02%	0.002%
20	4.328	942	945	950	rBV2	285	337	0.01%	0.002%
21	4.399	960	967	974	rVB3	609	1021	0.05%	0.006%
22	4.656	1023	1047	1075	rBV2	811585	2249170	100.00%	12.868%
23	5.055	1154	1171	1191	rBV	355896	792395	35.23%	4.533%
24	5.283	1240	1242	1247	rVB4	706	499	0.02%	0.003%
25	5.309	1247	1250	1251	rBV	1096	582	0.03%	0.003%
26	5.328	1253	1256	1263	rVB5	1834	2173	0.10%	0.012%
27	5.486	1301	1305	1307	rBV2	473	397	0.02%	0.002%
28	5.647	1351	1355	1356	rBV	512	396	0.02%	0.002%
29	5.717	1357	1377	1409	rBV3	699660	1953283	86.84%	11.175%
30	6.055	1480	1482	1486	rVB3	828	435	0.02%	0.002%
31	6.245	1527	1541	1566	rBV	551925	1085716	48.27%	6.211%
32	6.431	1597	1599	1606	rVB5	745	675	0.03%	0.004%
33	6.537	1617	1632	1656	rBV2	275991	546874	24.31%	3.129%
34	6.685	1665	1678	1702	rBV	442879	881399	39.19%	5.043%
35	6.859	1727	1732	1735	rVB4	680	611	0.03%	0.003%
36	6.901	1740	1745	1749	rVB3	430	385	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055856.D
 Acq On : 23 Oct 2023 15:28
 Operator : MD/SY
 Sample : 04947-07 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.068	1792	1797	1798	rBV2	562	457	0.02%	0.003%
38	7.184	1819	1833	1848	rBV4	6739	16933	0.75%	0.097%
39	7.386	1893	1896	1898	rBV	552	327	0.01%	0.002%
40	7.479	1921	1925	1929	rBV2	452	390	0.02%	0.002%
41	7.563	1937	1951	1974	rBV	235810	428784	19.06%	2.453%
42	7.692	1987	1991	1992	rBV3	2642	1671	0.07%	0.010%
43	7.804	2022	2026	2033	rVB4	1100	1382	0.06%	0.008%
44	7.894	2040	2054	2090	rBV	850794	1497625	66.59%	8.568%
45	8.177	2130	2142	2165	rBV	164595	287131	12.77%	1.643%
46	8.402	2206	2212	2214	rBV3	633	603	0.03%	0.003%
47	8.473	2233	2234	2239	rVB2	819	422	0.02%	0.002%
48	8.550	2247	2258	2273	rBV	94601	160527	7.14%	0.918%
49	8.634	2273	2284	2324	rBV4	386389	961923	42.77%	5.503%
50	8.856	2351	2353	2355	rBV3	785	384	0.02%	0.002%
51	8.920	2367	2373	2377	rBV4	773	896	0.04%	0.005%
52	8.942	2377	2380	2385	rVV5	751	598	0.03%	0.003%
53	9.020	2401	2404	2406	rVB2	677	380	0.02%	0.002%
54	9.142	2438	2442	2443	rBV	538	396	0.02%	0.002%
55	9.219	2463	2466	2471	rVB2	667	476	0.02%	0.003%
56	9.412	2514	2526	2547	rBV	818544	1384499	61.56%	7.921%
57	9.643	2594	2598	2602	rVV2	498	453	0.02%	0.003%
58	9.692	2609	2613	2615	rBV3	1749	1294	0.06%	0.007%
59	9.795	2641	2645	2648	rVV2	460	419	0.02%	0.002%
60	9.859	2661	2665	2669	rBV2	430	327	0.01%	0.002%
61	9.965	2695	2698	2701	rBV2	521	405	0.02%	0.002%
62	10.467	2851	2854	2857	rBV2	525	378	0.02%	0.002%
63	10.499	2857	2864	2869	rVB3	772	1138	0.05%	0.007%
64	10.534	2869	2875	2881	rVB2	692	740	0.03%	0.004%
65	10.566	2881	2885	2890	rBV2	821	710	0.03%	0.004%
66	10.637	2903	2907	2910	rBV2	371	348	0.02%	0.002%
67	10.701	2923	2927	2930	rBV2	560	449	0.02%	0.003%
68	10.753	2930	2943	2963	rBV	717238	1174482	52.22%	6.719%
69	10.965	3006	3009	3011	rVV2	700	386	0.02%	0.002%
70	10.991	3011	3017	3020	rVB3	543	588	0.03%	0.003%
71	11.026	3025	3028	3031	rBV2	458	378	0.02%	0.002%
72	11.097	3046	3050	3054	rBV5	689	605	0.03%	0.003%
73	11.148	3061	3066	3068	rBV3	499	380	0.02%	0.002%
74	11.171	3068	3073	3074	rBV3	459	372	0.02%	0.002%
75	11.245	3089	3096	3097	rBV2	341	358	0.02%	0.002%
76	11.528	3180	3184	3187	rVB3	553	502	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055856.D
 Acq On : 23 Oct 2023 15:28
 Operator : MD/SY
 Sample : 04947-07 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45J4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.553	3187	3192	3193	rBV	471	417	0.02%	0.002%
78	11.608	3206	3209	3212	rBV2	489	334	0.01%	0.002%
79	11.756	3247	3255	3259	rBV4	1145	1446	0.06%	0.008%
80	11.811	3259	3272	3304	rBV	843695	1369255	60.88%	7.834%
81	12.019	3335	3337	3340	rBV3	615	381	0.02%	0.002%
82	12.190	3377	3390	3416	rBV	857385	1447675	64.36%	8.282%
83	12.351	3438	3440	3443	rVB4	789	354	0.02%	0.002%
84	12.460	3471	3474	3476	rBV2	496	414	0.02%	0.002%
85	12.502	3483	3487	3489	rBV2	789	590	0.03%	0.003%
86	12.704	3547	3550	3555	rBV4	622	542	0.02%	0.003%
87	12.775	3569	3572	3580	rVB5	1029	1078	0.05%	0.006%
88	12.855	3594	3597	3603	rVB3	670	565	0.03%	0.003%
89	12.884	3603	3606	3609	rBV2	709	394	0.02%	0.002%
90	12.991	3636	3639	3641	rBV2	726	509	0.02%	0.003%
91	13.003	3641	3643	3647	rVB3	904	608	0.03%	0.003%
92	13.145	3683	3687	3688	rBV	644	447	0.02%	0.003%
93	13.183	3696	3699	3702	rBV2	655	542	0.02%	0.003%
94	13.216	3706	3709	3713	rBV3	616	570	0.03%	0.003%
95	13.460	3782	3785	3787	rBV2	696	393	0.02%	0.002%
96	13.579	3818	3822	3825	rBV2	576	561	0.02%	0.003%
97	13.865	3907	3911	3914	rBV4	1137	885	0.04%	0.005%
98	14.126	3984	3992	3995	rBV3	2090	2960	0.13%	0.017%
99	14.341	4051	4059	4065	rBV7	1640	2643	0.12%	0.015%
100	15.068	4282	4285	4288	rBV4	1188	708	0.03%	0.004%




Sum of corrected areas: 17479362

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055856.D
Acq On : 23 Oct 2023 15:28
Operator : MD/SY
Sample : 04947-07 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

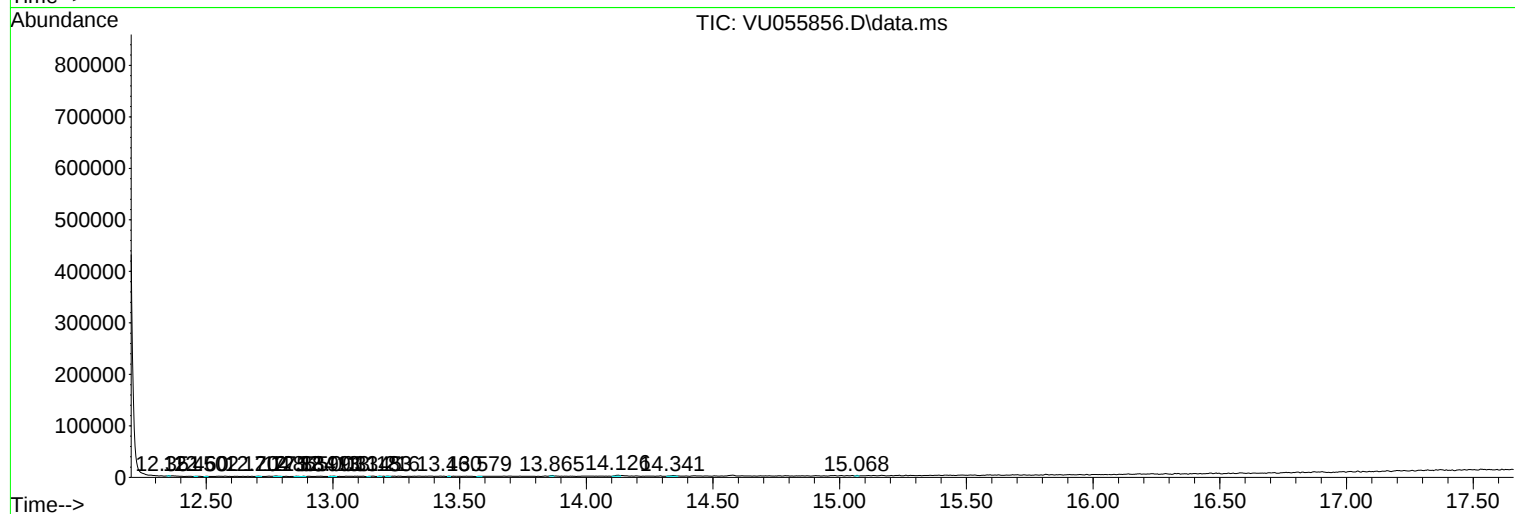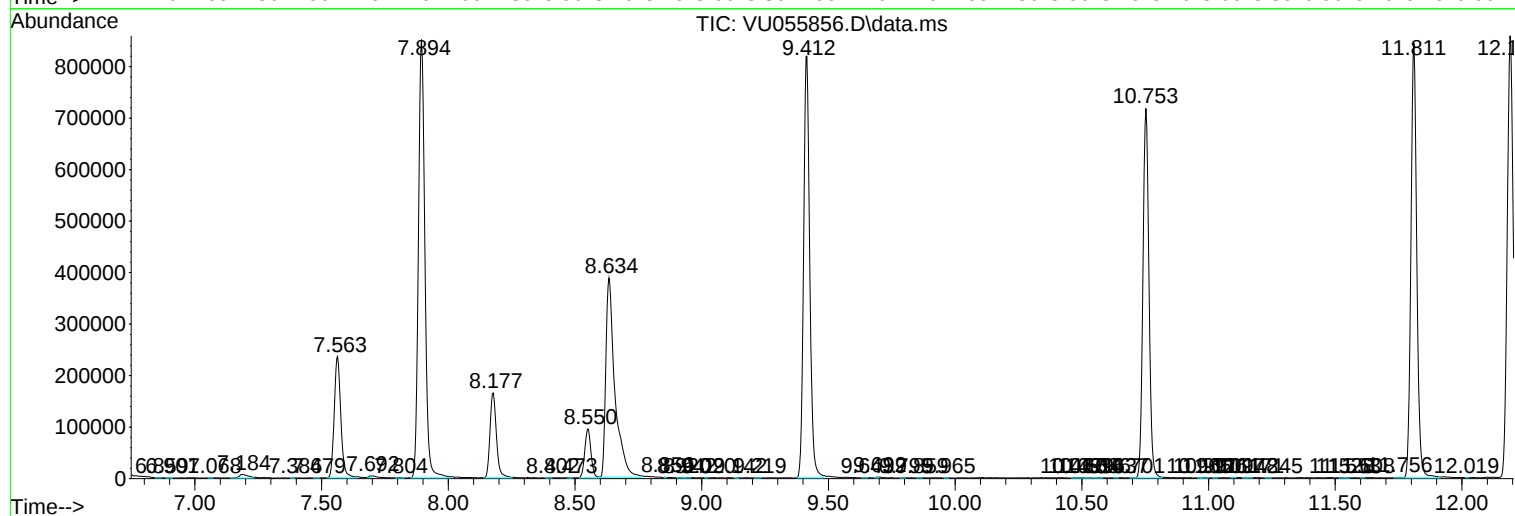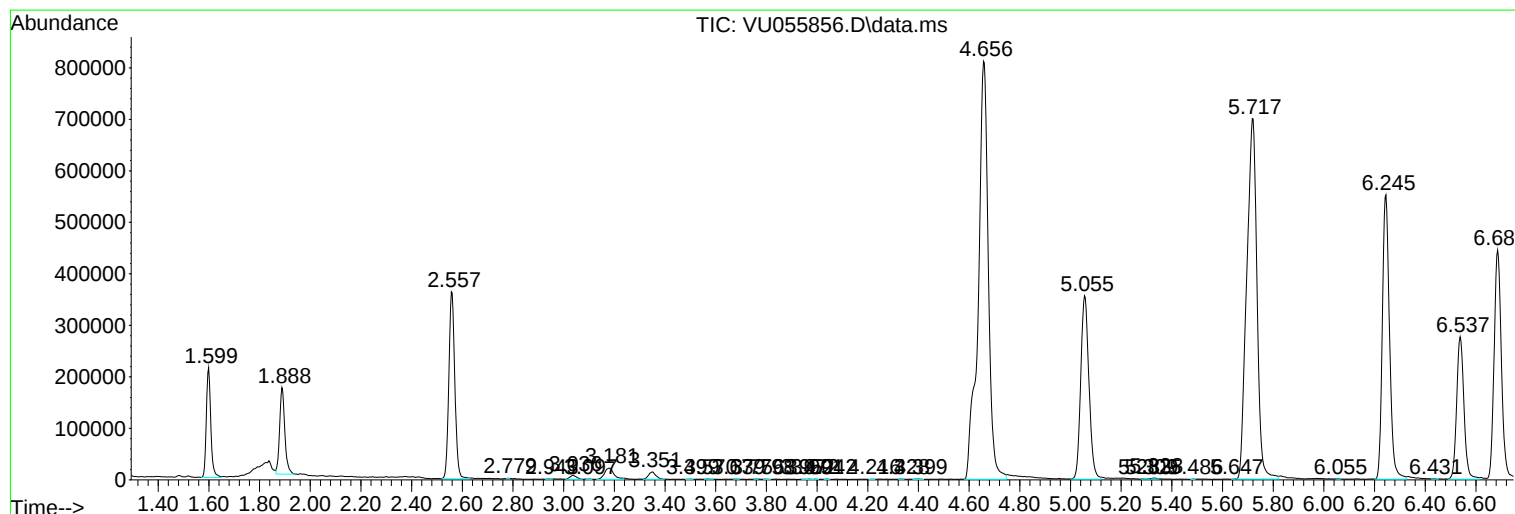

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055856.D
Acq On : 23 Oct 2023 15:28
Operator : MD/SY
Sample : 04947-07 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055856.D
Acq On : 23 Oct 2023 15:28
Operator : MD/SY
Sample : 04947-07 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45J4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------