

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055857.D
 Acq On : 23 Oct 2023 16:28
 Operator : MD/SY
 Sample : 04947-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

Signal : TIC: VU055857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	111	rBV	210781	250333	11.77%	1.543%
2	1.888	178	186	206	rVB	178002	262134	12.33%	1.615%
3	2.509	377	379	382	rBV4	579	336	0.02%	0.002%
4	2.557	382	394	411	rBV	391277	642281	30.20%	3.958%
5	2.782	461	464	474	rVB4	2528	3122	0.15%	0.019%
6	2.891	495	498	499	rBV	607	350	0.02%	0.002%
7	2.901	499	501	505	rVB	727	394	0.02%	0.002%
8	2.956	513	518	523	rBV5	728	756	0.04%	0.005%
9	2.994	527	530	533	rVB2	504	309	0.01%	0.002%
10	3.039	535	544	553	rVB4	4247	7816	0.37%	0.048%
11	3.184	576	589	594	rBV6	1955	4196	0.20%	0.026%
12	3.345	635	639	642	rBV6	1489	1561	0.07%	0.010%
13	3.477	673	680	682	rBV2	414	408	0.02%	0.003%
14	3.547	698	702	710	rVB3	476	643	0.03%	0.004%
15	3.737	756	761	764	rBV3	454	333	0.02%	0.002%
16	3.952	826	828	832	rBV	335	318	0.01%	0.002%
17	4.026	844	851	854	rBV2	378	412	0.02%	0.003%
18	4.165	890	894	899	rBV2	288	318	0.01%	0.002%
19	4.248	911	920	924	rVB2	416	582	0.03%	0.004%
20	4.354	949	953	957	rVB2	481	332	0.02%	0.002%
21	4.431	971	977	984	rBV2	452	642	0.03%	0.004%
22	4.615	1019	1034	1063	rBV	171462	463926	21.81%	2.859%
23	5.055	1151	1171	1198	rBV	389700	871272	40.97%	5.369%
24	5.303	1243	1248	1250	rBV3	1036	890	0.04%	0.005%
25	5.518	1308	1315	1322	rBV3	954	1496	0.07%	0.009%
26	5.721	1356	1378	1405	rBV2	756557	2126715	100.00%	13.105%
27	6.026	1470	1473	1476	rBV2	473	370	0.02%	0.002%
28	6.042	1476	1478	1482	rVV3	541	343	0.02%	0.002%
29	6.245	1525	1541	1571	rBV	589286	1151868	54.16%	7.098%
30	6.460	1606	1608	1612	rVB2	943	457	0.02%	0.003%
31	6.528	1616	1629	1642	rBV2	23835	49257	2.32%	0.304%
32	6.685	1663	1678	1707	rBV	494924	976164	45.90%	6.015%
33	6.862	1730	1733	1735	rBV3	499	306	0.01%	0.002%
34	7.087	1799	1803	1805	rBV2	523	394	0.02%	0.002%
35	7.190	1823	1835	1851	rVV4	8246	18197	0.86%	0.112%
36	7.296	1865	1868	1871	rVB3	612	404	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055857.D
 Acq On : 23 Oct 2023 16:28
 Operator : MD/SY
 Sample : 04947-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

37	7.316	1871	1874	1881	rBV2	583	728	0.03%	0.004%
38	7.357	1881	1887	1891	rBV3	556	475	0.02%	0.003%
39	7.483	1920	1926	1929	rBV3	376	344	0.02%	0.002%
40	7.563	1938	1951	1981	rBV	252543	469069	22.06%	2.890%
41	7.695	1985	1992	2002	rBV5	4269	6909	0.32%	0.043%
42	7.769	2012	2015	2021	rBV4	642	673	0.03%	0.004%
43	7.798	2021	2024	2031	rVB5	1330	1502	0.07%	0.009%
44	7.830	2031	2034	2038	rVB3	479	389	0.02%	0.002%
45	7.894	2040	2054	2094	rBV	924117	1637110	76.98%	10.088%
46	8.065	2104	2107	2110	rVB3	722	483	0.02%	0.003%
47	8.177	2127	2142	2160	rBV	178441	311348	14.64%	1.919%
48	8.316	2182	2185	2187	rBV2	609	379	0.02%	0.002%
49	8.367	2199	2201	2205	rVB3	488	348	0.02%	0.002%
50	8.409	2205	2214	2222	rBV9	946	2007	0.09%	0.012%
51	8.550	2253	2258	2266	rVB7	2066	3452	0.16%	0.021%
52	8.634	2272	2284	2327	rBV3	413720	1052586	49.49%	6.486%
53	8.917	2369	2372	2373	rBV2	703	353	0.02%	0.002%
54	9.142	2439	2442	2451	rVB3	687	778	0.04%	0.005%
55	9.415	2514	2527	2551	rBV	875790	1474024	69.31%	9.083%
56	9.566	2569	2574	2576	rBV3	1865	1657	0.08%	0.010%
57	9.701	2607	2616	2624	rBV5	2340	3744	0.18%	0.023%
58	9.785	2640	2642	2649	rVB	642	494	0.02%	0.003%
59	9.824	2649	2654	2659	rBV3	553	472	0.02%	0.003%
60	9.936	2685	2689	2693	rBV2	411	330	0.02%	0.002%
61	9.984	2701	2704	2708	rBV	514	537	0.03%	0.003%
62	10.097	2734	2739	2740	rBV2	644	521	0.02%	0.003%
63	10.110	2740	2743	2744	rBV2	989	511	0.02%	0.003%
64	10.254	2784	2788	2791	rVB	526	354	0.02%	0.002%
65	10.322	2803	2809	2813	rBV2	519	534	0.03%	0.003%
66	10.383	2824	2828	2833	rBV	432	448	0.02%	0.003%
67	10.489	2854	2861	2877	rVB3	1894	2940	0.14%	0.018%
68	10.621	2897	2902	2906	rBV2	511	572	0.03%	0.004%
69	10.653	2910	2912	2918	rVB2	469	432	0.02%	0.003%
70	10.692	2918	2924	2926	rBV2	455	450	0.02%	0.003%
71	10.753	2930	2943	2961	rBV	780000	1277115	60.05%	7.870%
72	10.869	2977	2979	2982	rVB3	825	409	0.02%	0.003%
73	10.891	2982	2986	2988	rVB2	484	332	0.02%	0.002%
74	11.013	3017	3024	3029	rVB2	416	505	0.02%	0.003%
75	11.039	3029	3032	3036	rBV	370	432	0.02%	0.003%
76	11.097	3048	3050	3056	rVV3	571	557	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055857.D
 Acq On : 23 Oct 2023 16:28
 Operator : MD/SY
 Sample : 04947-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis

77	11.348	3124	3128	3130	rBV	398	339	0.02%	0.002%
78	11.470	3160	3166	3168	rBV3	1299	1254	0.06%	0.008%
79	11.515	3178	3180	3186	rBV2	395	333	0.02%	0.002%
80	11.746	3244	3252	3260	rBV4	1750	2696	0.13%	0.017%
81	11.811	3260	3272	3294	rBV	906801	1482109	69.69%	9.133%
82	12.049	3341	3346	3349	rBV2	841	721	0.03%	0.004%
83	12.113	3360	3366	3370	rBV	665	587	0.03%	0.004%
84	12.190	3376	3390	3421	rBV	984406	1632166	76.75%	10.058%
85	12.438	3464	3467	3469	rBV3	725	464	0.02%	0.003%
86	12.637	3525	3529	3532	rVB2	459	339	0.02%	0.002%
87	12.766	3566	3569	3574	rVV4	727	771	0.04%	0.005%
88	12.814	3581	3584	3587	rBV2	512	325	0.02%	0.002%
89	13.232	3711	3714	3716	rBV3	766	512	0.02%	0.003%
90	13.515	3799	3802	3806	rBV2	542	453	0.02%	0.003%
91	13.582	3821	3823	3826	rVB2	635	332	0.02%	0.002%
92	14.216	4018	4020	4024	rVB3	759	447	0.02%	0.003%
93	14.347	4053	4061	4073	rBV8	1894	3549	0.17%	0.022%
94	14.499	4106	4108	4113	rBV3	621	510	0.02%	0.003%
95	14.550	4121	4124	4126	rBV3	839	571	0.03%	0.004%
96	14.627	4146	4148	4150	rBV2	552	340	0.02%	0.002%
97	14.775	4191	4194	4197	rBV4	922	637	0.03%	0.004%
98	14.852	4215	4218	4221	rBV4	770	642	0.03%	0.004%
99	15.148	4308	4310	4319	rBV5	865	963	0.05%	0.006%
100	15.267	4342	4347	4349	rBV3	1329	1090	0.05%	0.007%




Sum of corrected areas: 16228088

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055857.D
Acq On : 23 Oct 2023 16:28
Operator : MD/SY
Sample : 04947-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

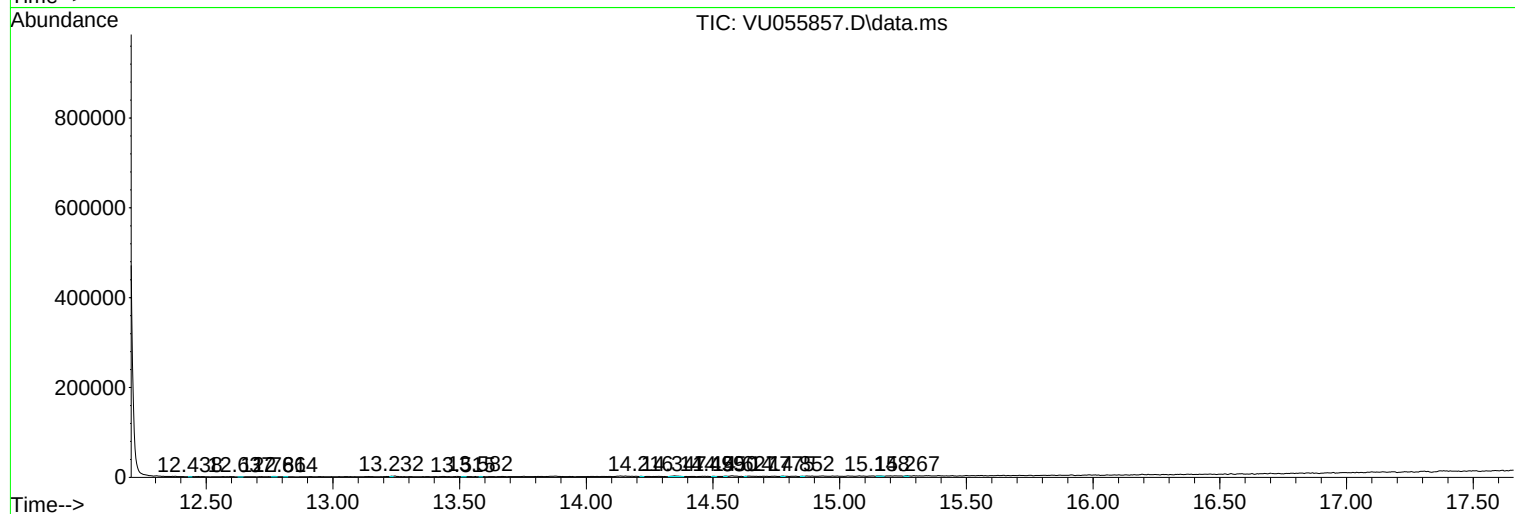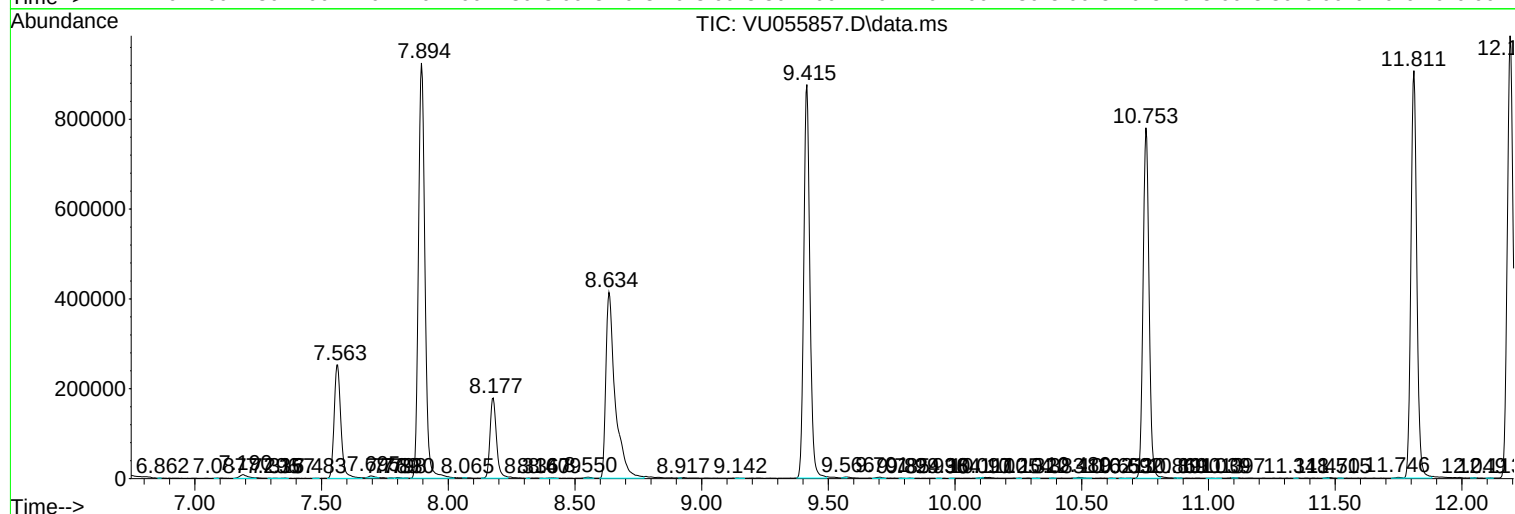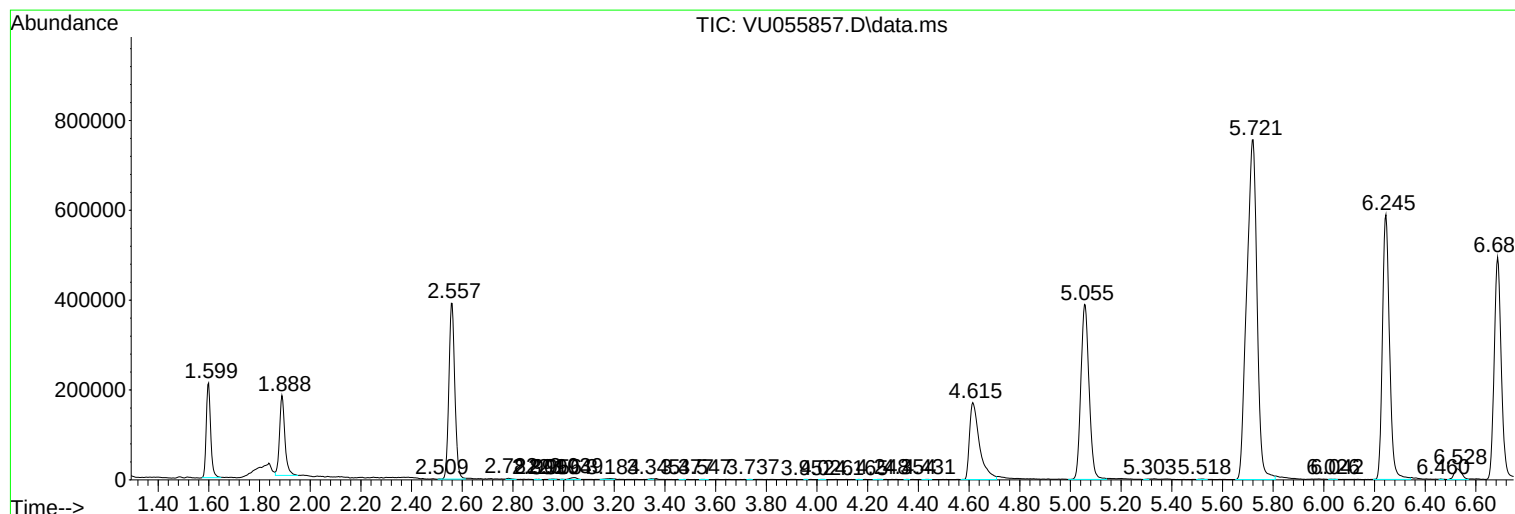

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055857.D
Acq On : 23 Oct 2023 16:28
Operator : MD/SY
Sample : 04947-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
Data File : VU055857.D
Acq On : 23 Oct 2023 16:28
Operator : MD/SY
Sample : 04947-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------