


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU102323\
 Data File : VU055846.D
 Acq On : 23 Oct 2023 08:46
 Operator : MD/SY
 Sample : BFB026
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB026

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM101023WMA.M
 Title : VOC Analysis
 Last Update : Thu Oct 26 01:50:39 2023

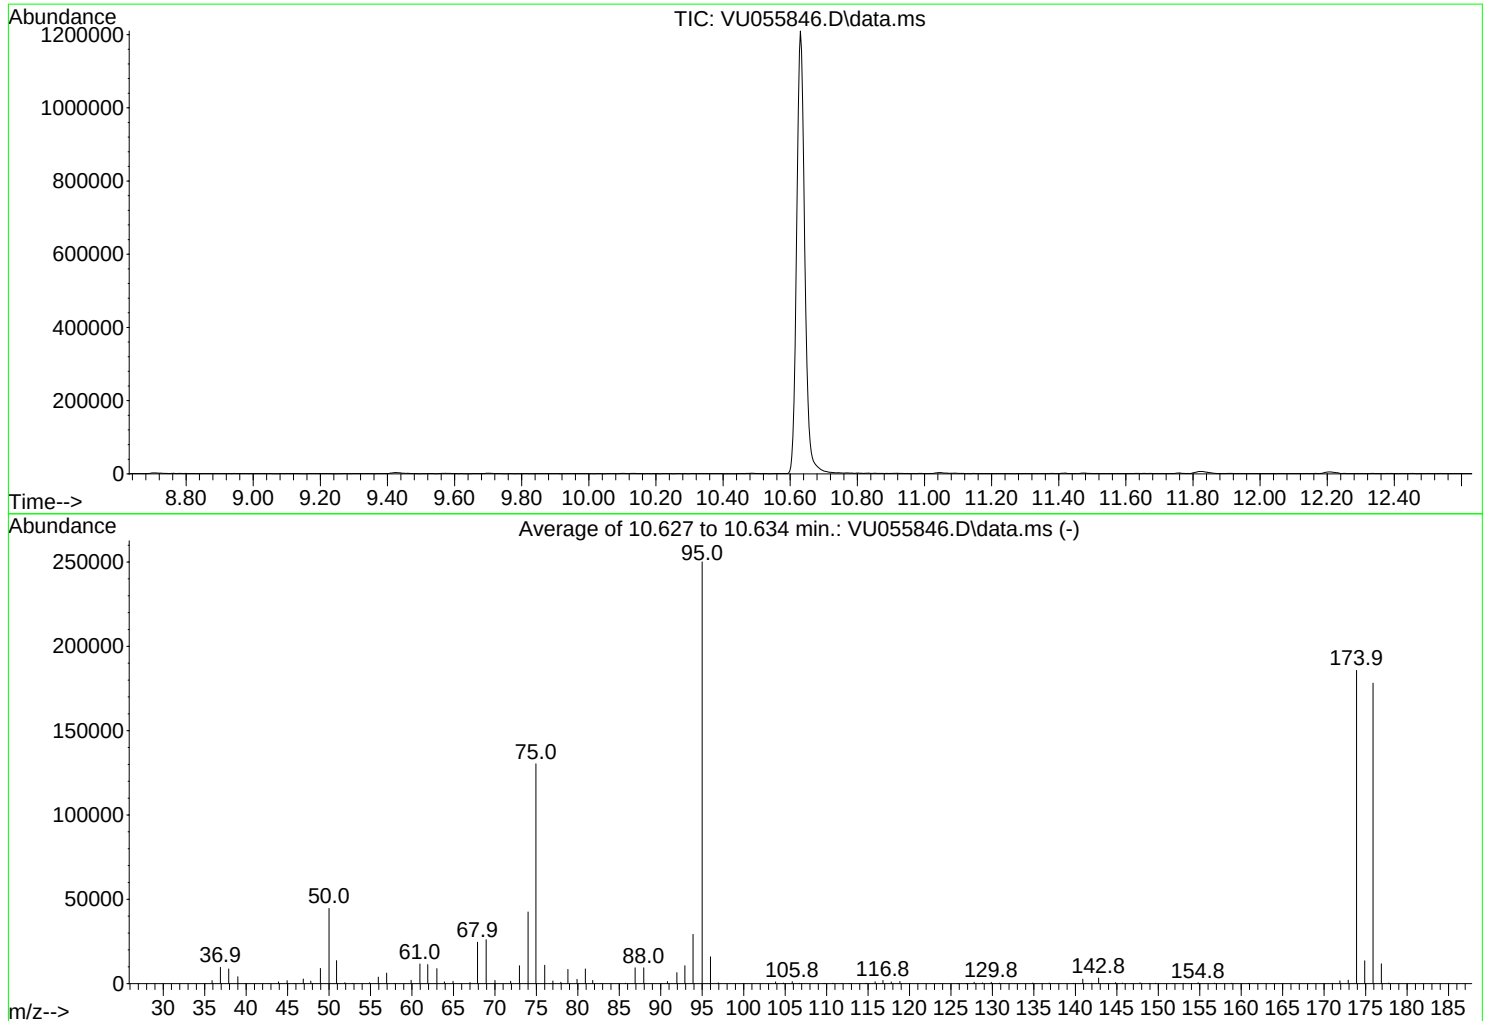

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	44592	PASS
75	95	30	80	52.1	130325	PASS
95	95	100	100	100.0	250112	PASS
96	95	5	9	6.4	15970	PASS
173	174	0.00	2	1.1	2090	PASS
174	95	50	120	74.3	185813	PASS
175	174	5	9	7.3	13626	PASS
176	174	95	101	95.9	178155	PASS
177	176	5	9	6.6	11776	PASS

m/z	Abundance
39.90	222.0
43.90	487.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	1750.0
36.90	9821.0
37.90	9025.0
39.00	4125.0
39.90	354.0
44.00	1657.0
45.00	1760.0
45.90	245.0
46.90	2770.0
47.80	1581.0
49.00	9354.0
50.00	44656.0
50.90	13372.0
51.90	618.0
52.90	220.0
54.90	620.0
55.90	3867.0
57.00	5870.0
58.00	260.0
59.90	1860.0
61.00	12054.0
61.90	11448.0
63.00	9219.0
63.90	1221.0
65.00	1516.0
65.90	118.0
67.00	767.0
67.90	24664.0
69.00	25560.0
70.00	1719.0
71.90	1336.0
73.00	10269.0
74.00	42072.0
75.00	128776.0
76.00	10461.0
77.00	1704.0
77.90	890.0
78.80	8267.0
79.90	2483.0
80.90	8673.0
81.80	1814.0
82.80	187.0
85.80	393.0
86.90	9528.0
88.00	9138.0
90.80	1318.0
91.90	6237.0
92.90	10283.0
93.90	28416.0
95.00	247232.0
96.00	16225.0
97.00	561.0
103.80	1102.0
104.80	457.0
105.90	1178.0
106.70	275.0
109.70	205.0
110.70	288.0
111.80	147.0
112.70	189.0
112.90	189.0
114.80	262.0
115.90	1223.0
116.80	1861.0
117.80	968.0
118.90	1361.0
123.60	133.0
125.80	116.0
127.80	845.0
128.80	345.0
129.90	858.0
130.80	292.0
134.90	320.0
136.80	439.0
139.80	257.0
140.90	2452.0
142.00	273.0
142.80	3230.0
143.80	147.0
144.90	766.0
145.70	420.0
146.80	167.0
147.80	588.0
148.90	256.0
149.70	382.0
151.70	105.0
153.00	184.0
154.90	570.0
156.70	268.0
158.90	297.0
160.90	179.0
171.00	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

171.90	1635.0
172.90	2118.0
173.90	178752.0
174.90	13194.0
175.90	171264.0
176.90	11891.0
177.80	340.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	1787.0
36.90	9906.0
37.90	8925.0
39.00	4338.0
39.90	330.0
42.70	122.0
43.90	1528.0
45.00	1811.0
45.80	239.0
46.90	2847.0
47.80	1631.0
48.90	9322.0
50.00	46064.0
50.90	14002.0
51.90	602.0
52.80	207.0
54.90	558.0
56.00	4078.0
56.90	6479.0
57.90	223.0
59.90	2064.0
60.90	12064.0
61.90	11662.0
63.00	9220.0
63.90	1070.0
64.90	1507.0
65.80	123.0
67.00	741.0
67.90	25440.0
68.90	26984.0
70.00	1967.0
71.90	1496.0
72.90	10991.0
74.00	43624.0
75.00	134784.0
76.00	11135.0
77.00	1682.0
78.00	932.0
78.80	8692.0
79.90	2663.0
80.90	9026.0
81.80	1952.0
82.80	281.0
85.70	355.0
86.90	9525.0
87.90	9692.0
90.80	1329.0
92.00	6739.0
92.90	10845.0
93.90	30184.0
95.00	257984.0
96.00	16400.0
97.00	473.0
103.90	1104.0
104.80	458.0
105.90	1272.0
106.80	206.0
107.00	208.0
109.70	250.0
110.70	275.0
111.80	209.0
112.70	216.0
114.80	328.0
115.80	1236.0
116.80	2005.0
117.80	1086.0
118.90	1394.0
123.70	139.0
127.80	871.0
128.80	449.0
129.90	865.0
130.90	303.0
134.90	405.0
136.80	400.0
139.80	214.0
140.90	2725.0
142.00	352.0
142.80	3453.0
143.80	174.0
144.80	711.0
145.70	401.0
146.80	145.0
147.80	613.0
148.90	242.0
149.70	315.0
151.80	157.0
153.00	247.0
154.80	538.0
156.80	294.0
158.90	272.0
160.90	208.0
171.00	213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

171.90	1747.0
172.90	2199.0
173.90	192064.0
174.90	14087.0
175.90	183680.0
176.90	12072.0
177.80	345.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	1760.0
36.90	9320.0
37.90	8199.0
39.00	3937.0
39.90	288.0
42.70	113.0
43.90	1459.0
44.90	1745.0
45.70	197.0
46.90	2650.0
47.80	1493.0
48.90	8480.0
50.00	43056.0
50.90	13585.0
51.90	535.0
52.80	194.0
54.90	442.0
56.00	3660.0
56.90	6556.0
57.90	183.0
59.90	2207.0
60.90	10989.0
61.90	10846.0
63.00	8432.0
63.90	950.0
64.90	1366.0
65.90	103.0
67.00	631.0
67.90	23736.0
68.90	25704.0
70.00	1986.0
71.90	1511.0
72.90	10545.0
74.00	41696.0
74.90	127416.0
76.00	11088.0
77.00	1411.0
77.90	801.0
78.80	8277.0
79.90	2608.0
80.90	8440.0
81.80	1963.0
82.80	273.0
85.70	257.0
86.90	9136.0
87.90	9431.0
90.80	1205.0
92.00	6753.0
92.90	10745.0
93.90	29048.0
95.00	245120.0
96.00	15285.0
96.90	373.0
103.80	1093.0
104.80	358.0
105.80	1240.0
107.00	188.0
109.70	272.0
110.80	213.0
111.80	228.0
112.80	213.0
114.70	377.0
115.80	1078.0
116.80	1768.0
117.80	1048.0
118.80	1363.0
123.80	179.0
126.80	114.0
127.80	761.0
128.80	557.0
129.80	760.0
130.80	332.0
134.80	441.0
136.90	375.0
139.70	160.0
140.90	2954.0
141.90	352.0
142.80	3274.0
143.80	130.0
144.80	549.0
145.70	328.0
146.80	116.0
147.80	634.0
148.90	163.0
149.70	233.0
151.80	171.0
153.00	241.0
154.70	519.0
156.90	394.0
158.80	247.0
160.90	234.0
171.00	227.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

171.90	1789.0
172.90	1952.0
173.90	186624.0
174.90	13596.0
175.90	179520.0
176.90	11366.0
177.80	323.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026