

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102418\
 Data File : VU027793.D
 Acq On : 24 Oct 2018 18:36
 Operator : MD/SY
 Sample : J5599-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H1A01

Quant Time: Oct 26 11:31:07 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102418WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Oct 25 07:21:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	39008	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	37679	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	18907	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	13720	4.31	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.20%
7) Chloroethane-d5	1.68	69	10706	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.00%
11) 1,1-Dichloroethene-d2	2.28	63	20246	3.33	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.60%
20) 2-Butanone-d5	4.20	46	48375	50.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.08%
24) Chloroform-d	4.65	84	25312	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	5.31	65	16327	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.34	84	48454	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
36) 1,2-Dichloropropane-d6	6.33	67	17416	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	7.57	98	43834	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.60%
43) trans-1,3-Dichloropropene-	7.85	79	6924	4.78	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.60%
46) 2-Hexanone-d5	8.31	63	40748	51.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.10%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	13323	4.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	17391	4.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.60%


Target Compounds					Qvalue
13) Acetone	2.31	43	8248	11.834 ug/L	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102418\
Data File : VU027793.D
Acq On : 24 Oct 2018 18:36
Operator : MD/SY
Sample : J5599-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H1A01

Quant Time: Oct 26 11:31:07 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102418WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Oct 25 07:21:42 2018
Response via : Initial Calibration

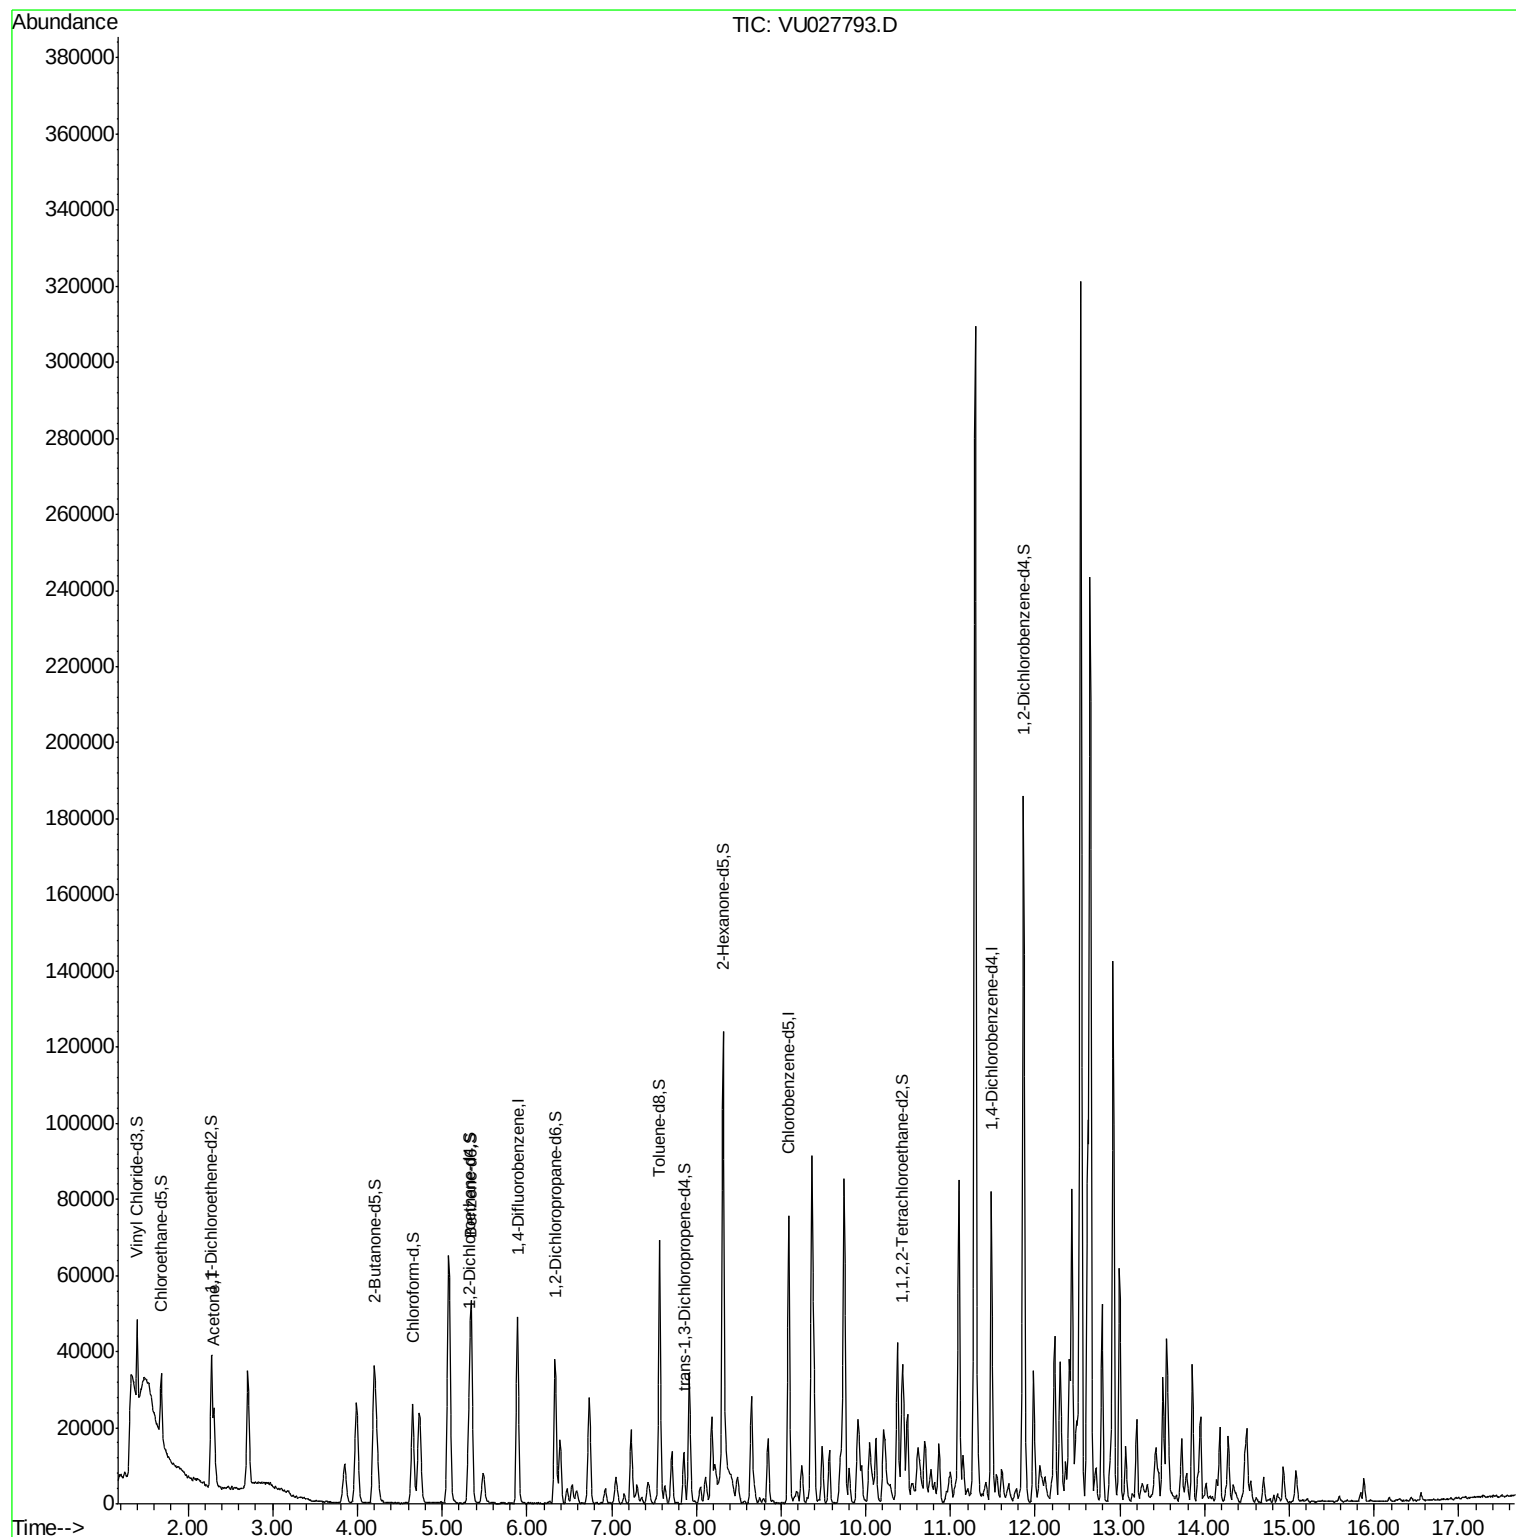

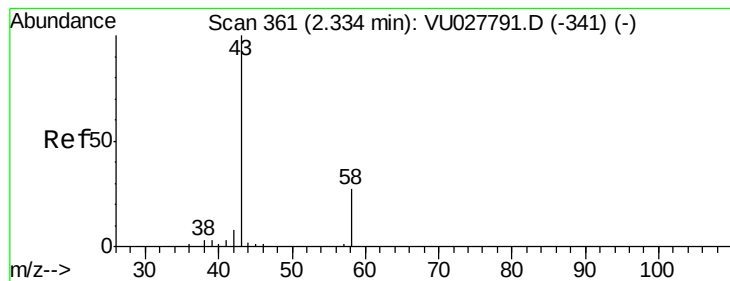

#13

Acetone

Concen: 11.834 ug/L

RT: 2.31 min Scan# 353

Delta R.T. -0.03 min

Lab File: VU027793.D

Acq: 24 Oct 2018 18:36

Instrument :
MSVOA_U
ClientSampleId :
H1A01

Tgt Ion: 43 Resp: 8248

Ion Ratio Lower Upper

43 100

58 6.3 0.0 52.8

