


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU102418\
Data File : VU027769.D
Acq On : 24 Oct 2018 07:35
Operator : MD/SY
Sample : BFB47
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB47

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102418WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Oct 29 08:53:28 2018

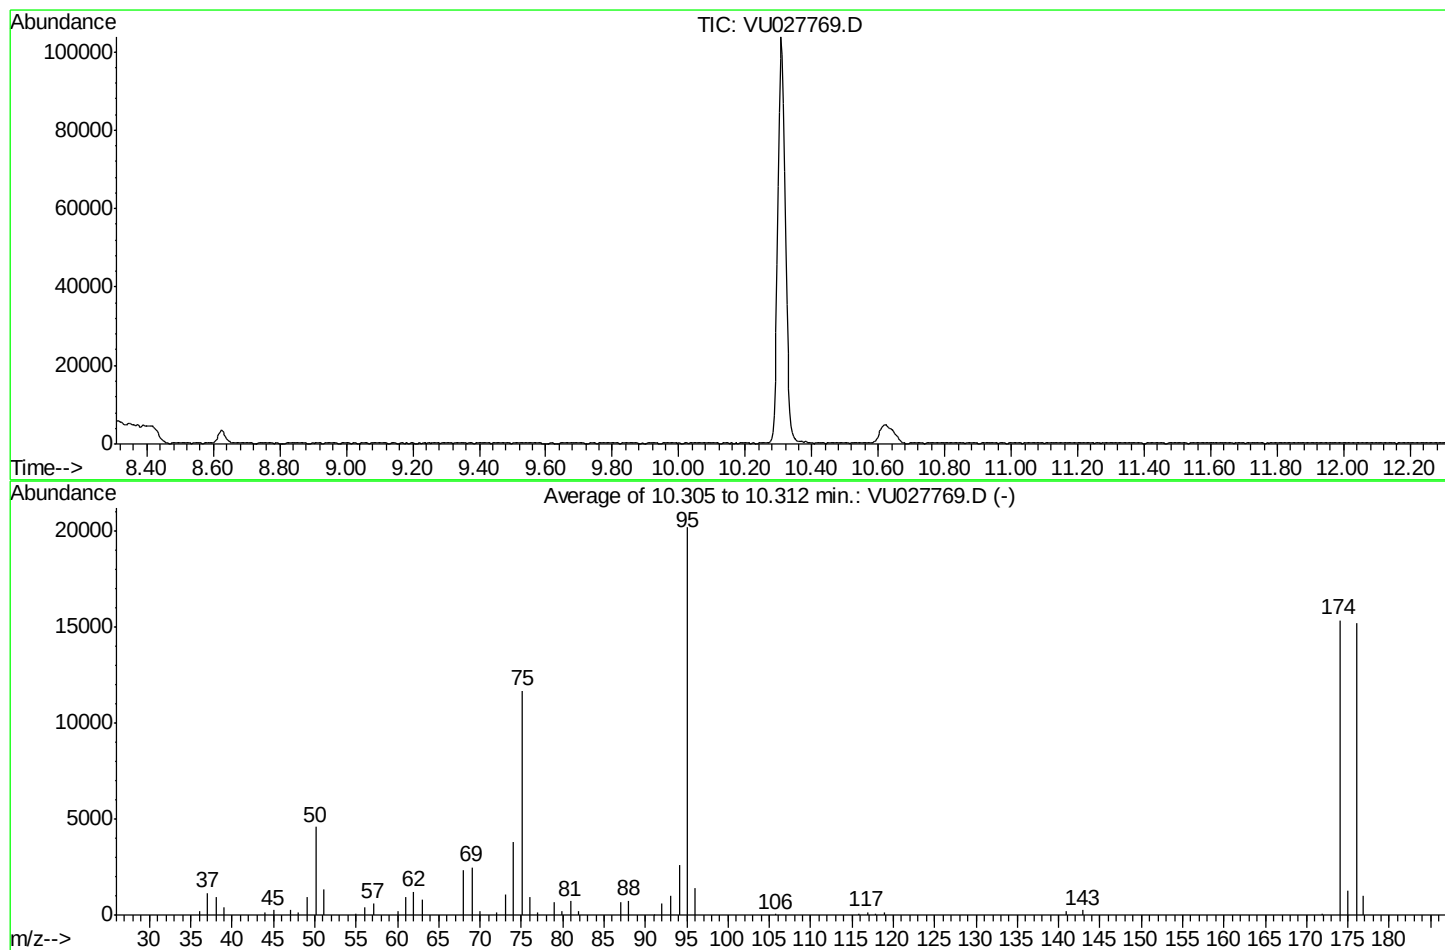

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	4577	PASS
75	95	30	80	57.8	11657	PASS
95	95	100	100	100.0	20168	PASS
96	95	5	9	7.1	1424	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.0	15321	PASS
175	174	5	9	8.4	1282	PASS
176	174	95	101	99.3	15208	PASS
177	176	5	9	6.4	971	PASS

m/z	Abundance
44.00	203.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	201.0
37.00	1175.0
38.00	895.0
39.00	472.0
44.00	386.0
45.00	288.0
47.00	289.0
48.00	116.0
49.00	899.0
50.10	4643.0
51.00	1377.0
56.00	381.0
57.00	597.0
60.00	201.0
61.00	994.0
62.00	1187.0
63.00	803.0
68.00	2283.0
69.00	2481.0
70.00	163.0
72.00	132.0
73.00	1078.0
74.10	3803.0
75.10	11451.0
76.00	865.0
76.80	103.0
78.90	705.0
79.90	220.0
80.90	748.0
81.90	195.0
87.00	652.0
88.00	779.0
92.00	582.0
93.00	973.0
94.10	2479.0
95.10	19544.0
96.00	1450.0
115.80	105.0
116.90	151.0
118.90	156.0
140.80	227.0
143.00	247.0
171.90	133.0
174.00	14922.0
175.00	1149.0
176.00	14579.0
176.90	959.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	202.0
37.00	1187.0
38.00	966.0
39.00	445.0
44.00	382.0
45.00	268.0
47.00	265.0
47.90	128.0
49.00	1009.0
50.10	4767.0
51.10	1411.0
55.00	104.0
56.00	403.0
57.00	605.0
60.00	205.0
61.10	962.0
62.00	1271.0
63.00	798.0
68.00	2422.0
69.00	2589.0
70.00	172.0
72.00	166.0
73.00	1089.0
74.10	3972.0
75.10	11999.0
76.00	913.0
76.90	109.0
78.90	705.0
79.90	232.0
80.90	733.0
81.90	182.0
87.00	707.0
88.00	809.0
91.00	100.0
92.00	601.0
93.00	985.0
94.10	2653.0
95.10	20744.0
96.00	1490.0
105.80	112.0
115.80	113.0
116.90	173.0
117.90	100.0
118.90	147.0
140.90	233.0
142.90	257.0
172.00	123.0
174.00	15679.0
175.00	1326.0
176.00	15699.0
176.90	1046.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	182.0
37.00	1061.0
38.00	957.0
39.00	353.0
44.00	333.0
45.00	203.0
47.00	261.0
47.90	116.0
49.00	979.0
50.10	4321.0
51.10	1300.0
55.00	116.0
56.00	393.0
57.10	572.0
60.00	192.0
61.10	918.0
62.00	1192.0
63.10	753.0
68.00	2287.0
69.10	2376.0
70.00	178.0
72.00	152.0
73.00	1059.0
74.00	3713.0
75.10	11521.0
76.00	999.0
77.00	114.0
78.90	637.0
79.90	218.0
81.00	666.0
81.90	153.0
87.00	698.0
88.00	711.0
92.00	597.0
93.00	955.0
94.10	2595.0
95.10	20216.0
96.00	1334.0
116.90	167.0
117.90	106.0
118.90	139.0
140.90	231.0
142.90	262.0
174.00	15362.0
175.00	1371.0
176.00	15348.0
176.90	908.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47